


Data Path : Z:\HPCHEM1\BNA M\Data\BM092915\
 Data File : BM002754.D
 Acq On : 29 Sep 2015 20:11
 Operator : UM/IZ
 Sample : DFTPP18
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP18

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092915.M
 Title : SVOA CALIBRATION
 Last Update : Wed Sep 30 06:48:30 2015

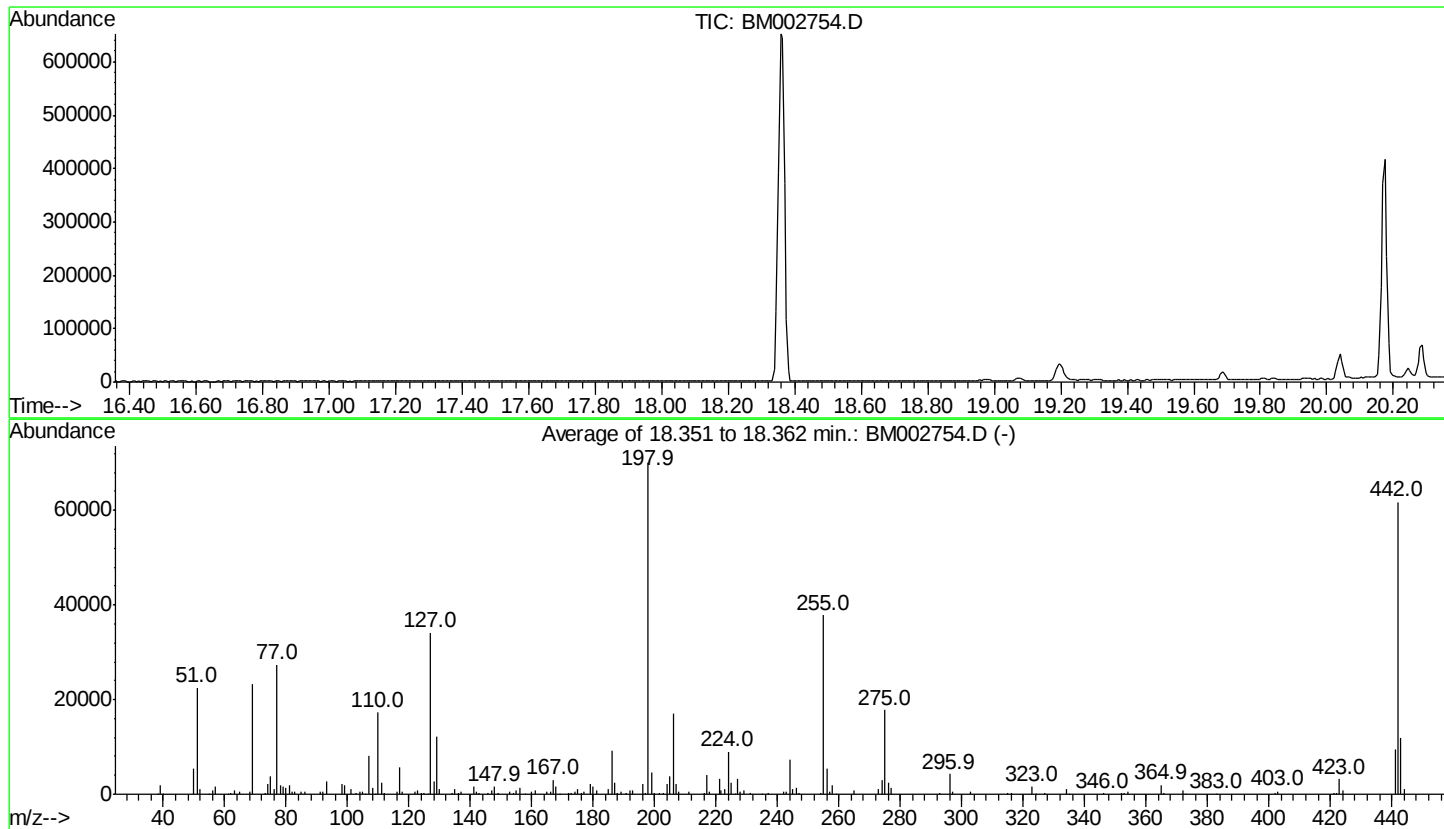

AutoFind: Scans 2595, 2596, 2597; Background Corrected with Scan 2590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	22453	PASS
68	69	0.00	2	1.9	435	PASS
69	198	0.00	100	33.3	23362	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	34208	PASS
197	198	0.00	2	0.5	337	PASS
198	198	100	100	100.0	70074	PASS
199	198	5	9	6.6	4613	PASS
275	198	10	60	25.5	17840	PASS
365	198	1	100	2.8	1929	PASS
441	443	0.01	100	78.8	9415	PASS
442	198	50	100	88.2	61794	PASS
443	442	15	24	19.3	11946	PASS

Scan 2590 (18.321 min): BM002754.D
DFTPP18

m/z	Abundance
39.90	346.0
44.00	1701.0
207.00	390.0

Instrument :
BNA_M
ClientSampleId :
DFTPP18

m/z	Abundance
39.00	1555.0
39.90	378.0
44.00	1721.0
50.00	4545.0
51.00	18656.0
52.00	990.0
55.90	593.0
57.00	1444.0
62.00	306.0
63.00	692.0
65.00	432.0
68.10	348.0
69.00	19232.0
73.00	365.0
74.00	1775.0
75.00	3105.0
76.00	968.0
77.00	22232.0
78.00	1642.0
79.00	1466.0
80.00	1037.0
81.00	1487.0
81.90	312.0
82.90	436.0
85.00	321.0
86.00	449.0
91.00	404.0
91.90	489.0
93.00	2171.0
98.00	1715.0
99.00	1633.0
101.00	864.0
103.90	538.0
104.90	573.0
107.00	6243.0
108.00	1000.0
110.00	13584.0
111.00	1943.0
116.00	348.0
117.00	4353.0
117.90	412.0
122.00	420.0
122.90	710.0
124.00	330.0
124.90	332.0
127.00	26352.0
128.00	1911.0
129.00	9304.0
130.00	796.0
134.90	760.0
137.00	413.0
141.00	1224.0
141.90	340.0
147.00	570.0
148.00	1204.0
152.90	391.0
153.90	307.0
155.00	644.0
156.00	1071.0
159.90	348.0
161.00	577.0
164.90	479.0
166.00	330.0
167.00	2162.0
168.00	1219.0
173.90	467.0
175.00	944.0
176.90	440.0
178.90	1681.0
180.00	1267.0
181.00	609.0
184.90	751.0
186.00	6388.0
187.00	1643.0
189.00	431.0
191.90	505.0
193.00	602.0
196.00	1680.0
197.90	49928.0
198.90	3522.0
204.00	1583.0
205.00	2713.0
206.00	12224.0
207.00	1828.0
207.90	645.0
210.90	461.0
216.90	2743.0
218.00	372.0
221.00	2423.0
221.80	552.0
223.00	749.0

Instrument :
BNA_M
ClientSampleId :
DFTPP18

224.00	6309.0
225.00	1679.0
227.00	2286.0
227.90	367.0
228.90	463.0
242.00	350.0
243.00	340.0
244.00	5007.0
245.00	720.0
245.90	862.0
255.00	25392.0
256.00	3609.0
256.90	332.0
258.00	1143.0
264.90	479.0
272.90	698.0
274.00	1849.0
275.00	11624.0
276.00	1627.0
277.00	956.0
295.90	2660.0
296.90	311.0
303.00	316.0
323.00	1013.0
334.00	530.0
354.10	329.0
365.00	1118.0
372.00	465.0
403.00	348.0
423.00	1838.0
424.00	397.0
441.00	4954.0
442.00	32824.0
443.00	6988.0
443.90	605.0

Instrument :
BNA_M
ClientSampleId :
DFTPP18

m/z	Abundance
38.00	400.0
39.00	2229.0
40.00	393.0
44.00	1571.0
50.00	6447.0
51.00	26224.0
52.00	1373.0
56.00	812.0
57.00	1894.0
61.00	398.0
61.90	342.0
63.00	1009.0
65.10	556.0
68.00	521.0
69.00	27576.0
73.00	394.0
74.00	2615.0
75.00	4320.0
76.00	1447.0
77.00	31664.0
78.00	2393.0
79.00	2007.0
80.00	1533.0
81.00	2219.0
81.90	601.0
83.00	628.0
85.00	499.0
85.90	584.0
90.90	554.0
91.90	591.0
93.00	3308.0
98.00	2763.0
99.00	2083.0
101.00	1472.0
102.90	487.0
104.00	764.0
104.90	752.0
105.90	352.0
107.00	9677.0
108.00	1796.0
109.00	399.0
110.00	20264.0
111.00	2855.0
112.00	392.0
115.90	585.0
117.00	6724.0
118.00	492.0
121.90	627.0
122.90	900.0
123.90	468.0
125.00	399.0
126.20	333.0
127.00	39480.0
128.00	2956.0
129.00	14133.0
130.00	1260.0
133.90	396.0
135.00	1218.0
136.00	514.0
137.00	612.0
141.00	1634.0
141.90	613.0
142.90	428.0
145.90	316.0
146.90	945.0
147.90	1883.0
149.00	402.0
152.90	611.0
154.00	467.0
155.00	994.0
156.00	1504.0
157.90	323.0
160.00	557.0
161.00	825.0
165.00	576.0
165.90	547.0
167.00	3431.0
168.00	1835.0
172.00	320.0
172.90	482.0
174.00	825.0
175.00	1401.0
176.00	543.0
176.90	785.0
178.90	2593.0
180.00	1938.0
180.90	1010.0
185.00	1222.0
186.00	10483.0
187.00	3048.0
188.00	313.0

Instrument :
BNA_M
ClientSampleId :
DFTPP18

188.90	634.0
190.90	348.0
191.90	819.0
193.00	1048.0
196.00	2499.0
197.00	491.0
198.00	81664.0
199.00	5282.0
200.00	461.0
201.40	486.0
202.90	530.0
204.00	2733.0
205.00	4322.0
206.00	19496.0
207.00	3152.0
207.90	577.0
211.00	813.0
216.00	432.0
216.90	4486.0
218.00	682.0
221.00	3743.0
221.80	935.0
223.00	1065.0
224.00	10318.0
225.00	2738.0
226.00	313.0
227.00	3818.0
227.90	611.0
228.90	857.0
231.00	372.0
237.00	324.0
242.00	507.0
242.90	593.0
244.00	8249.0
245.00	1204.0
246.00	1425.0
246.90	311.0
254.10	315.0
255.00	43248.0
256.00	6383.0
257.00	539.0
258.00	2219.0
265.00	737.0
273.00	1118.0
274.00	3519.0
275.00	20472.0
276.00	2916.0
276.90	1512.0
293.00	323.0
296.00	4988.0
297.00	691.0
302.90	618.0
314.90	589.0
316.00	326.0
323.00	1683.0
326.90	393.0
334.00	1220.0
346.00	358.0
352.00	497.0
353.00	433.0
354.00	588.0
365.00	2203.0
365.90	301.0
372.00	921.0
402.00	345.0
403.00	632.0
421.00	443.0
421.90	487.0
423.00	3389.0
424.00	788.0
441.00	10412.0
442.00	68696.0
443.00	13097.0
444.00	1292.0

Instrument :

BNA_M

ClientSampleId :

DFTPP18

m/z	Abundance
39.00	1877.0
39.90	380.0
44.00	1552.0
50.00	5500.0
51.00	22480.0
52.00	1186.0
55.00	314.0
56.00	744.0
57.00	1572.0
61.90	320.0
63.00	888.0
65.00	502.0
68.00	436.0
69.00	23280.0
73.00	342.0
74.00	2243.0
75.00	3611.0
76.00	1253.0
77.10	28224.0
78.10	1958.0
79.00	1714.0
79.90	1310.0
81.00	1937.0
82.00	547.0
82.90	522.0
85.00	430.0
86.00	523.0
91.00	440.0
92.00	539.0
93.00	2841.0
98.00	2130.0
99.00	1727.0
101.00	1181.0
102.90	407.0
104.00	711.0
104.90	649.0
107.00	8328.0
108.00	1468.0
110.00	17912.0
111.00	2595.0
111.90	305.0
115.90	558.0
117.00	6182.0
117.90	407.0
121.90	586.0
123.00	888.0
124.00	415.0
125.00	400.0
127.00	36792.0
128.00	2921.0
129.00	12958.0
130.00	1127.0
133.90	371.0
135.00	1088.0
136.00	420.0
137.00	530.0
141.00	1743.0
142.00	593.0
142.80	340.0
145.90	377.0
147.00	864.0
148.00	1644.0
148.90	426.0
152.90	507.0
153.90	454.0
155.00	992.0
156.00	1446.0
159.90	523.0
160.90	709.0
165.00	683.0
166.00	417.0
167.00	3409.0
168.00	1448.0
168.90	321.0
171.90	390.0
172.90	369.0
174.00	717.0
175.00	1308.0
176.00	411.0
176.90	658.0
179.00	2373.0
180.00	1612.0
181.00	951.0
185.00	1284.0
186.00	10687.0
186.90	2919.0
188.00	347.0
188.90	663.0
190.90	305.0
191.90	918.0
192.90	894.0

Instrument :
BNA_M
ClientSampleId :
DFTPP18

196.00	2243.0
197.00	520.0
198.00	78632.0
198.90	5035.0
200.00	367.0
201.50	356.0
202.90	478.0
204.00	2540.0
205.00	4334.0
206.00	19280.0
207.10	2888.0
207.90	536.0
210.90	734.0
216.00	387.0
217.00	4595.0
218.00	698.0
221.00	3894.0
221.70	799.0
223.00	1102.0
224.00	10208.0
225.00	2666.0
227.00	3789.0
227.90	473.0
229.00	910.0
231.00	347.0
234.90	330.0
237.00	310.0
242.00	537.0
243.10	614.0
244.00	8774.0
245.00	1049.0
246.00	1496.0
246.90	302.0
254.10	402.0
255.00	44688.0
256.00	6526.0
257.00	468.0
258.00	2093.0
259.00	407.0
264.90	945.0
273.00	1344.0
274.00	3521.0
275.00	21424.0
276.00	2804.0
277.00	1697.0
293.00	420.0
296.00	5067.0
296.90	674.0
303.00	612.0
314.90	584.0
316.00	382.0
323.00	2031.0
324.00	349.0
326.90	338.0
334.00	1261.0
334.90	300.0
346.00	363.0
352.00	450.0
353.00	407.0
354.00	665.0
364.90	2467.0
365.90	343.0
372.00	1235.0
372.90	319.0
383.00	349.0
401.90	494.0
403.00	684.0
421.00	683.0
422.00	573.0
423.00	4469.0
424.00	959.0
441.00	12879.0
442.00	83864.0
443.00	15755.0
444.00	1434.0

Instrument :

BNA_M

ClientSampleId :

DFTPP18