

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092916\
 Data File : BM007634.D
 Acq On : 29 Sep 2016 19:23
 Operator : UM/SJ
 Sample : H4955-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4VL7

Quant Time: Sep 30 01:34:46 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 30 01:33:49 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	1763	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.56	136	7120	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.40	164	5162	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.24	188	711892	0.40	ng/ul	0.09
16) Chrysene-d12	21.35	240	10478	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	475468	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.16	152	2730	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.18	212	9357	0.01	ng/ul	0.00
Target Compounds						
17) Pyrene	19.54	202	1423	0.04	ng/ul#	Qvalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092916\
Data File : BM007634.D
Acq On : 29 Sep 2016 19:23
Operator : UM/SJ
Sample : H4955-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4VL7

Quant Time: Sep 30 01:34:46 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 30 01:33:49 2016
Response via : Initial Calibration

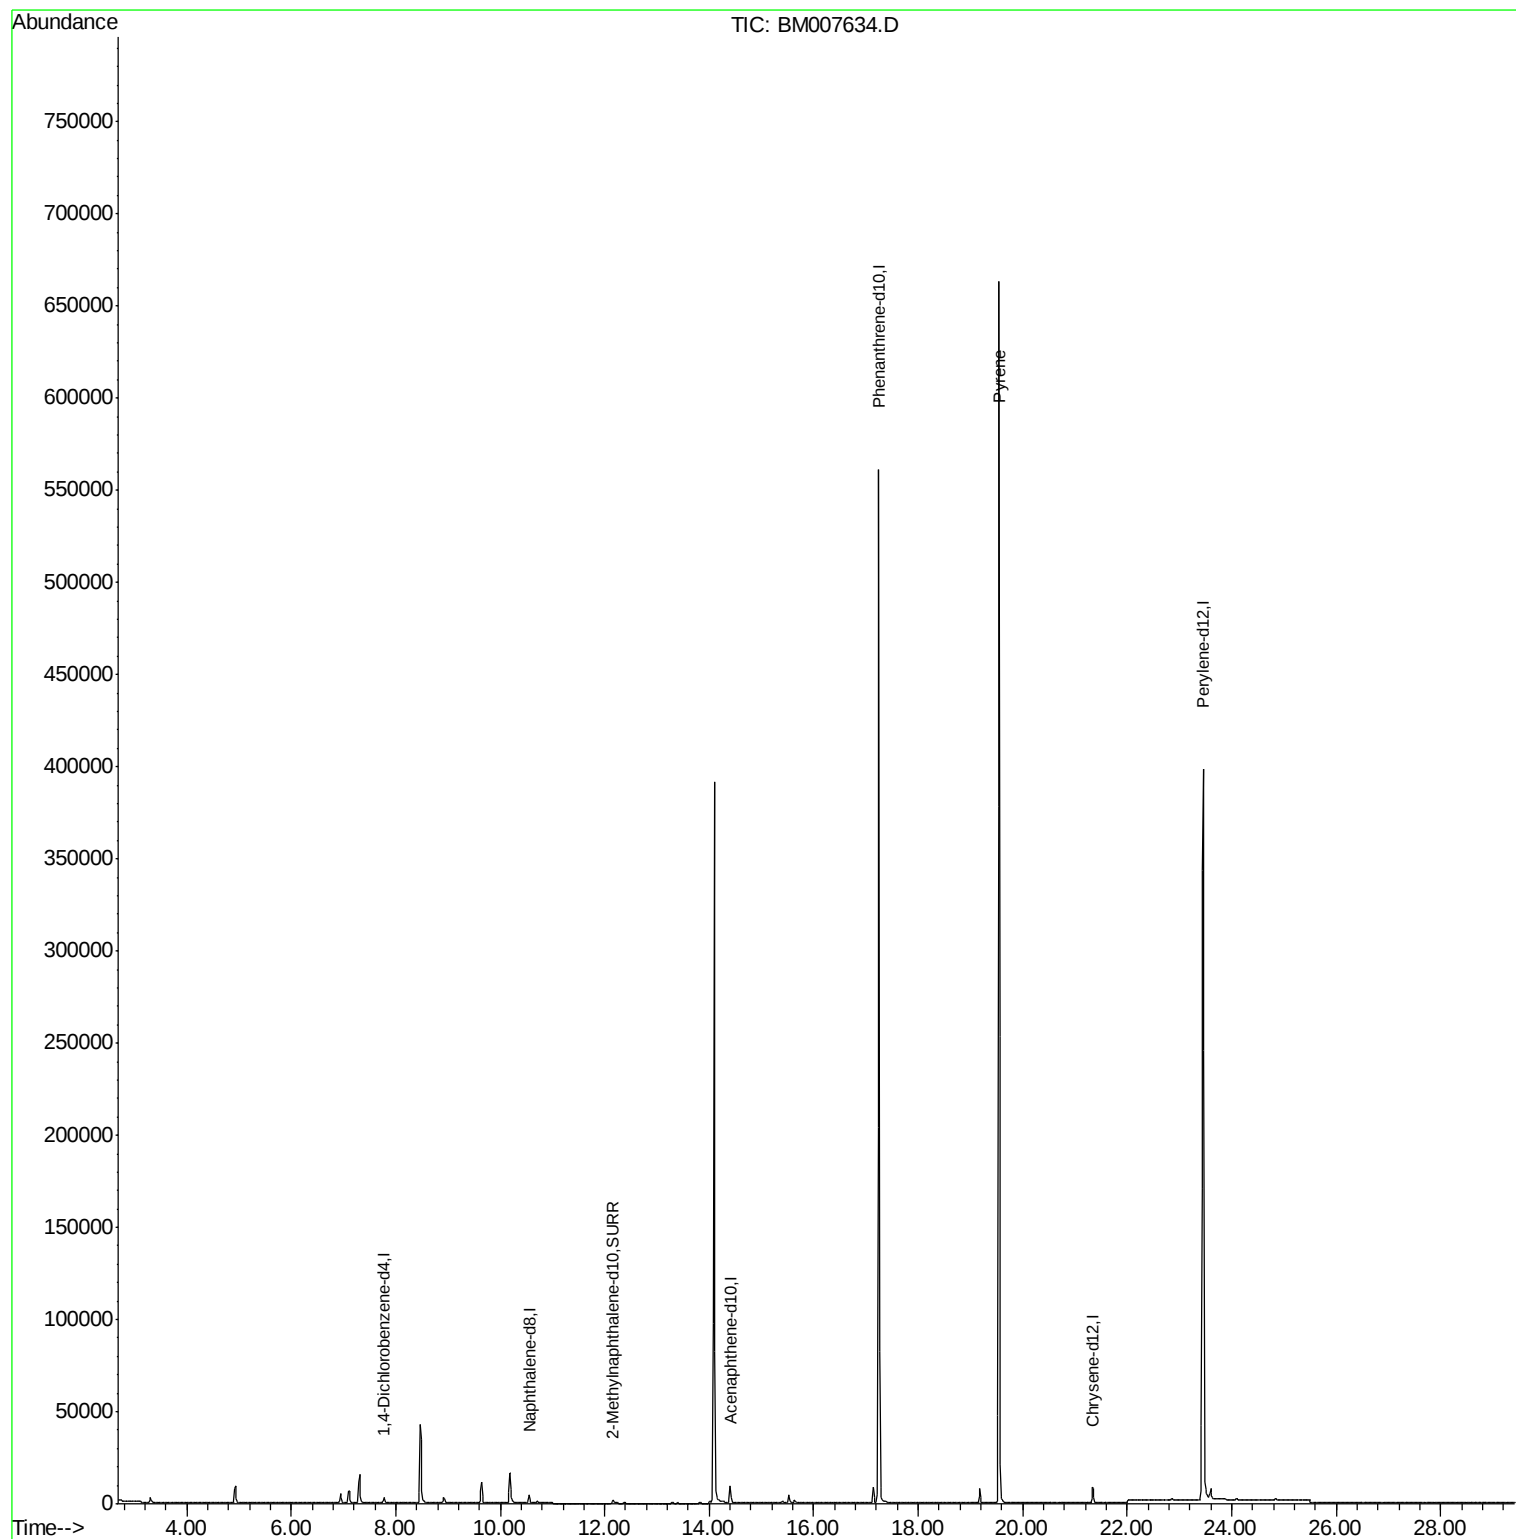

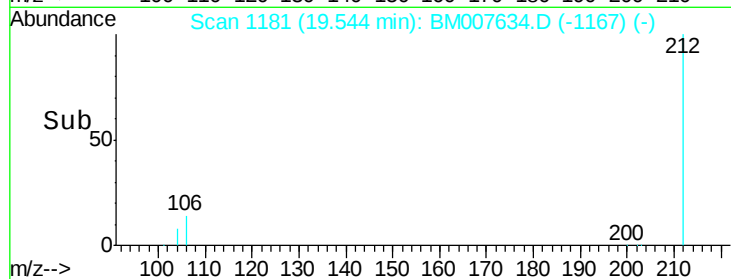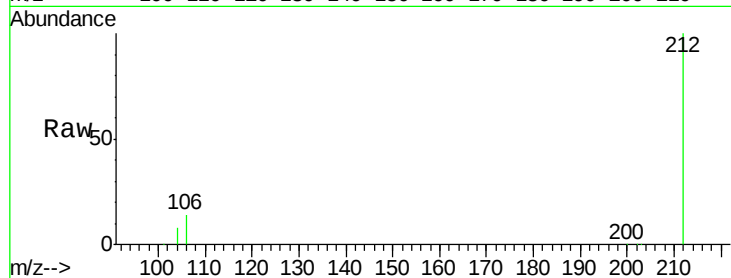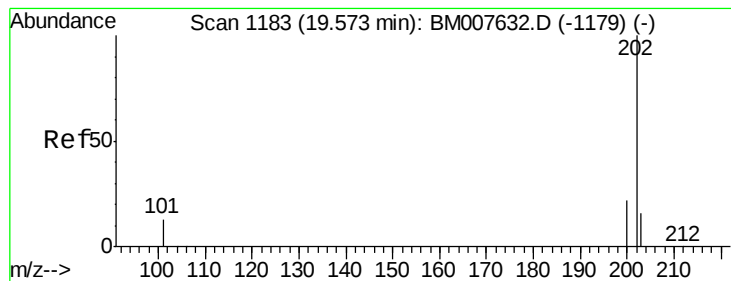

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.54 min Scan# 1181

Delta R.T. -0.03 min

Lab File: BM007634.D

Acq: 29 Sep 2016 19:23

Instrument :

BNA_M

ClientSampleId :

A4VL7

Tgt Ion: 202 Resp: 1423

Ion Ratio Lower Upper

202 100

200 8.2 15.9 23.9#

203 189.2 15.0 22.4#

