

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092916\
 Data File : BM007642.D
 Acq On : 30 Sep 2016 00:10
 Operator : UM/SJ
 Sample : H4955-17
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4VM5

Quant Time: Sep 30 01:35:29 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 30 01:33:49 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	1532	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.56	136	6363	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.40	164	4584	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.24	188	654752	0.40	ng/ul	0.09
16) Chrysene-d12	21.34	240	9700	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	528220	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.16	152	2765	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.18	212	8588	0.01	ng/ul	0.00
Target Compounds						
9) Fluorene	15.39	166	1191	0.06	ng/ul#	18
17) Pyrene	19.54	202	1395	0.04	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092916\
Data File : BM007642.D
Acq On : 30 Sep 2016 00:10
Operator : UM/SJ
Sample : H4955-17
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4VM5

Quant Time: Sep 30 01:35:29 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 30 01:33:49 2016
Response via : Initial Calibration

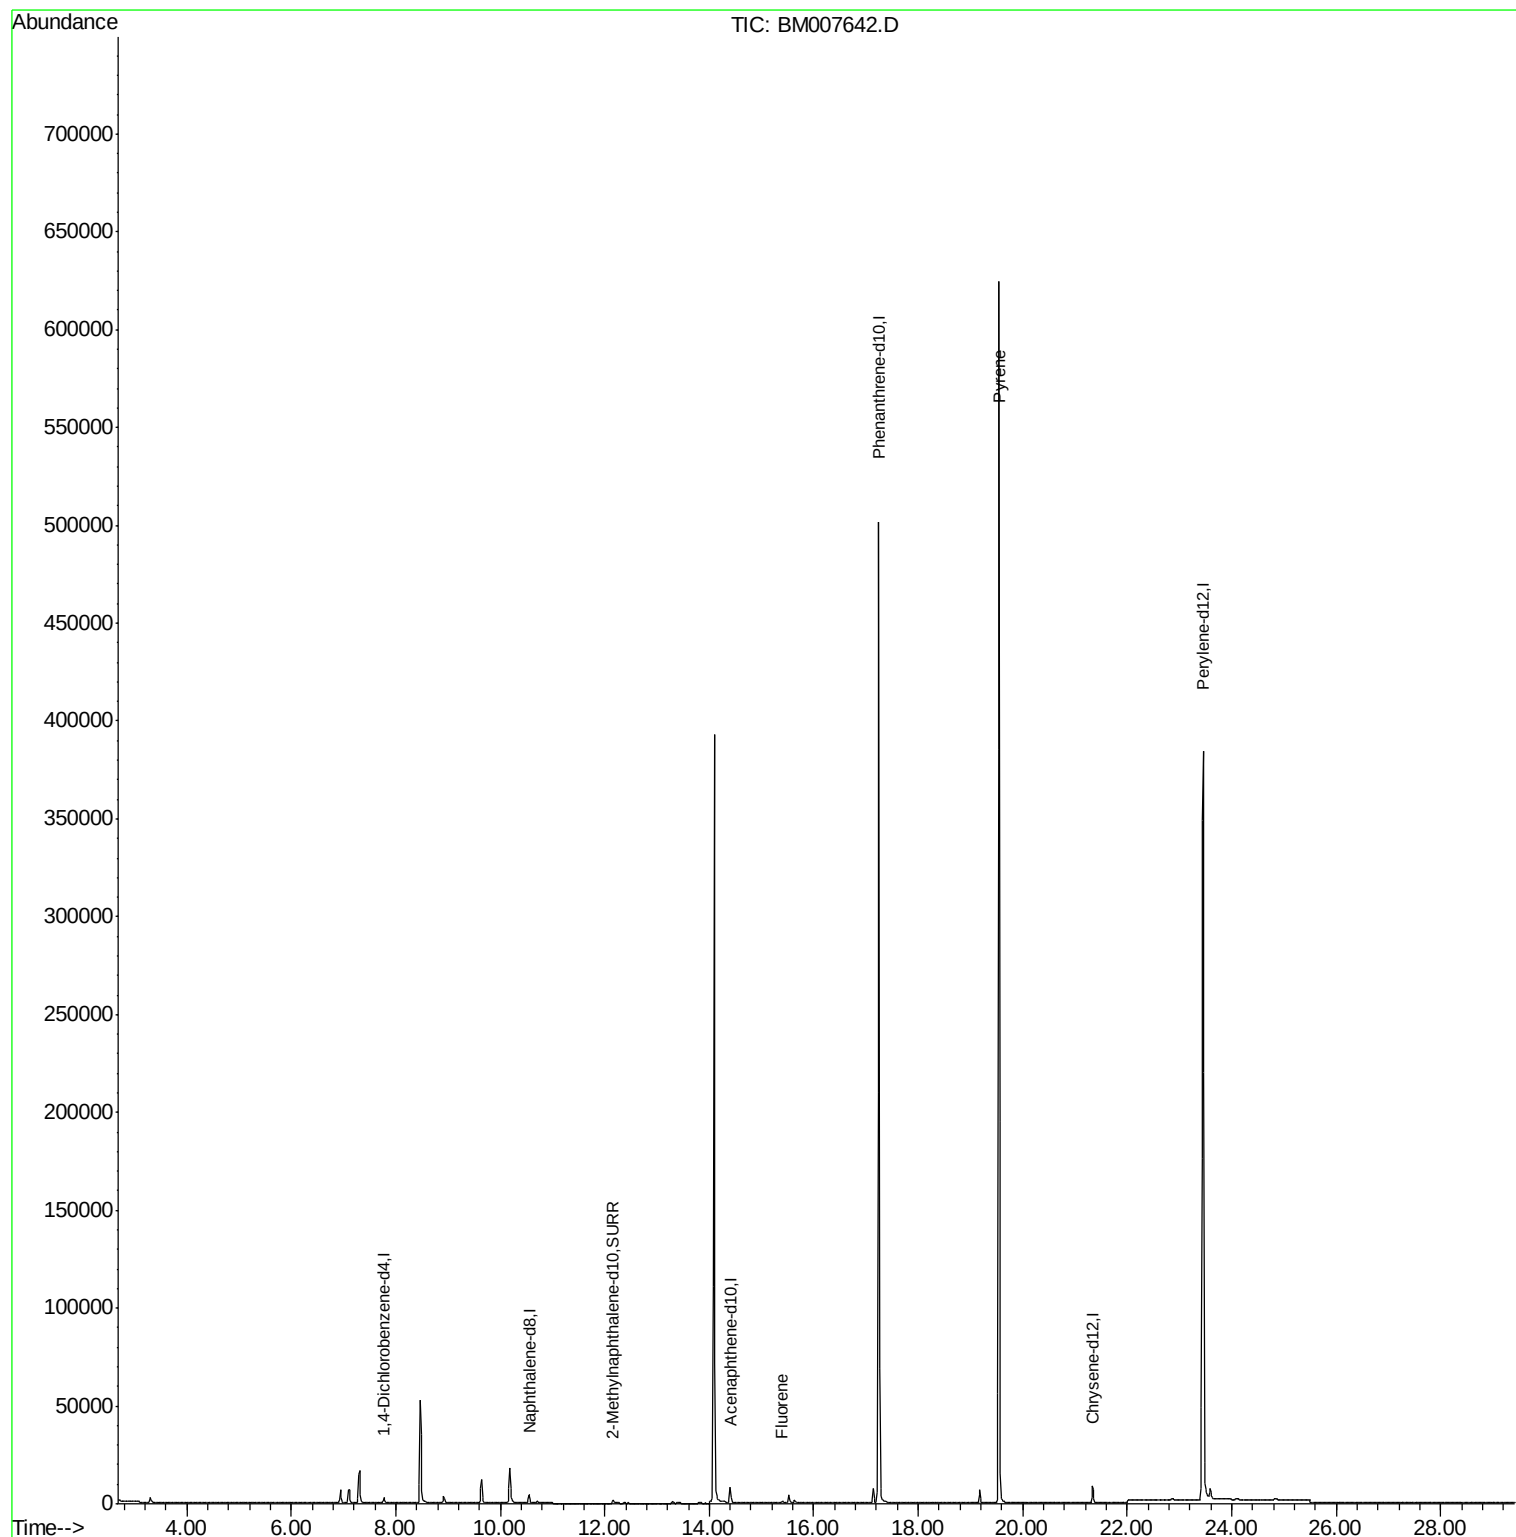

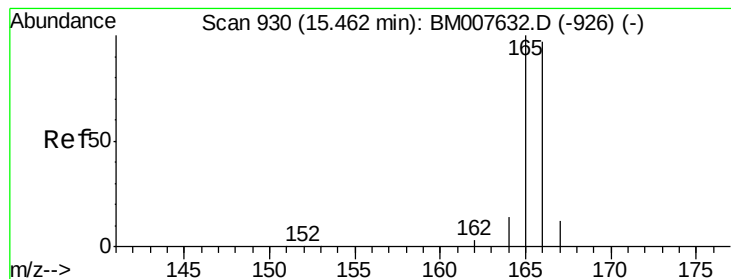

#9

Fluorene

Concen: 0.06 ng/ul

RT: 15.39 min Scan# 926

Delta R.T. -0.07 min

Lab File: BM007642.D

Acq: 30 Sep 2016 00:10

Instrument :

BNA_M

ClientSampleId :

A4VM5


Tgt Ion:166 Resp: 1191

Ion Ratio Lower Upper

166 100

165 11.4 79.8 119.8#




167 29.8 11.5 17.3#

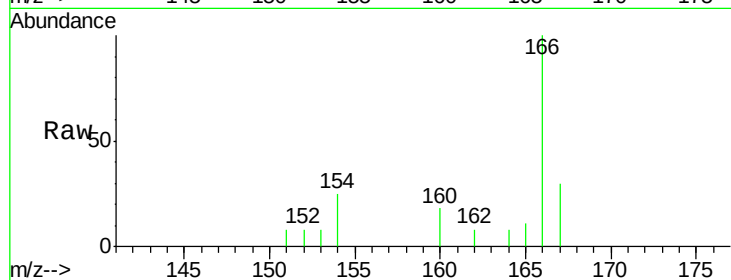

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

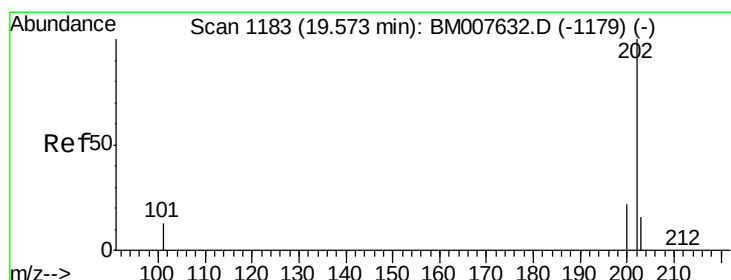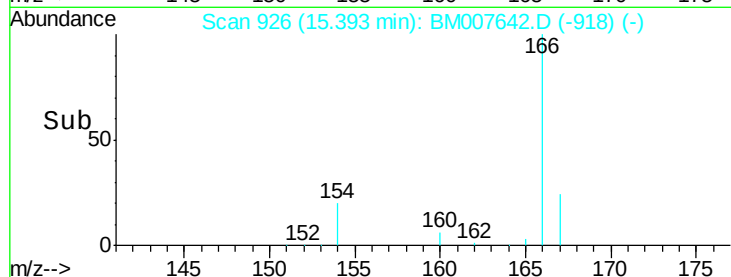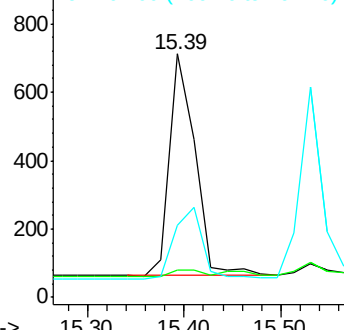

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.54 min Scan# 1181

Delta R.T. -0.03 min

Lab File: BM007642.D

Acq: 30 Sep 2016 00:10


Tgt Ion:202 Resp: 1395

Ion Ratio Lower Upper

202 100

200 8.5 15.9 23.9#

203 196.7 15.0 22.4#

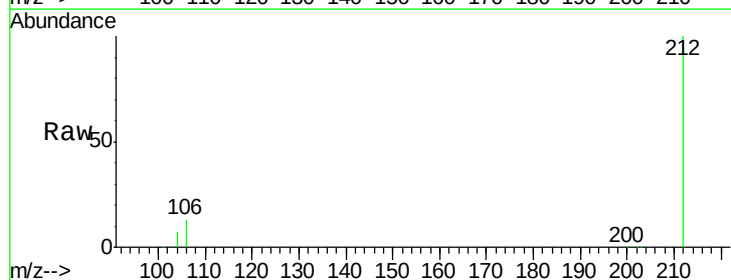

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

