

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092916\
 Data File : BM007643.D
 Acq On : 30 Sep 2016 00:46
 Operator : UM/SJ
 Sample : H4955-18
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4VM6

Quant Time: Sep 30 01:35:34 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 30 01:33:49 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	1507	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.56	136	6241	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.40	164	4587	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.24	188	730680	0.40	ng/ul	0.09
16) Chrysene-d12	21.35	240	9730	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	498733	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.16	152	2897	0.40	ng/ul	0.00
14) Fluoranthene-d10	19.18	212	9440	0.01	ng/ul	0.00
Target Compounds						
9) Fluorene	15.39	166	1289	0.07	ng/ul#	17
17) Pyrene	19.54	202	1473	0.05	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092916\
Data File : BM007643.D
Acq On : 30 Sep 2016 00:46
Operator : UM/SJ
Sample : H4955-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4VM6

Quant Time: Sep 30 01:35:34 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 30 01:33:49 2016
Response via : Initial Calibration




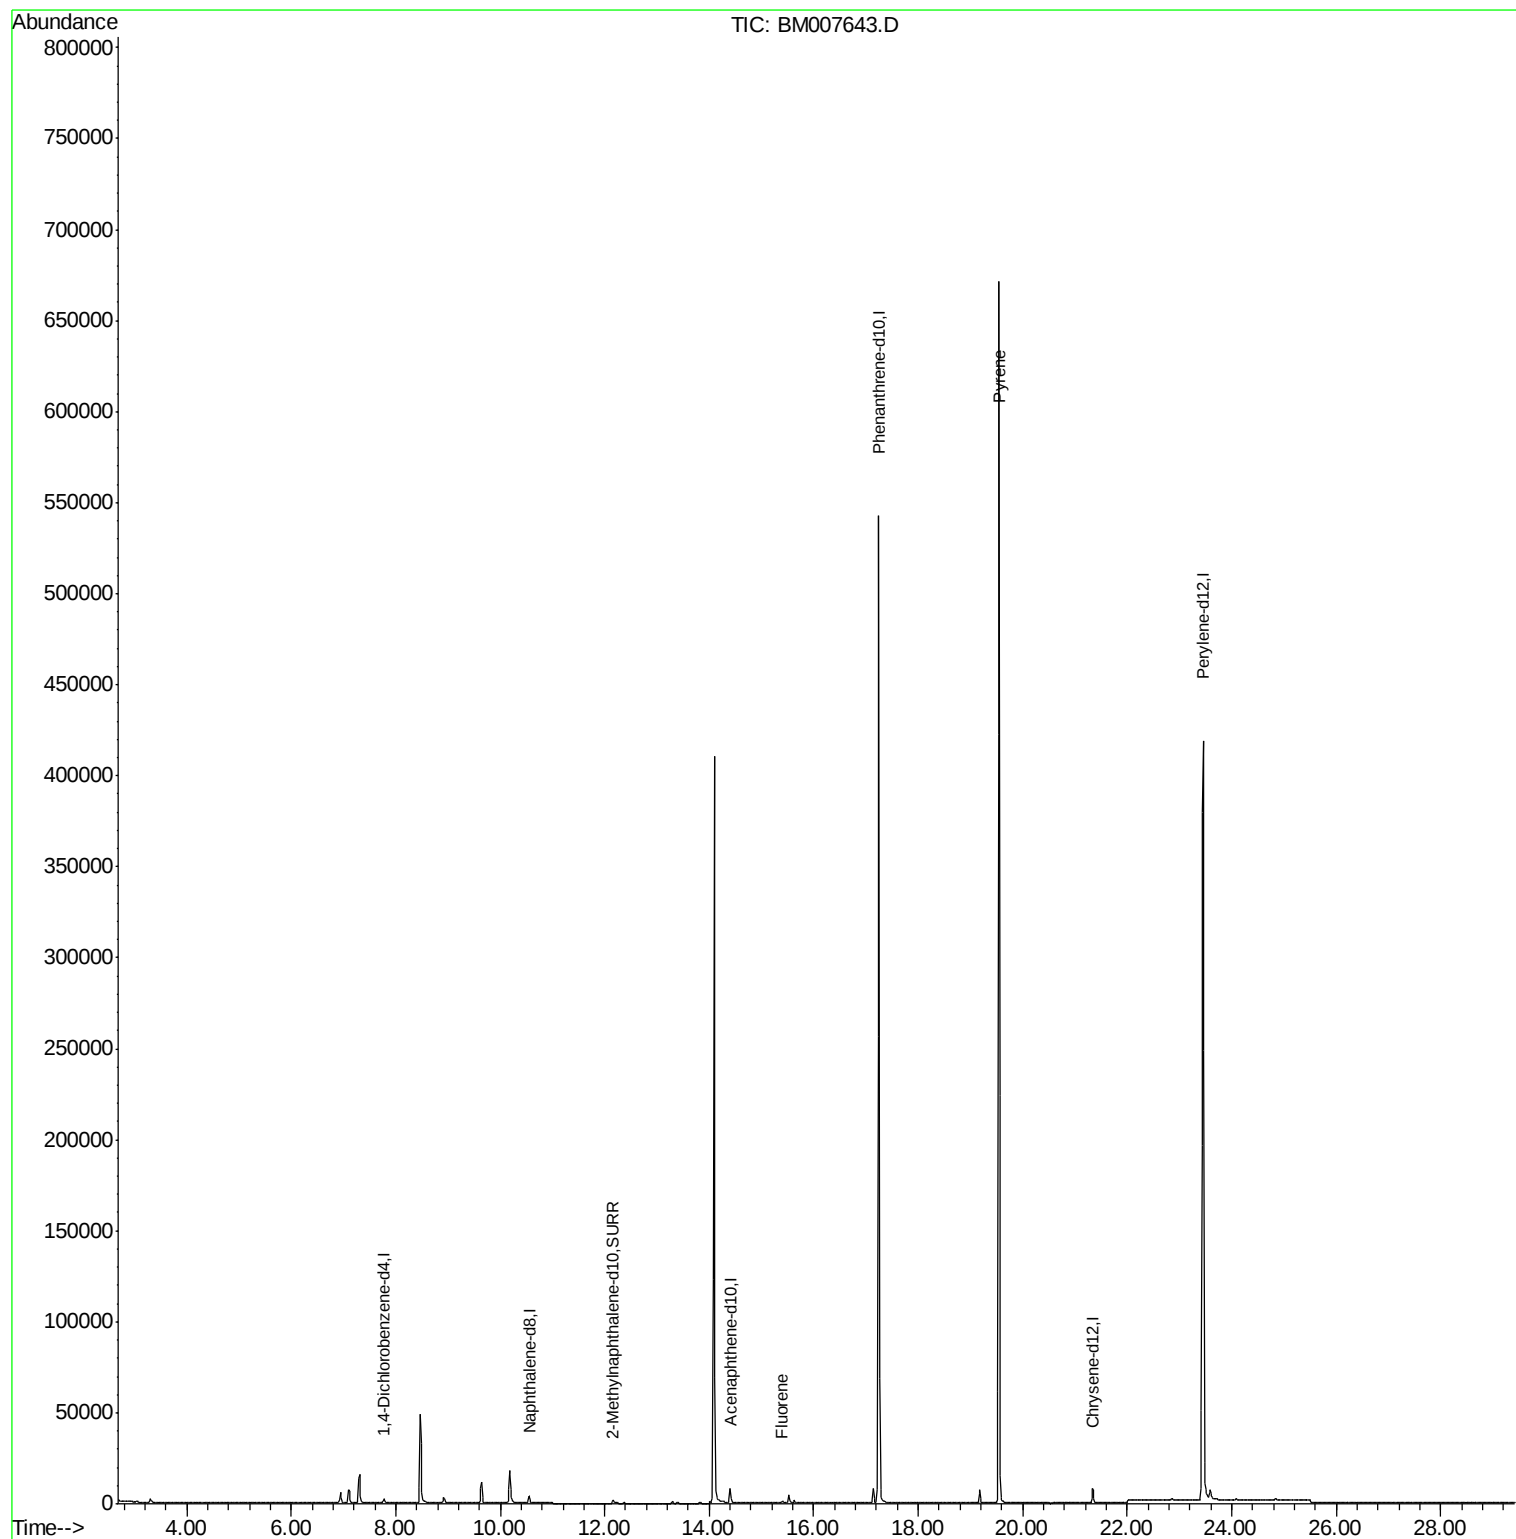


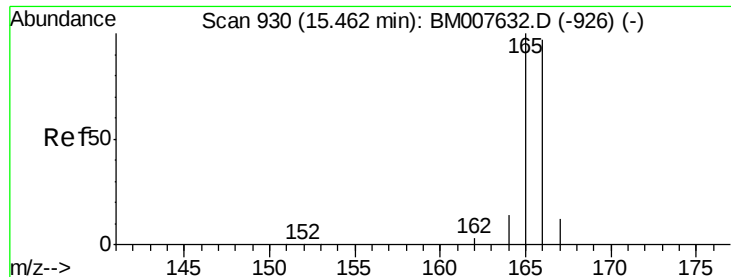

#9
Fluorene
 Concen: 0.07 ng/ul
 RT: 15.39 min Scan# 926
 Delta R.T. -0.07 min
 Lab File: BM007643.D
 Acq: 30 Sep 2016 00:46

Instrument :
 BNA_M
 ClientSampleId :
 A4VM6

Tgt Ion:166 Resp: 1289
 Ion Ratio Lower Upper
 166 100
 165 10.2 79.8 119.8#
 167 29.5 11.5 17.3#

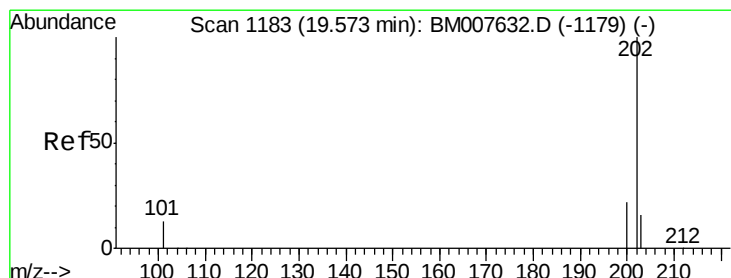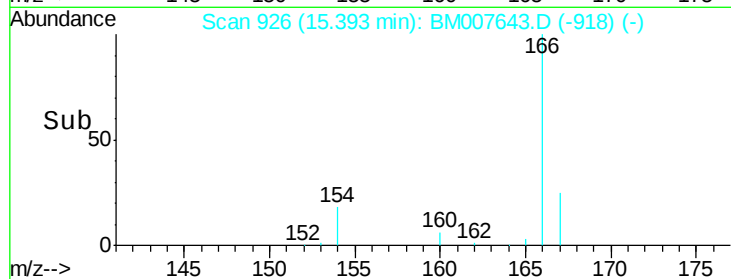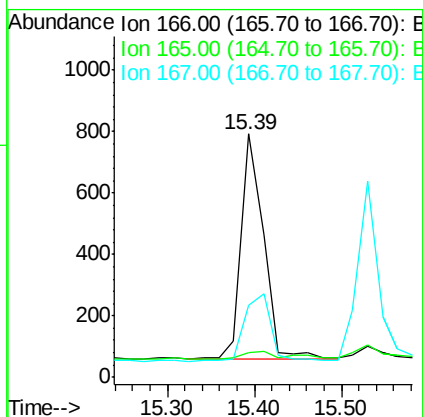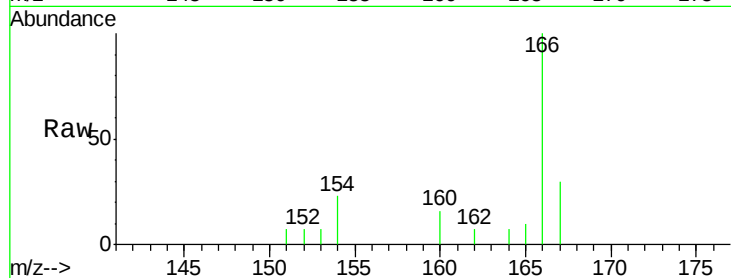

#17
Pyrene
 Concen: 0.05 ng/ul
 RT: 19.54 min Scan# 1181
 Delta R.T. -0.03 min
 Lab File: BM007643.D
 Acq: 30 Sep 2016 00:46

Tgt Ion:202 Resp: 1473
 Ion Ratio Lower Upper
 202 100
 200 8.1 15.9 23.9#
 203 193.8 15.0 22.4#

