

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092916\
 Data File : BM007645.D
 Acq On : 30 Sep 2016 01:57
 Operator : UM/SJ
 Sample : H4955-26
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4VN7

Quant Time: Sep 30 03:00:59 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 30 01:33:49 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	1597	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.56	136	6605	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.40	164	4830	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.24	188	736807	0.40	ng/ul	0.09
16) Chrysene-d12	21.34	240	10446	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	592277	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.15	152	3237	0.42	ng/ul	-0.01
14) Fluoranthene-d10	19.18	212	10019	0.01	ng/ul	0.00
Target Compounds						
17) Pyrene	19.54	202	1553	0.04	ng/ul#	Qvalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092916\
Data File : BM007645.D
Acq On : 30 Sep 2016 01:57
Operator : UM/SJ
Sample : H4955-26
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4VN7

Quant Time: Sep 30 03:00:59 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 30 01:33:49 2016
Response via : Initial Calibration

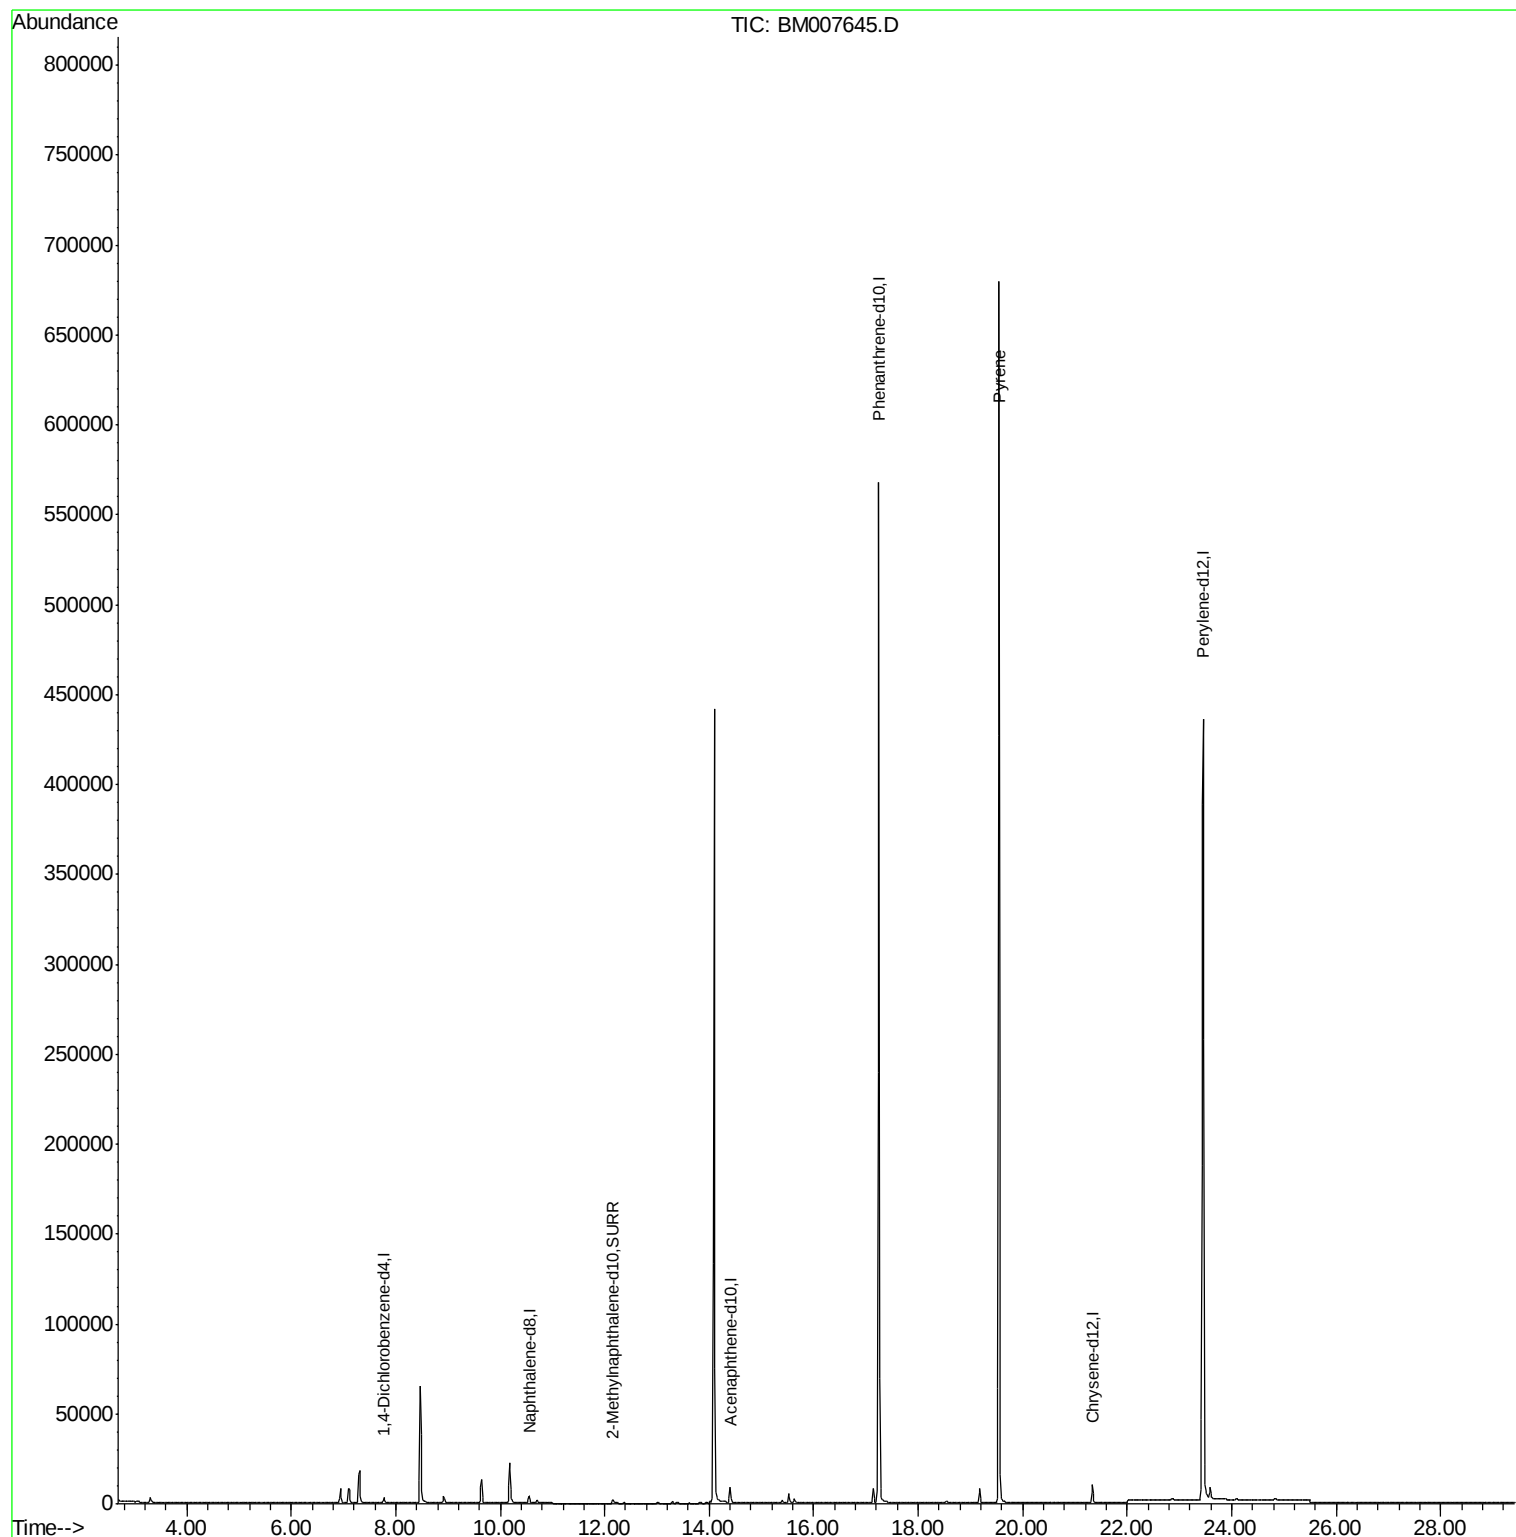

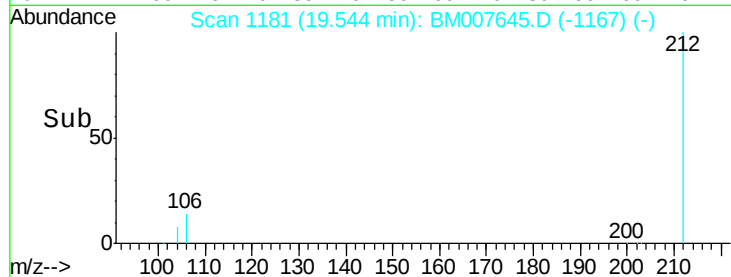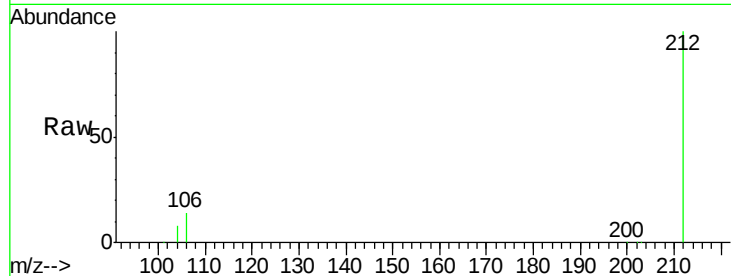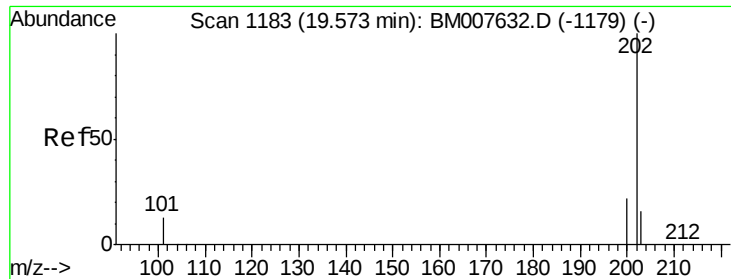

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.54 min Scan# 1181

Delta R.T. -0.03 min

Lab File: BM007645.D

Acq: 30 Sep 2016 01:57

Instrument :

BNA_M

ClientSampleId :

A4VN7

Tgt Ion: 202 Resp: 1553

Ion Ratio Lower Upper

202 100

200 9.1 15.9 23.9#

203 188.7 15.0 22.4#

