

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092917\
 Data File : BM011778.D
 Acq On : 29 Sep 2017 21:50
 Operator : SJ/JU
 Sample : I5354-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 30 01:20:32 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM092717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 30 00:51:32 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	219097	20.00	ng/ul	0.00
18) Naphthalene-d8	10.74	136	990012	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.57	164	549008	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.31	188	1188871	20.00	ng/ul	0.00
75) Chrysene-d12	21.47	240	954249	20.00	ng/ul	0.00
83) Perylene-d12	23.84	264	767946	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.36	96	29234	5.95	ng/uL	0.00
5) Phenol-d5	7.09	99	641932	29.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.26	67	499513	31.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.46	132	526297	32.83	ng/ul	0.00
13) 4-Methylphenol-d8	8.63	113	527411	31.25	ng/ul	0.00
19) Nitrobenzene-d5	9.10	128	261428	33.85	ng/ul	0.00
22) 2-Nitrophenol-d4	9.82	143	282790	34.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.35	165	504839	32.12	ng/ul	0.00
29) 4-Chloroaniline-d4	10.87	131	566095	32.57	ng/ul	0.00
43) Dimethylphthalate-d6	13.97	166	1655285	35.15	ng/ul	0.00
46) Acenaphthylene-d8	14.26	160	2006389	35.23	ng/ul	0.00
51) 4-Nitrophenol-d4	14.76	143	220644	27.42	ng/ul	0.00
57) Fluorene-d10	15.56	176	1427081	35.20	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	202747	25.18	ng/ul	0.00
70) Anthracene-d10	17.41	188	2177473	35.99	ng/ul	0.00
76) Pyrene-d10	19.70	212	2359477	51.81	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.69	264	1343306	36.53	ng/ul	0.00
Target Compounds						
15) N-Nitroso-di-n-propylamine	8.63	70	16605	1.085	ng/ul#	1
44) Dimethylphthalate	14.02	163	379461	8.426	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092917\
Data File : BM011778.D
Acq On : 29 Sep 2017 21:50
Operator : SJ/JU
Sample : I5354-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 30 01:20:32 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM092717.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 30 00:51:32 2017
Response via : Initial Calibration




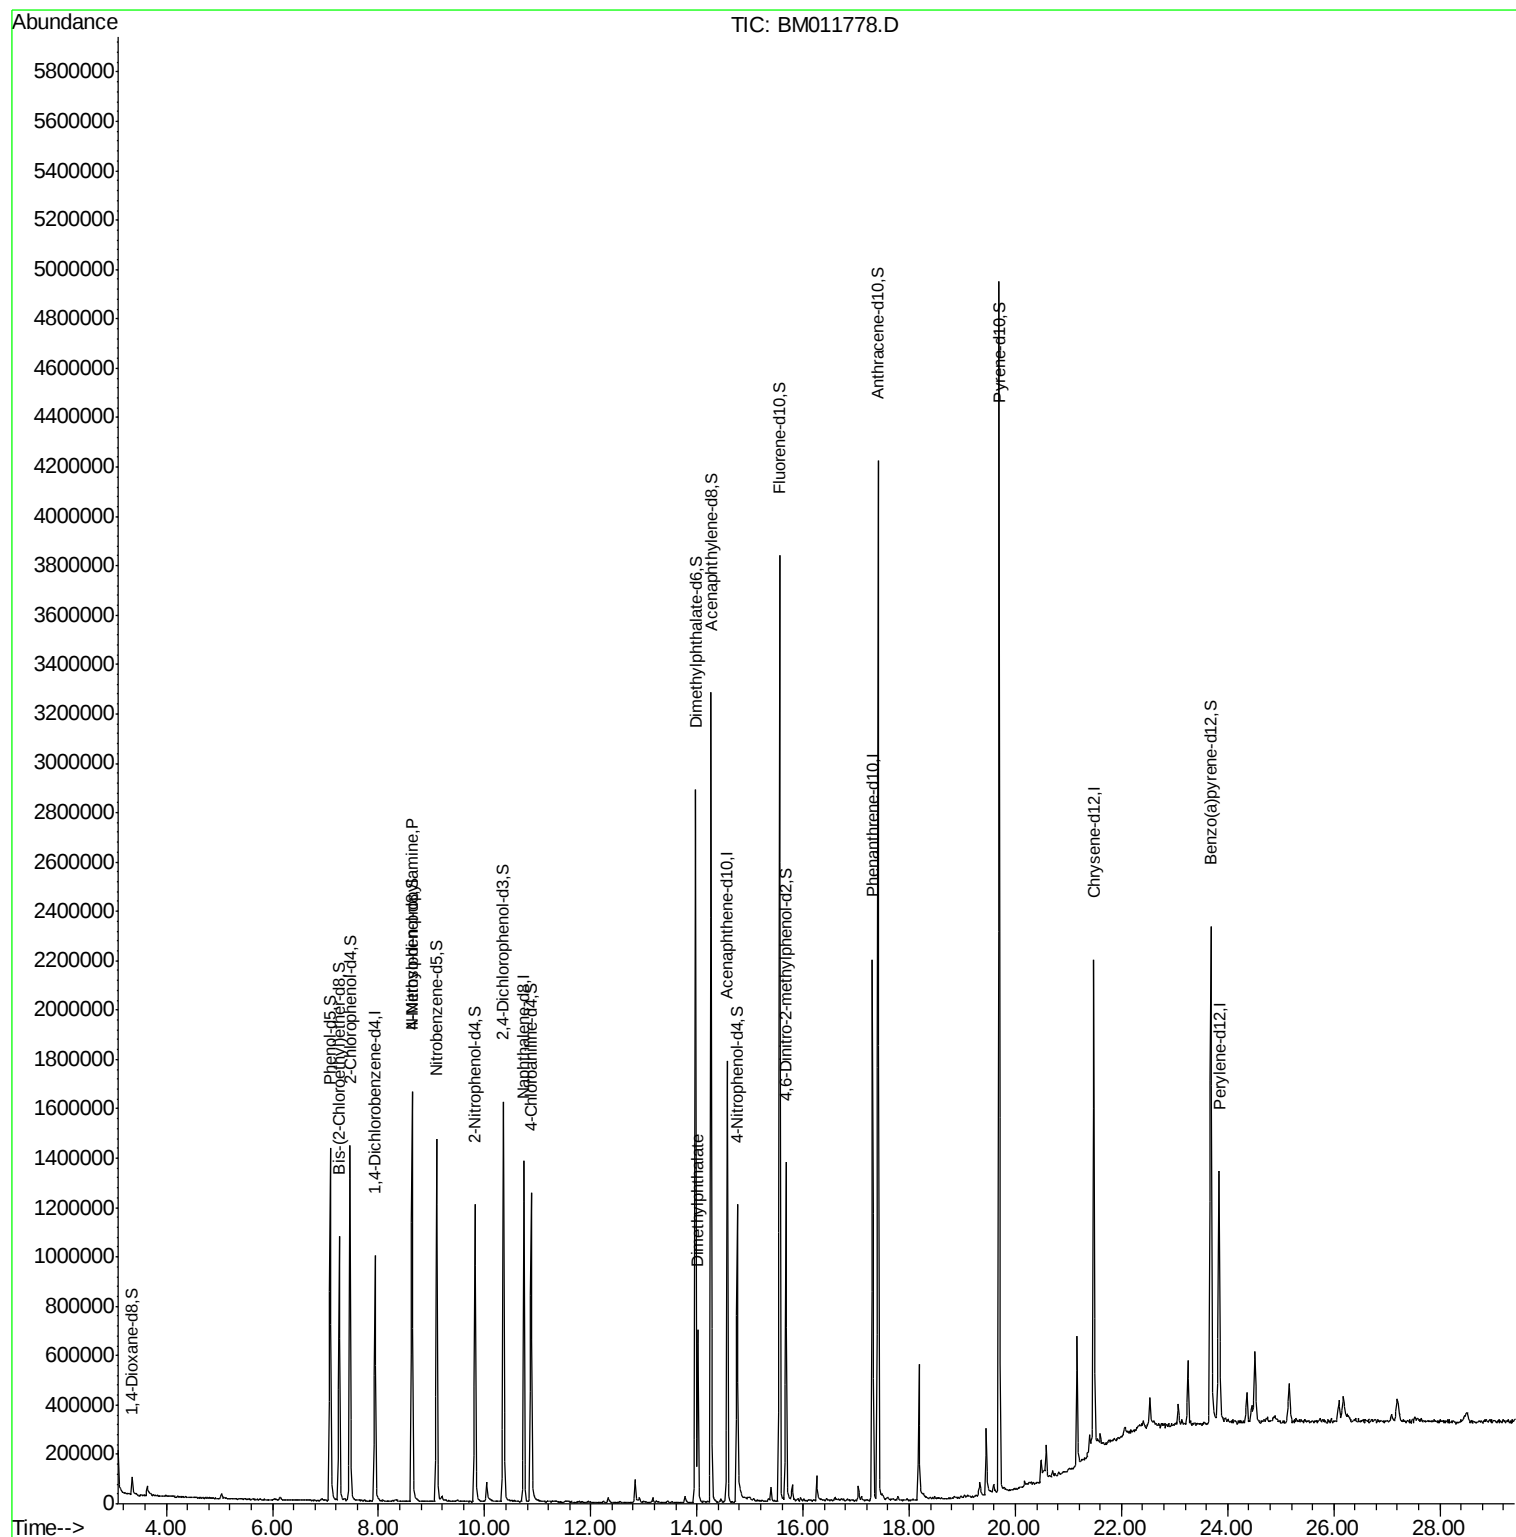


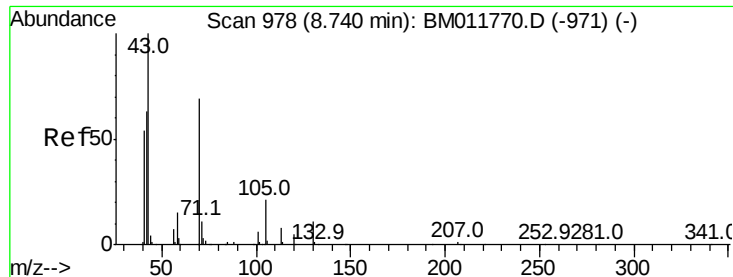

#15
N-Nitroso-di-n-propylamine
Concen: 1.085 ng/ul
RT: 8.63 min Scan# 942
Delta R.T. -0.11 min
Lab File: BM011778.D
Acq: 29 Sep 2017 21:50

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
70	100		
42	590.1	76.0	114.0#
101	0.0	6.7	10.1#
130	0.0	14.6	22.0#

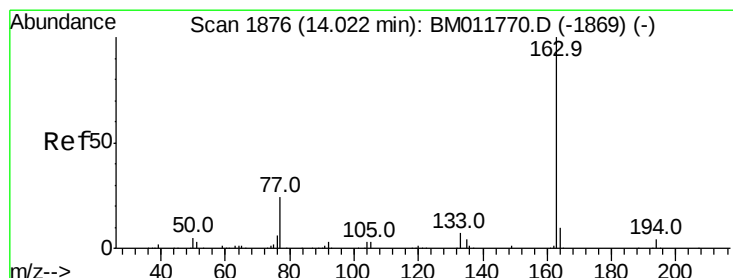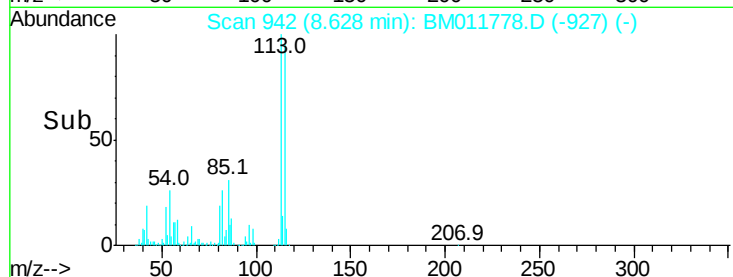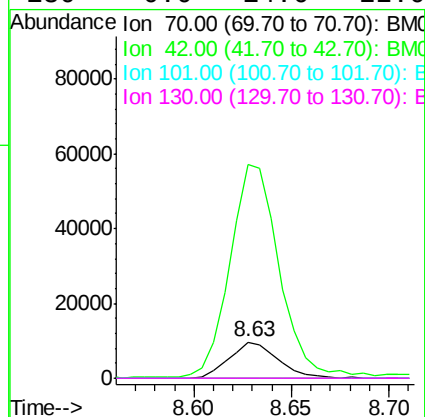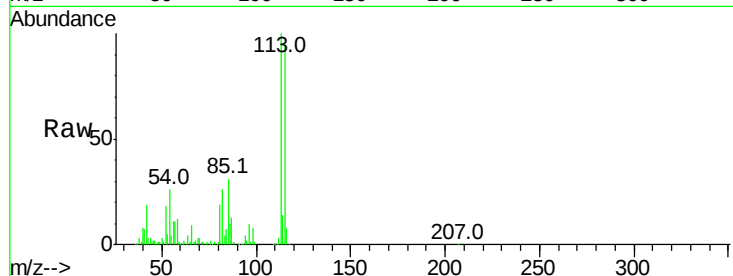

#44
Dimethylphthalate
Concen: 8.426 ng/ul
RT: 14.02 min Scan# 1858
Delta R.T. -0.01 min
Lab File: BM011778.D
Acq: 29 Sep 2017 21:50

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.5	5.3
164	10.4	8.2	12.4

