

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092917\
 Data File : BM011793.D
 Acq On : 30 Sep 2017 06:52
 Operator : SJ/JU
 Sample : I5354-20
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 30 09:11:40 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM092717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 30 06:38:23 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	296364	20.00	ng/ul	0.00
18) Naphthalene-d8	10.74	136	1399353	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.57	164	790012	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.31	188	1693878	20.00	ng/ul	0.00
75) Chrysene-d12	21.48	240	1335184	20.00	ng/ul	0.00
83) Perylene-d12	23.84	264	1107049	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.36	96	19488	2.93	ng/uL	0.00
5) Phenol-d5	7.09	99	456265	15.65	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.26	67	345516	16.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.46	132	383015	17.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.63	113	381235	16.70	ng/ul	0.00
19) Nitrobenzene-d5	9.10	128	189526	17.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.82	143	206114	17.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.36	165	371204	16.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.87	131	256290	10.43	ng/ul	0.00
43) Dimethylphthalate-d6	13.97	166	1190225	17.57	ng/ul	0.00
46) Acenaphthylene-d8	14.26	160	1458259	17.80	ng/ul	0.00
51) 4-Nitrophenol-d4	14.76	143	110885	9.58	ng/ul	0.00
57) Fluorene-d10	15.56	176	1012229	17.35	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	83049	7.24	ng/ul	0.00
70) Anthracene-d10	17.41	188	1553705	18.02	ng/ul	0.00
76) Pyrene-d10	19.70	212	1644303	25.80	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.69	264	951680	17.95	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.02	163	239641	3.698	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092917\
Data File : BM011793.D
Acq On : 30 Sep 2017 06:52
Operator : SJ/JU
Sample : I5354-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :

Quant Time: Sep 30 09:11:40 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM092717.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 30 06:38:23 2017
Response via : Initial Calibration

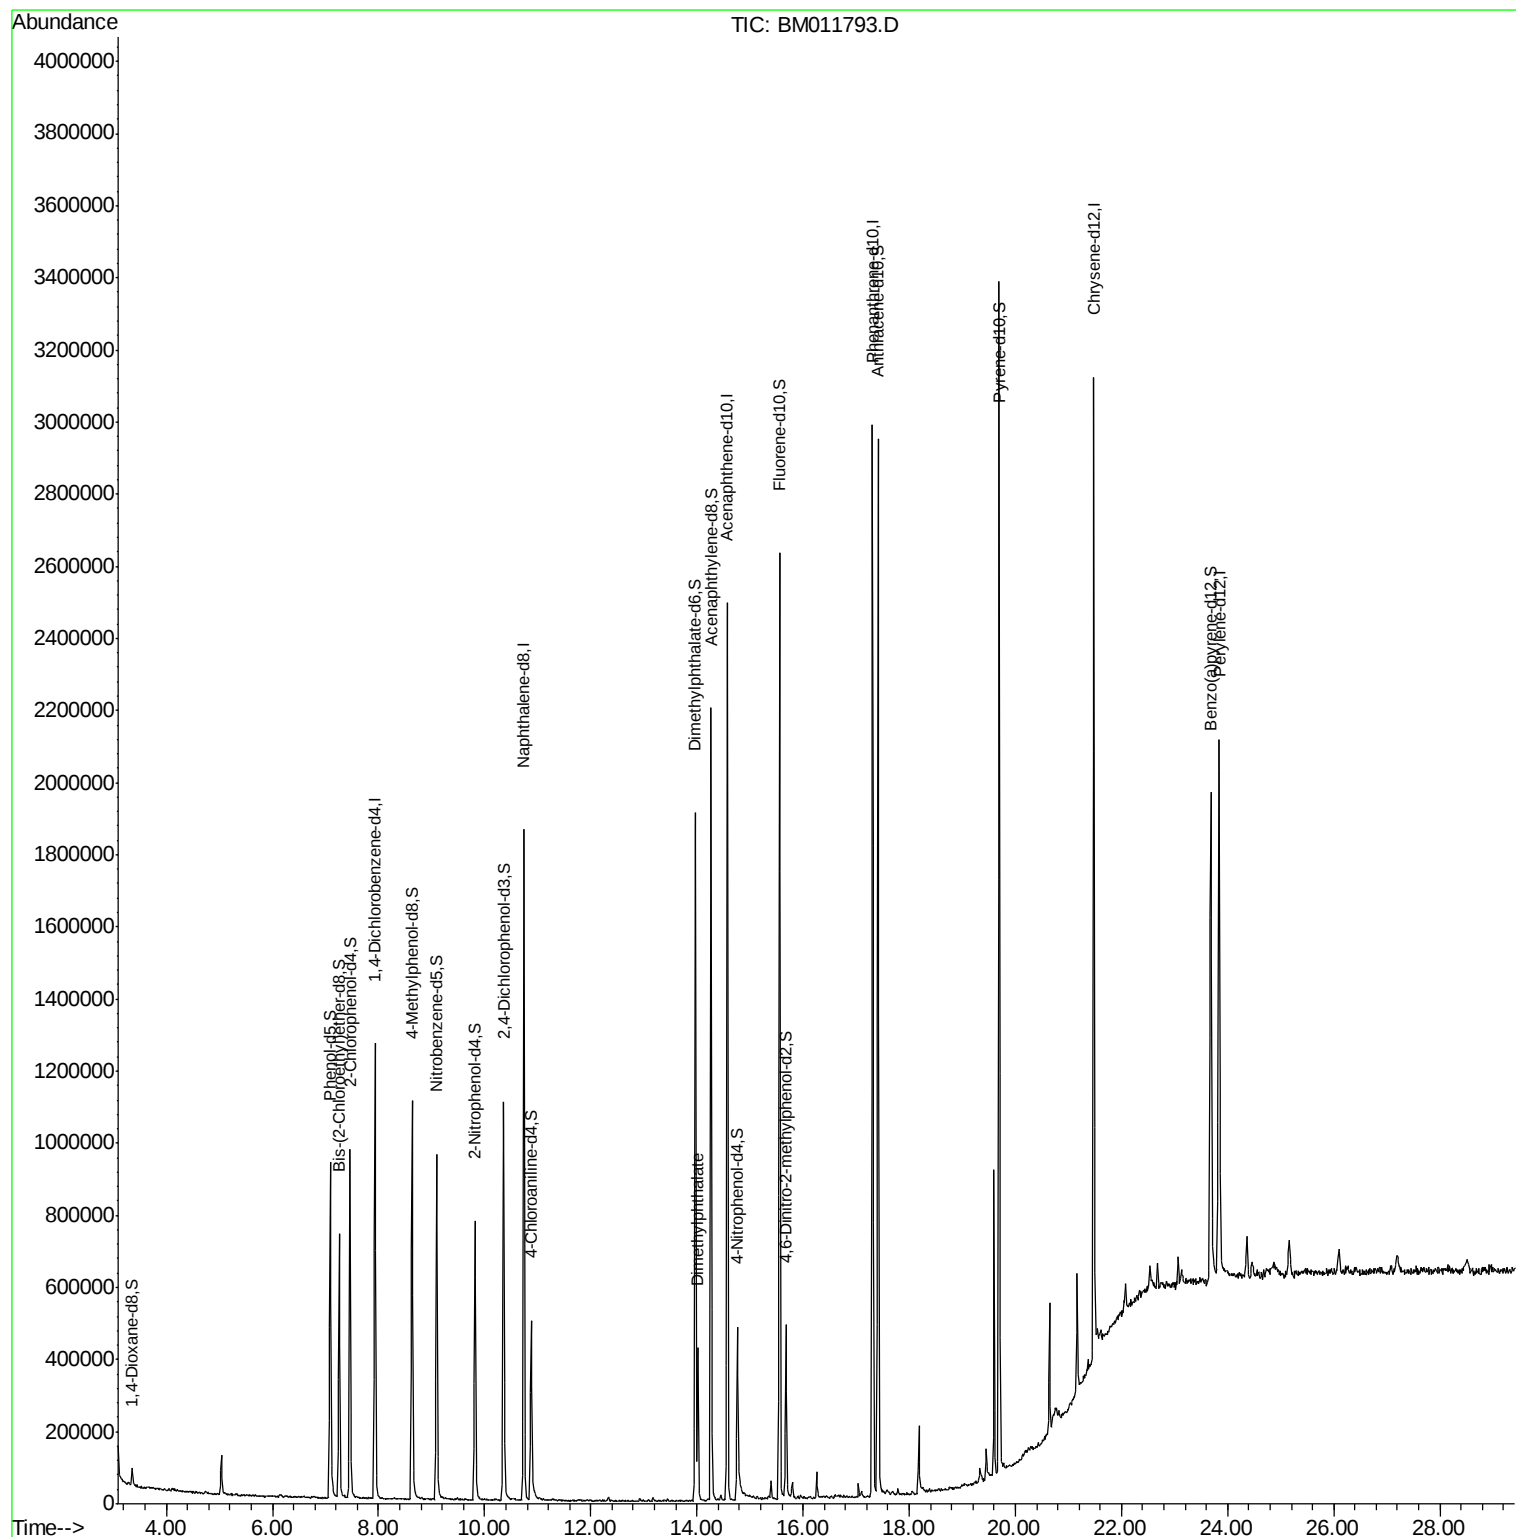

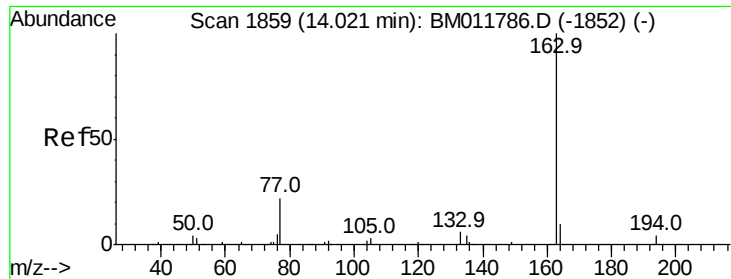

#44

Dimethylphthalate

Concen: 3.698 ng/ul

RT: 14.02 min Scan# 1858

Delta R.T. -0.01 min

Lab File: BM011793.D

Acq: 30 Sep 2017 06:52

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 239641

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 9.8 8.2 12.4

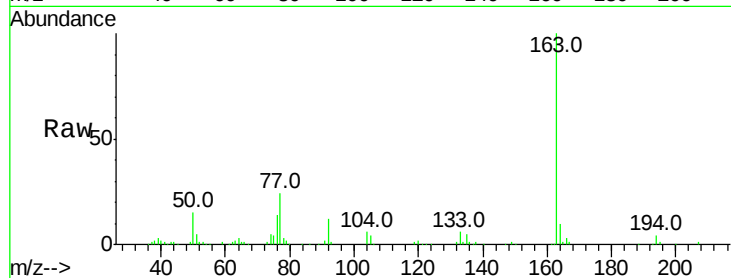

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

