

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA M\Data\BM092917\
 Data File : BM011787.D
 Acq On : 30 Sep 2017 03:15
 Operator : SJ/JU
 Sample : I5354-13
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 B0BB3

Quant Time: Sep 30 06:43:10 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM092717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 30 06:38:23 2017
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 10/2/2017 5:41:32 PM

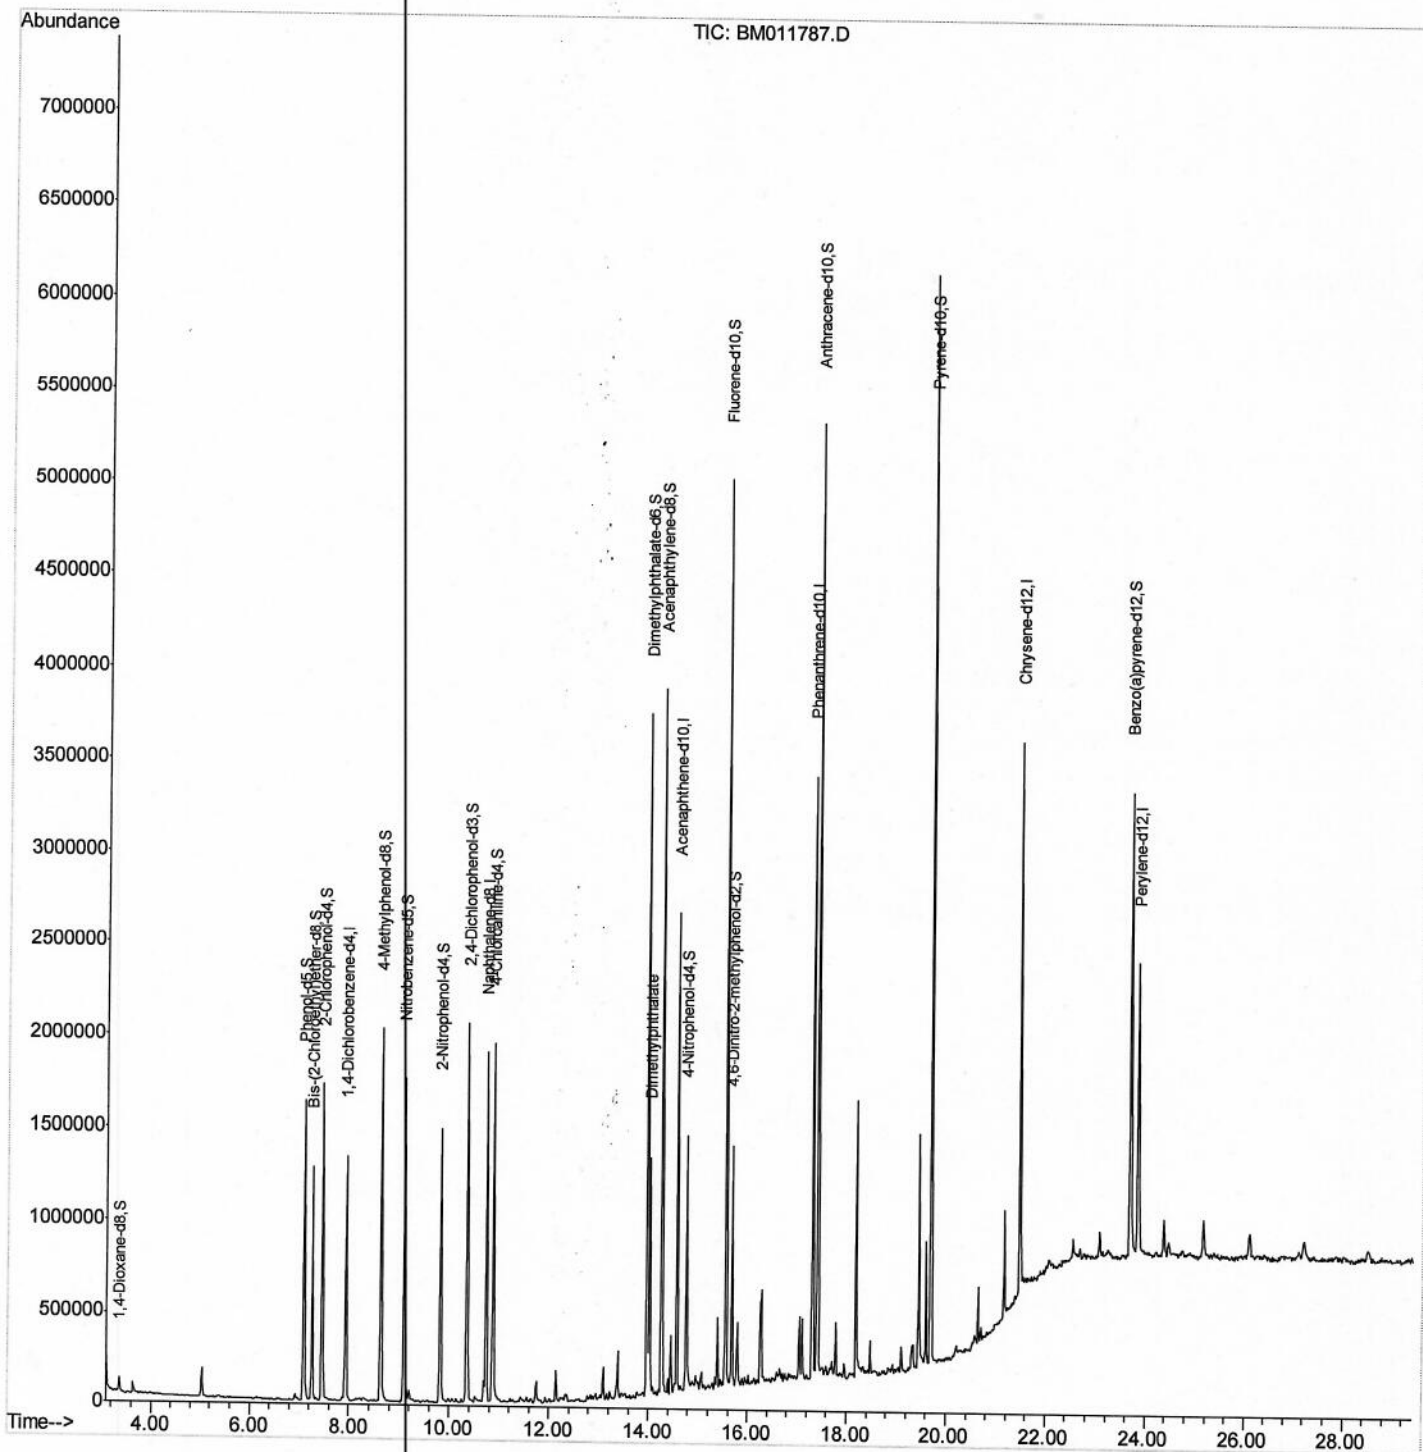

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM092917\
 Data File : BM011787.D
 Acq On : 30 Sep 2017 03:15
 Operator : SJ/JU
 Sample : I5354-13
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B0BB3

Manual Integrations
 APPROVED

Sohil
 10/2/2017 5:41:32 PM

Quant Time: Oct 07 05:06:28 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM092717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 02 07:18:07 2017
 Response via : Initial Calibration

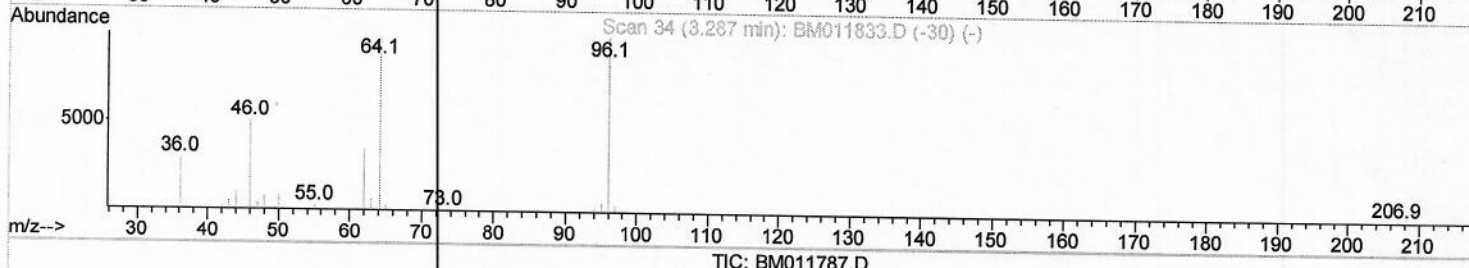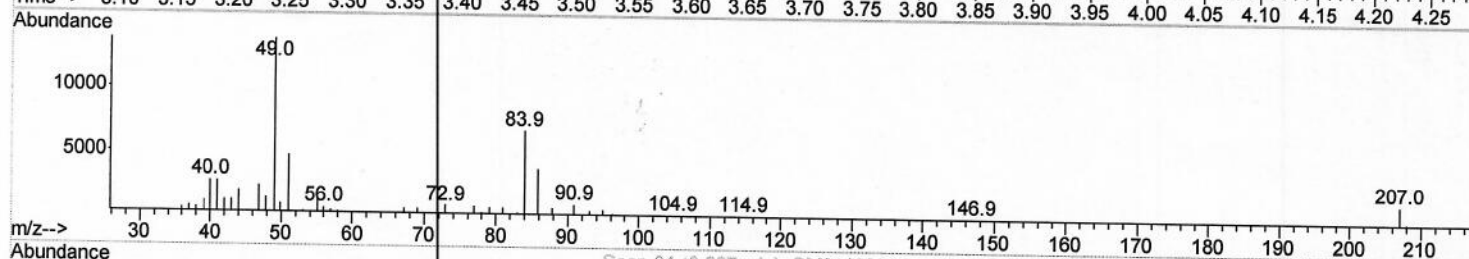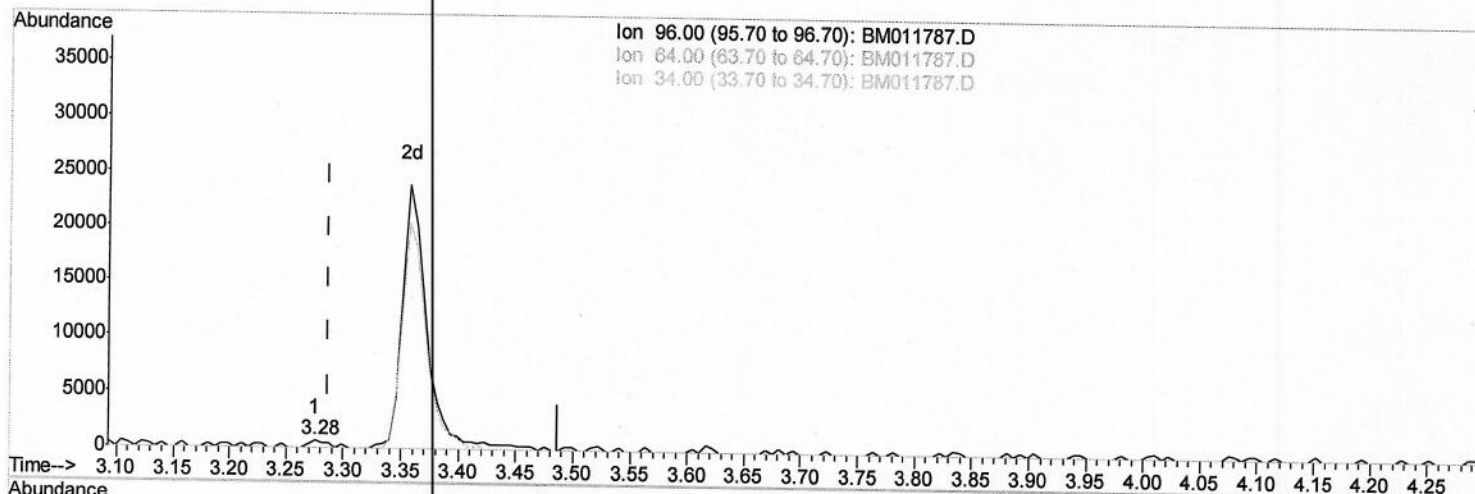

TIC: BM011787.D

(3) 1,4-Dioxane-d8 (S)

3.275min (-0.012) 0.09ng/uL

response 656

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	0.00#
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM092917\
 Data File : BM011787.D
 Acq On : 30 Sep 2017 03:15
 Operator : SJ/JU
 Sample : I5354-13
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B0BB3

Manual Integrations
 APPROVED

Sohil
 10/2/2017 5:41:32 PM

Quant Time: Sep 30 06:43:10 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM092717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 30 06:38:23 2017
 Response via : Initial Calibration

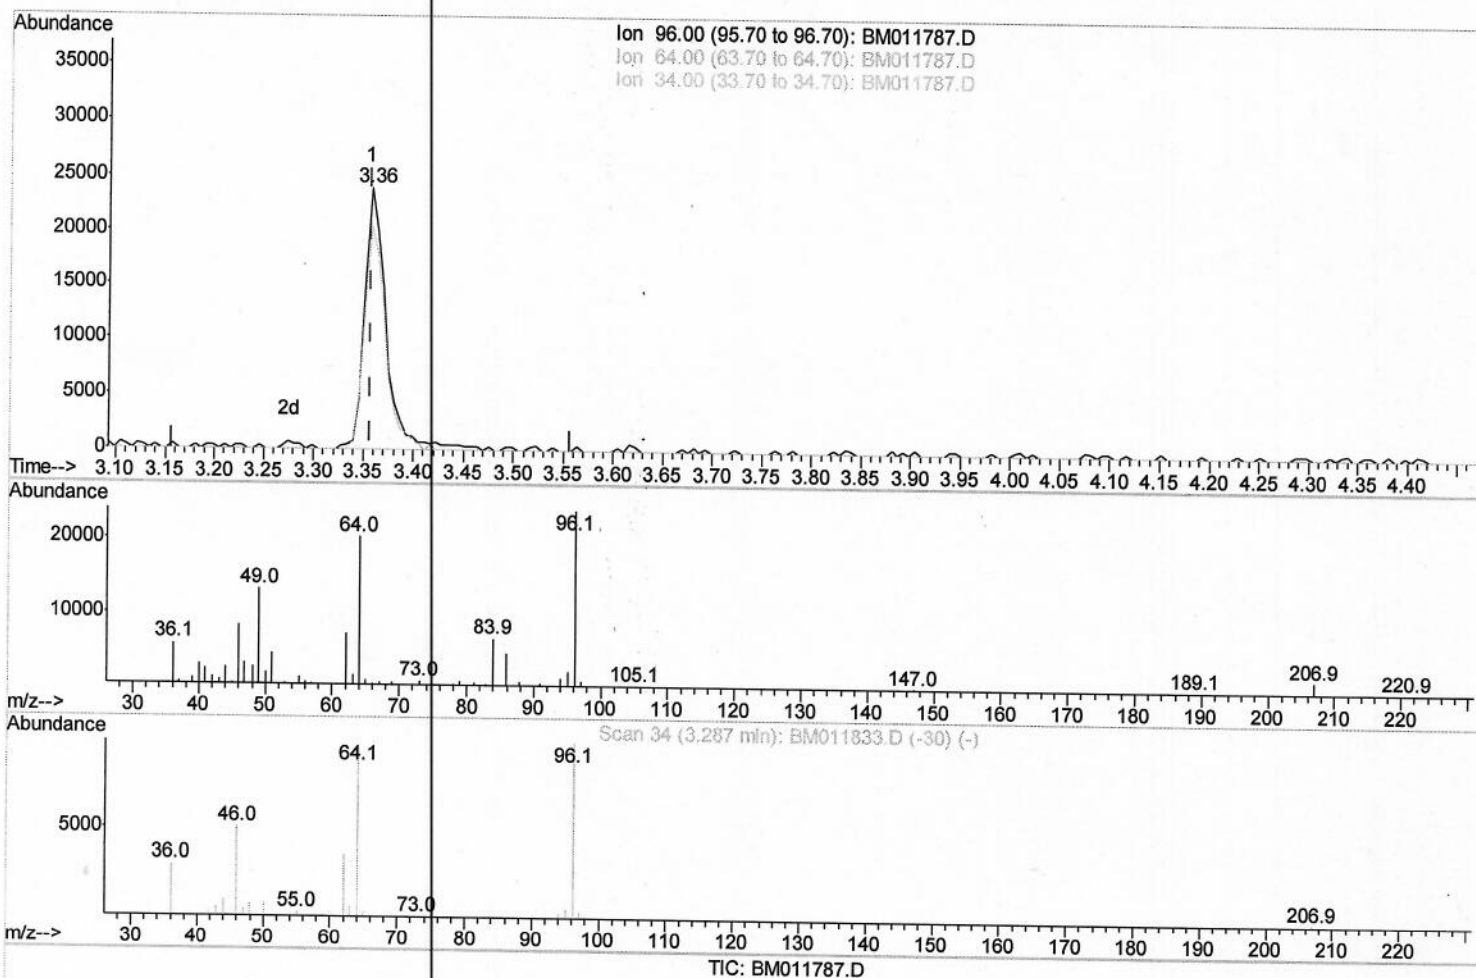

(3) 1,4-Dioxane-d8 (S)

3.357min (-0.000) 5.02ng/uL m

response 35904

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	83.95
34.00	0.00	0.00
0.00	0.00	0.00

> Jy 10/06/17

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA M\Data\BM092917\
 Data File : BM011787.D
 Acq On : 30 Sep 2017 03:15
 Operator : SJ/JU
 Sample : I5354-13
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 B0BB3

Manual Integrations
 APPROVED

Sohil
 10/2/2017 5:41:32 PM

Quant Time: Sep 30 06:43:10 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM092717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 30 06:38:23 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	318631	20.00	ng/ul	0.00
18) Naphthalene-d8	10.74	136	1444907	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.57	164	821110	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.32	188	1786129	20.00	ng/ul	0.00
75) Chrysene-d12	21.48	240	1408126	20.00	ng/ul	0.00
83) Perylene-d12	23.84	264	1167045	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.36	96	35904m	5.02	ng/uL	0.00
5) Phenol-d5	7.09	99	807348	25.76	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	7.26	67	604278	26.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.46	132	670930	28.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.63	113	682402	27.80	ng/ul	0.00
19) Nitrobenzene-d5	9.10	128	337273	29.92	ng/ul	0.00
22) 2-Nitrophenol-d4	9.82	143	383724	31.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.36	165	664871	28.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.87	131	925251	36.48	ng/ul	0.00
43) Dimethylphthalate-d6	13.97	166	2158496	30.65	ng/ul	0.00
46) Acenaphthylene-d8	14.27	160	2657158	31.20	ng/ul	0.00
51) 4-Nitrophenol-d4	14.76	143	296129	24.60	ng/ul	0.00
57) Fluorene-d10	15.56	176	1832409	30.22	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.68	200	209259	17.30	ng/ul	0.00
70) Anthracene-d10	17.42	188	2860944	31.48	ng/ul	0.00
76) Pyrene-d10	19.70	212	3002348	44.68	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.69	264	1772749	31.73	ng/ul	0.00
Target Compounds						
44) Dimethylphthalate	14.02	163	683677	10.150	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed