
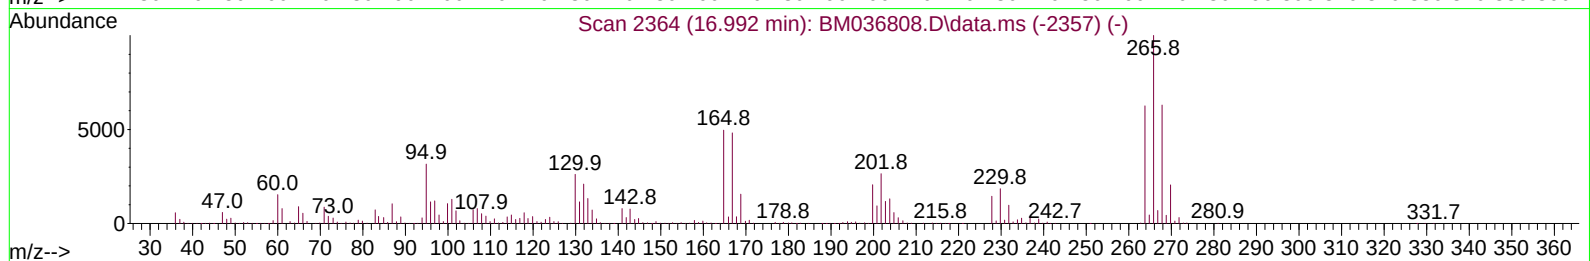
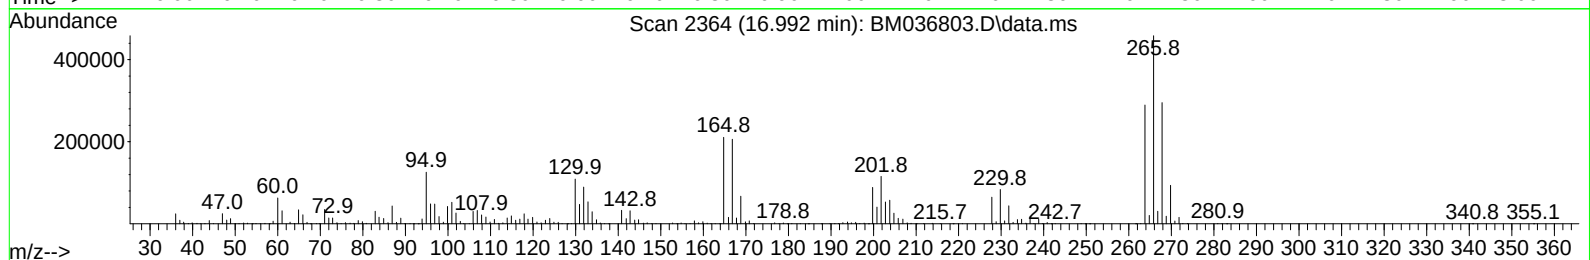


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093022\
Data File : BM036803.D
Acq On : 30 Sep 2022 09:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 15:52:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM093022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 30 15:41:14 2022
Response via : Initial Calibration

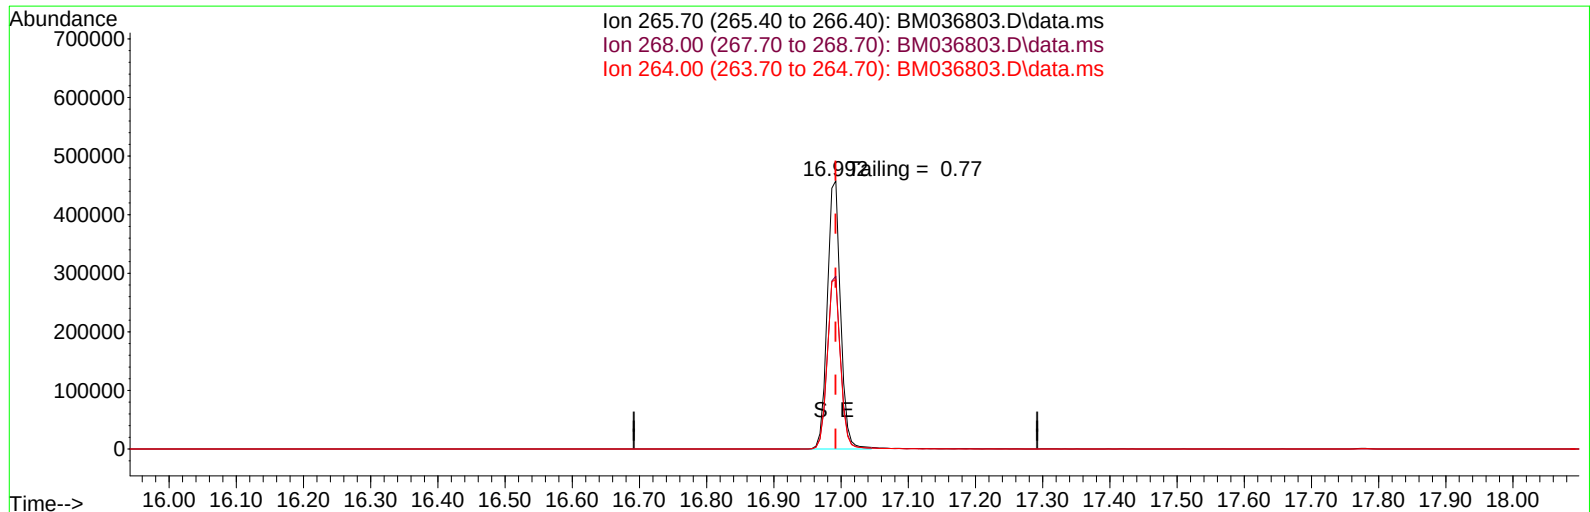

TIC: BM036803.D\data.ms

(70) Pentachlorophenol (C)




16.992min (+ 0.000) 1769348.61 ng

response 631213

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	64.42
264.00	64.10	63.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093022\
Data File : BM036803.D
Acq On : 30 Sep 2022 09:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 15:52:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM093022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 30 15:41:14 2022
Response via : Initial Calibration

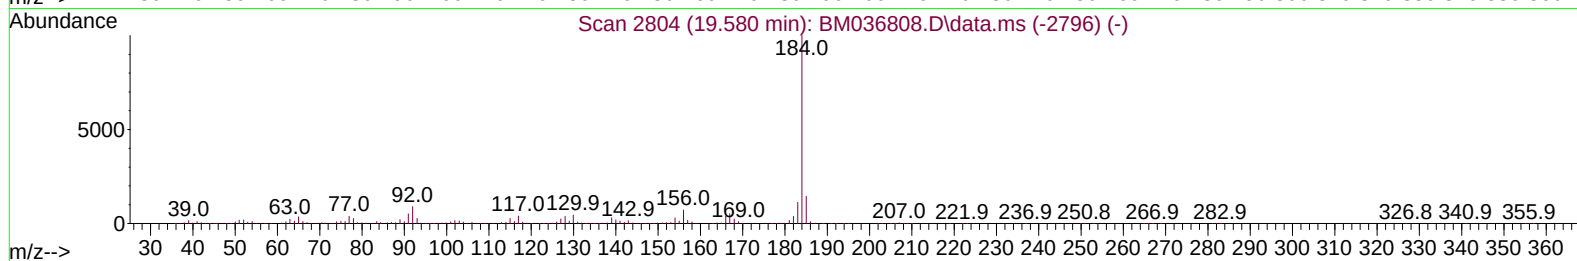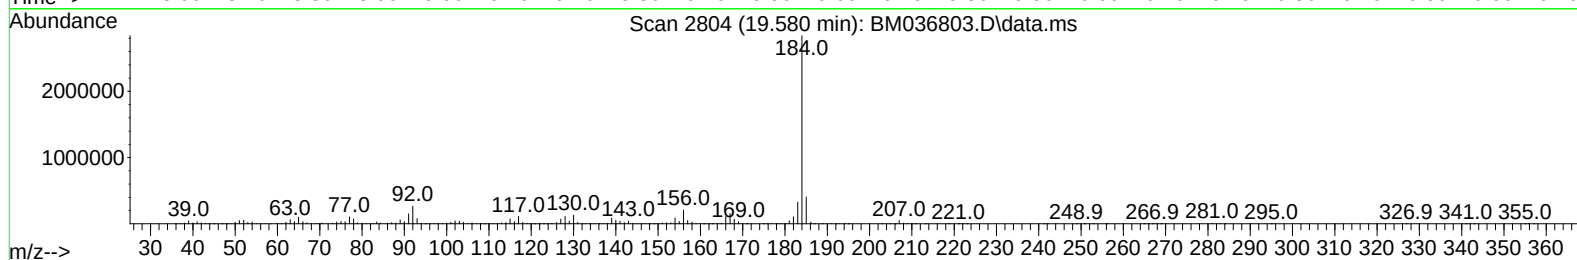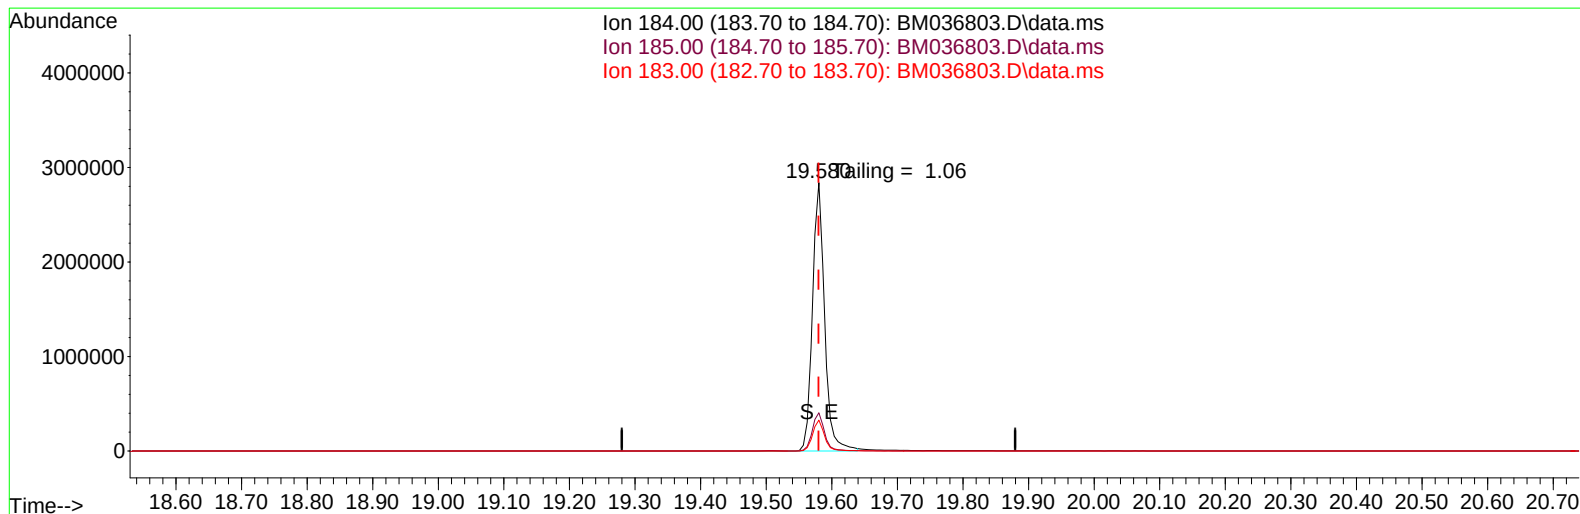

TIC: BM036803.D\data.ms

(77) Benzidine

19.580min (+ 0.000) 432351.92 ng

response 3685287

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.26
183.00	11.00	11.51
0.00	0.00	0.00