

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093022\
 Data File : BM036813.D
 Acq On : 30 Sep 2022 15:54
 Operator : CG/JU
 Sample : PB147971BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB147971BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM093022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036813.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.063	331	336	346	rVB	211042	302163	1.26%	0.304%
2	5.534	408	416	431	rBV	6767374	9957121	41.67%	10.020%
3	7.139	679	689	704	rBV	6736126	10576936	44.26%	10.644%
4	7.975	824	831	843	rBV	1122125	1707524	7.15%	1.718%
5	9.145	1022	1030	1044	rBV	3805197	6215202	26.01%	6.254%
6	10.786	1301	1309	1317	rBV	1524780	2500552	10.46%	2.516%
7	13.233	1718	1725	1738	rBV	10158674	14709508	61.56%	14.802%
8	14.604	1951	1958	1973	rBV	2422824	3456284	14.46%	3.478%
9	16.086	2202	2210	2228	rBV	8320356	11296252	47.27%	11.367%
10	17.339	2417	2423	2433	rBV	2968005	4309528	18.03%	4.337%
11	19.956	2863	2868	2877	rBV	18841242	23895697	100.00%	24.046%
12	20.721	2994	2998	3002	rVB	314241	339889	1.42%	0.342%
13	21.515	3128	3133	3141	rBV	4033418	4971765	20.81%	5.003%
14	23.933	3538	3544	3556	rVB2	2625639	5135664	21.49%	5.168%




Sum of corrected areas: 99374085

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093022\
Data File : BM036813.D
Acq On : 30 Sep 2022 15:54
Operator : CG/JU
Sample : PB147971BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB147971BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM093022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

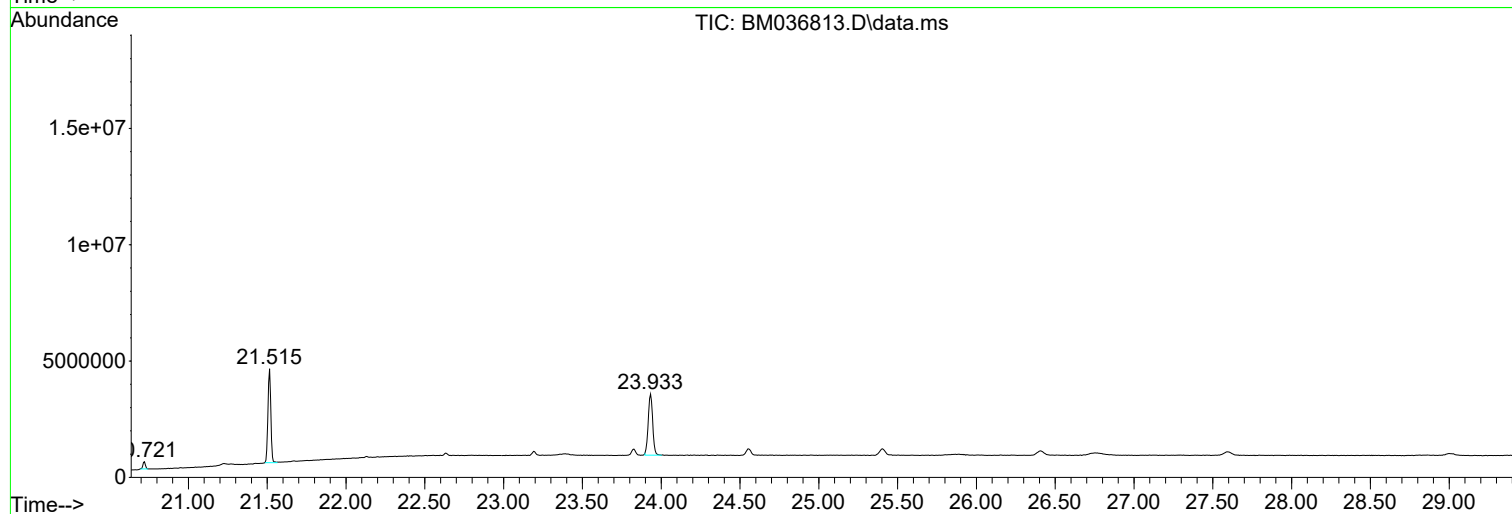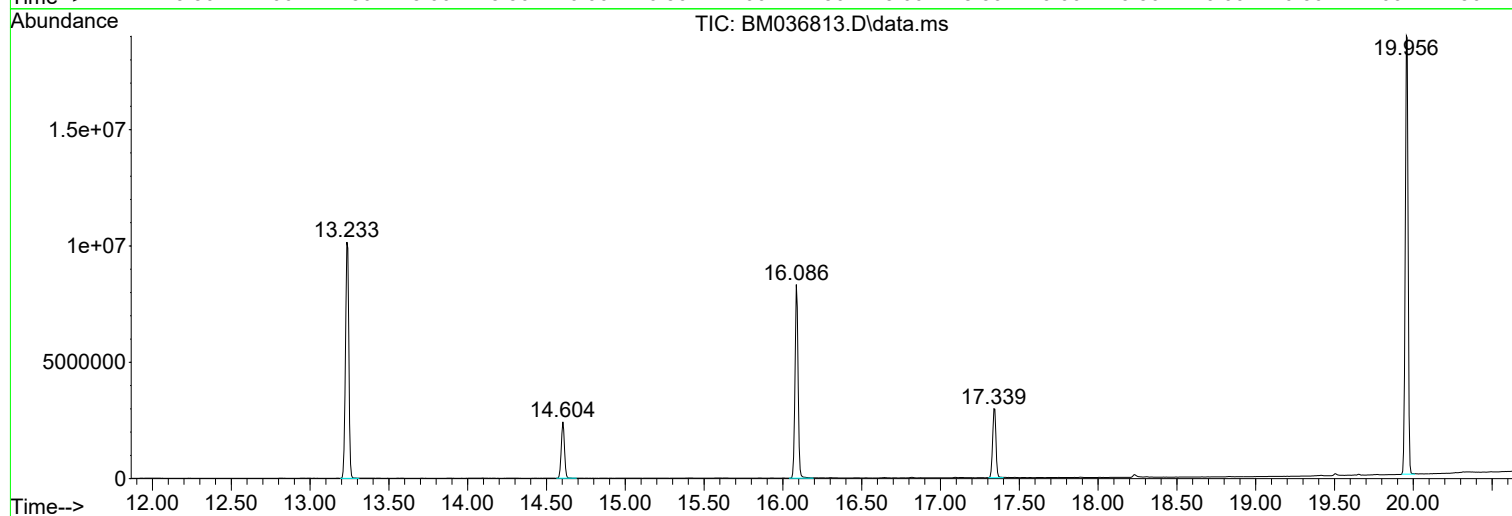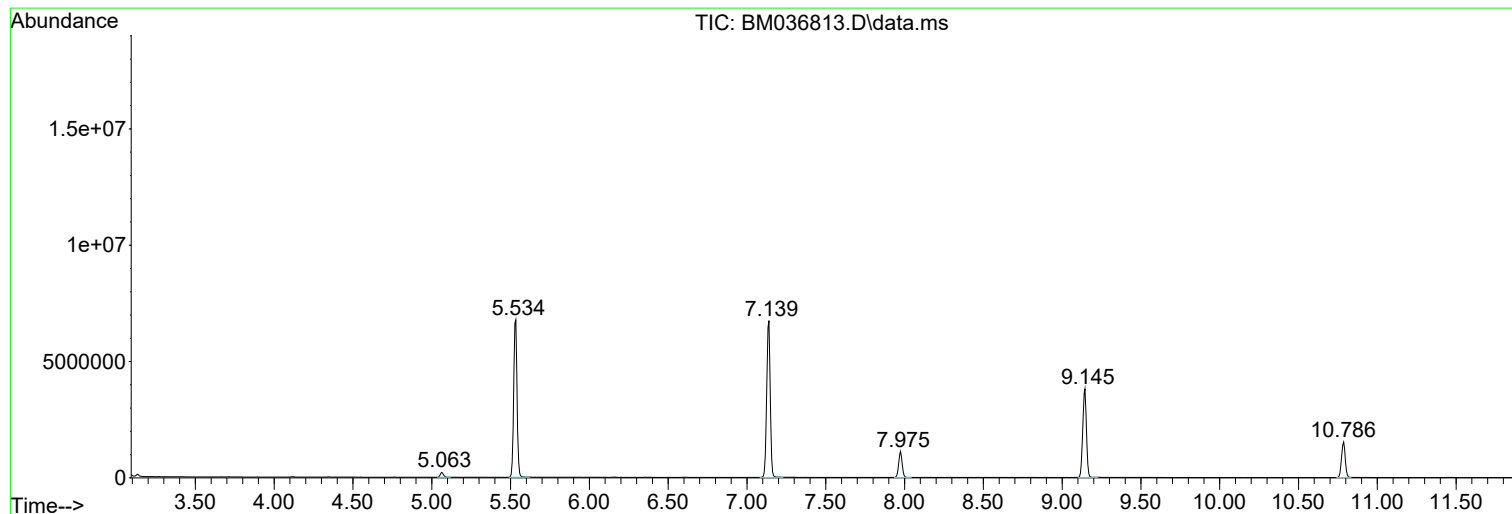

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093022\
Data File : BM036813.D
Acq On : 30 Sep 2022 15:54
Operator : CG/JU
Sample : PB147971BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB147971BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM093022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.063	3.54 ng	302163	1,4-Dichlorobenzene-d4	7.975

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	53		
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25		
3	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		
4	5-Hexen-2-one	98	C6H10O	000109-49-9	9		
5	Methyl 2,5,8,11-tetraoxatridecan...	236	C10H20O6	1000366-78-2	9		

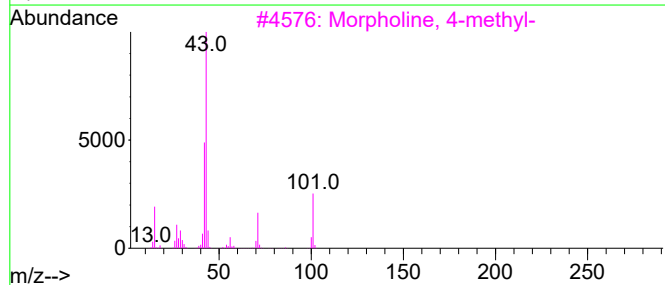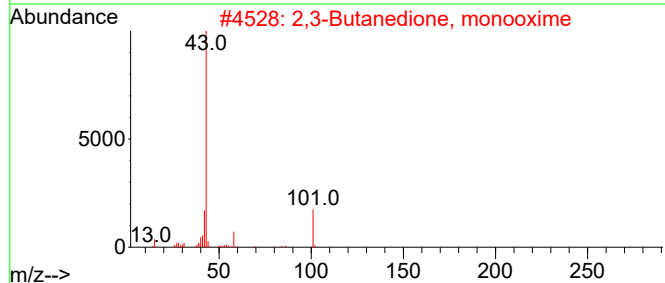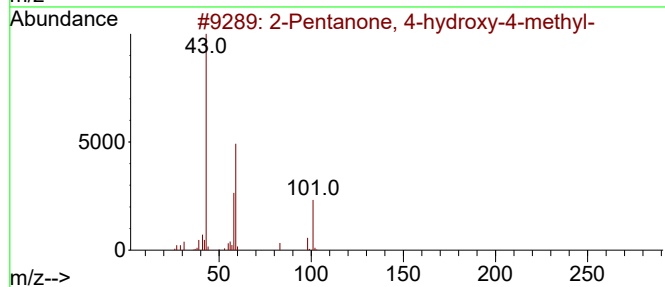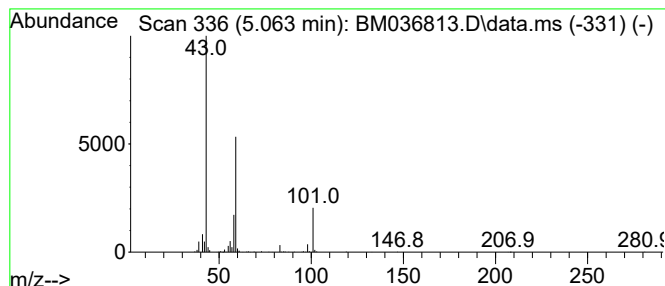

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093022\
Data File : BM036813.D
Acq On : 30 Sep 2022 15:54
Operator : CG/JU
Sample : PB147971BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB147971BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM093022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.063	3.5	ng	302163	1	7.975	1707520	20.0