


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM093022\  
 Data File : BM036803.D  
 Acq On : 30 Sep 2022 09:38  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM093022.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Sep 30 15:41:14 2022

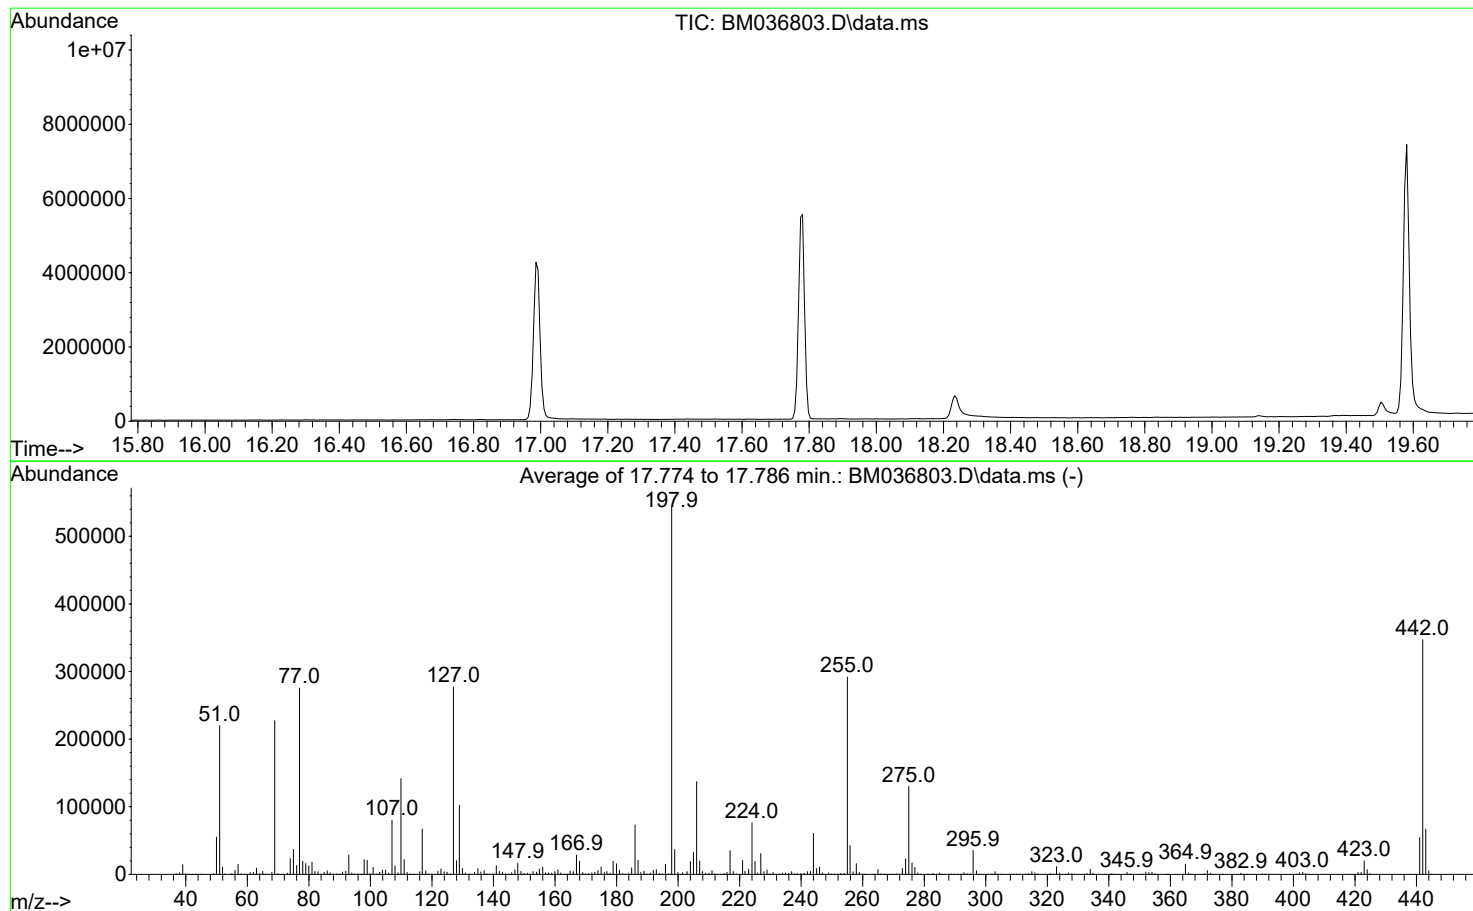

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2489

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 40.4         | 219907     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.4          | 3175       | PASS                |
| 69             | 198             | 0.00            | 100             | 41.8         | 227254     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 1145       | PASS                |
| 127            | 198             | 10              | 80              | 51.0         | 277269     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.2          | 880        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 544107     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 36805      | PASS                |
| 275            | 198             | 10              | 60              | 23.9         | 129824     | PASS                |
| 365            | 198             | 1               | 100             | 2.8          | 15181      | PASS                |
| 441            | 198             | 0.01            | 100             | 10.0         | 54520      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 347115     | PASS                |
| 443            | 442             | 15              | 24              | 19.3         | 67069      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 9/30/2022     | BNA_M            | <u>BM036803.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1954069          | 20.83              |
| DDD           | 15378            | 20.36              |
| DDE           | 1155             | 19.86              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 16533         | 1970602          | 0.84               |
|               |                  |                    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM093022\  
Data File : BM036803.D  
Acq On : 30 Sep 2022 09:38  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Sep 30 15:52:35 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM093022.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Sep 30 15:41:14 2022  
Response via : Initial Calibration

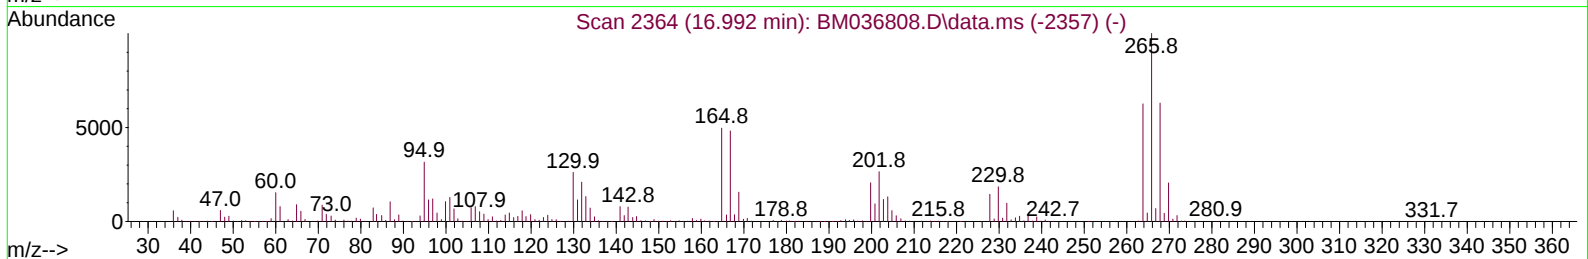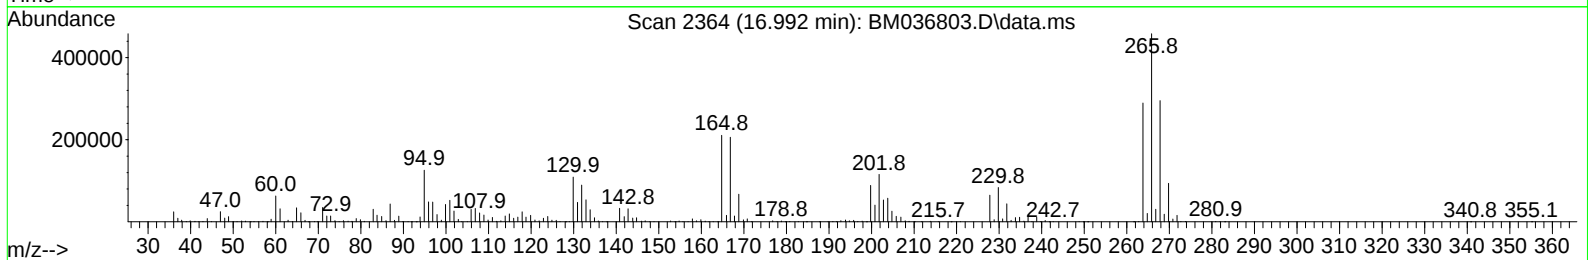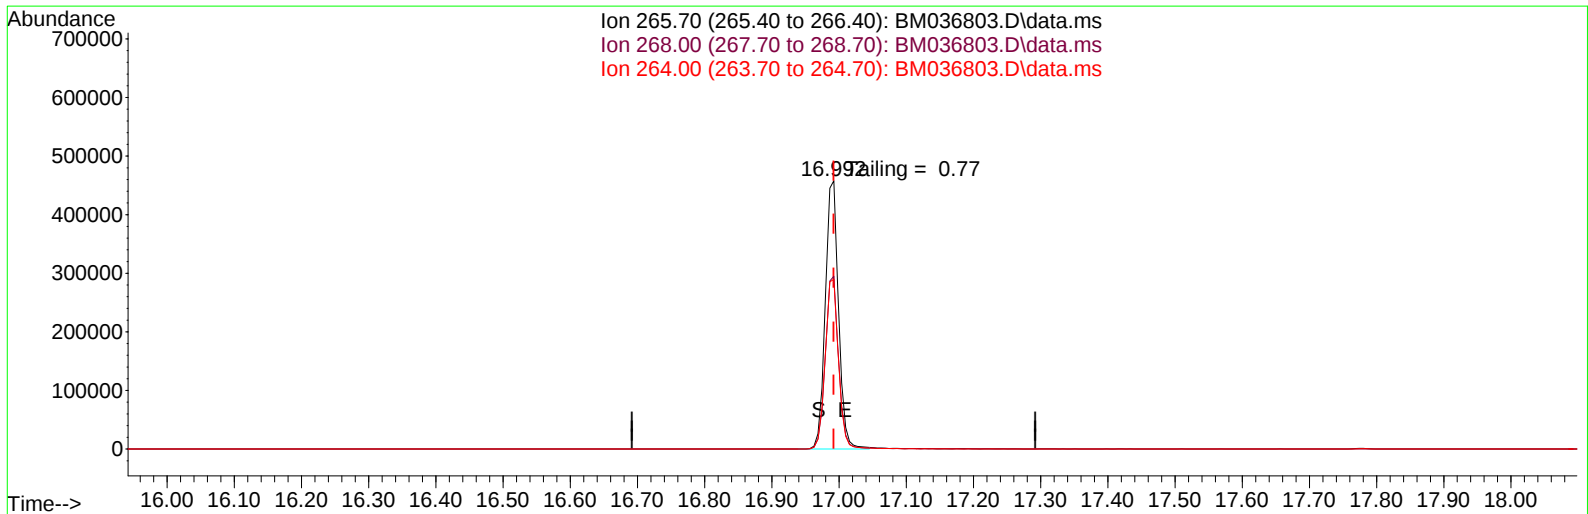

TIC: BM036803.D\data.ms

**(70) Pentachlorophenol (C)**

16.992min (+ 0.000) 1769348.61 ng




response 631213

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.40  | 64.42  |
| 264.00 | 64.10  | 63.20  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM093022\  
Data File : BM036803.D  
Acq On : 30 Sep 2022 09:38  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Sep 30 15:52:35 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM093022.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Sep 30 15:41:14 2022  
Response via : Initial Calibration

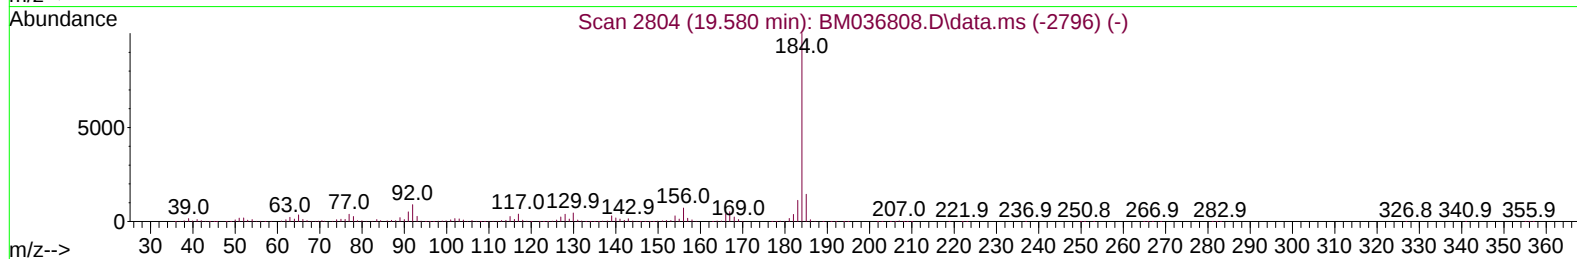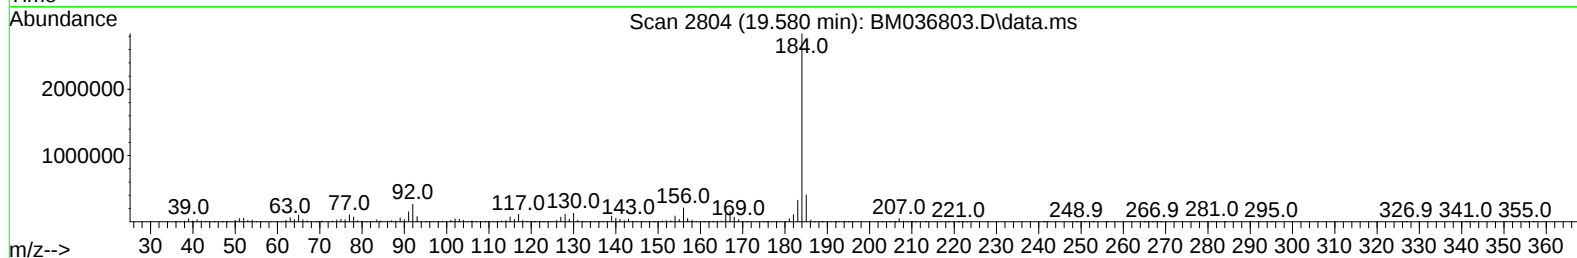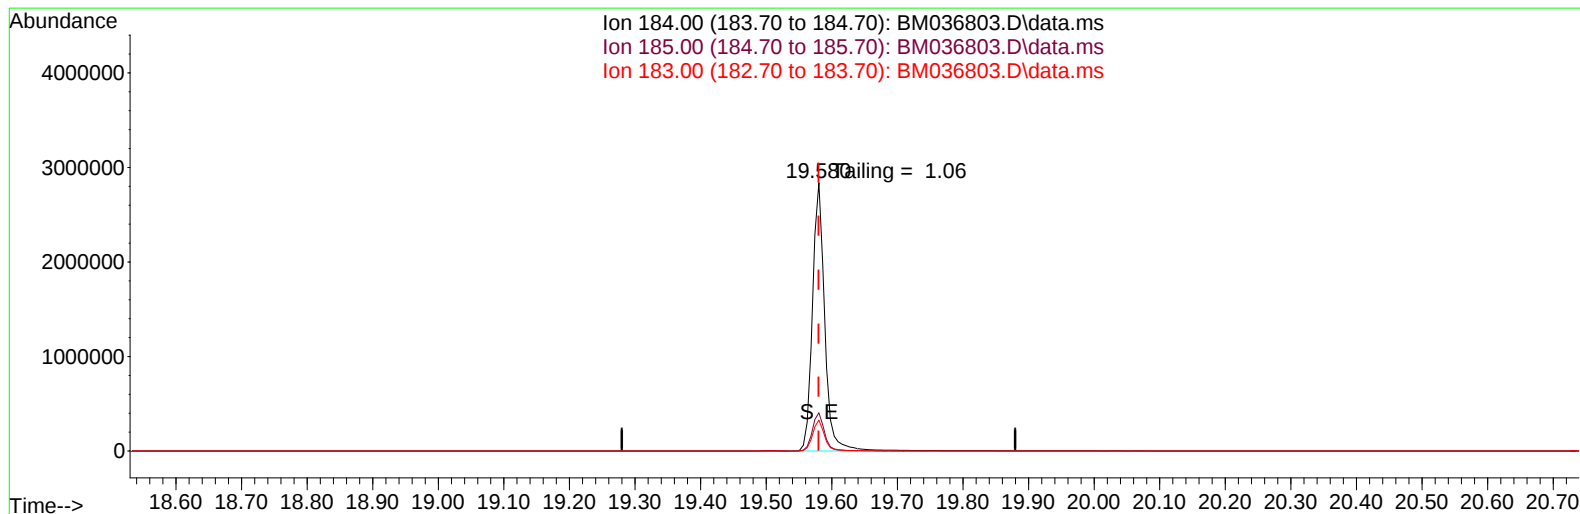

TIC: BM036803.D\data.ms

(77) Benzidine

19.580min (+ 0.000) 432351.92 ng

response 3685287

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.10  | 14.26  |
| 183.00 | 11.00  | 11.51  |
| 0.00   | 0.00   | 0.00   |