




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047712.D
Acq On : 30 Sep 2024 11:19
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK375

Manual IntegrationsAPPROVED

Quant Time: Sep 30 11:55:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/01/2024
Supervised By :mohammad ahmed 10/01/2024

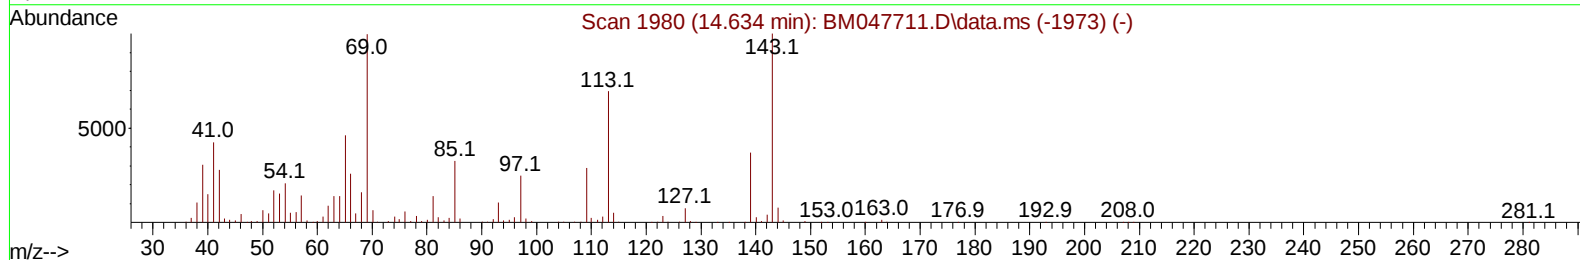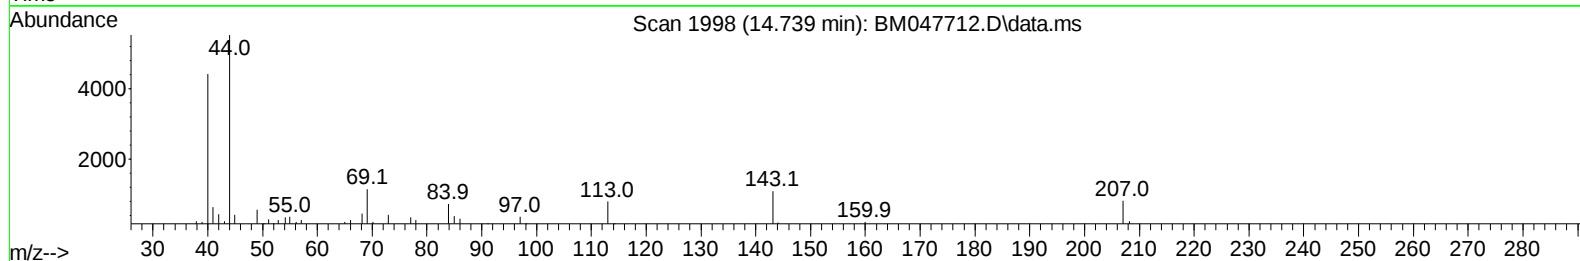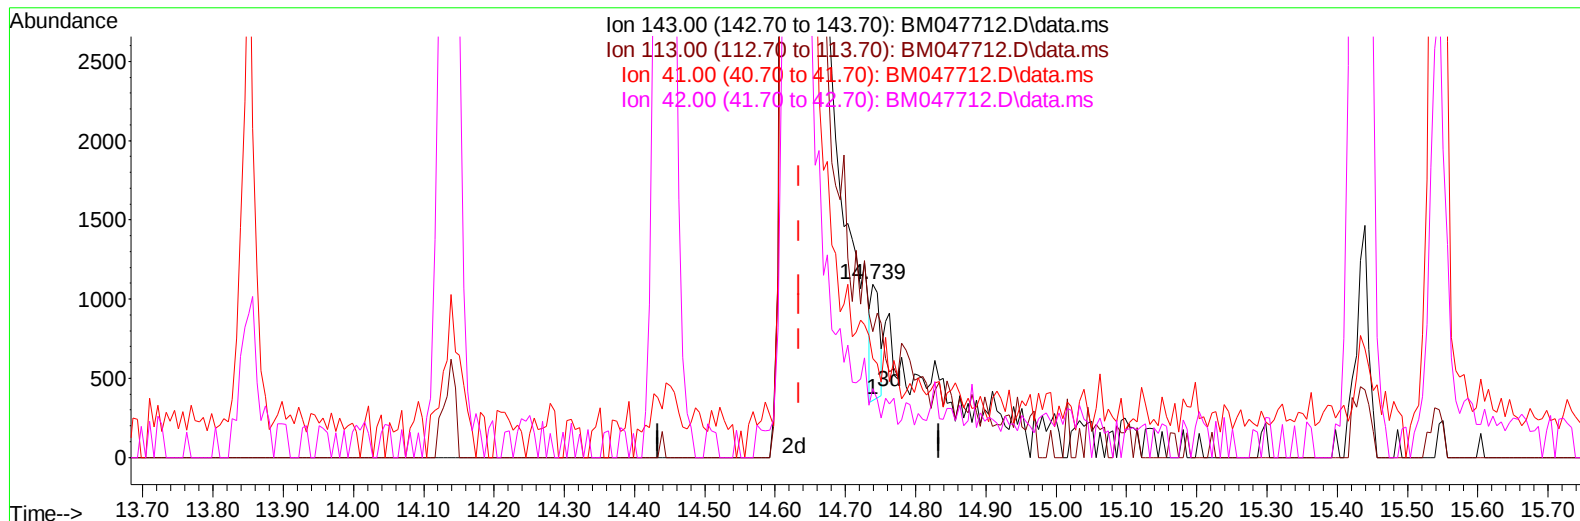

TIC: BM047712.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.739min (+ 0.106) 0.08 ng/u1

response 605

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.20	72.60
41.00	60.00	57.26
42.00	40.50	39.63




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047712.D
Acq On : 30 Sep 2024 11:19
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK375

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/01/2024
Supervised By :mohammad ahmed 10/01/2024

Quant Time: Sep 30 11:55:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

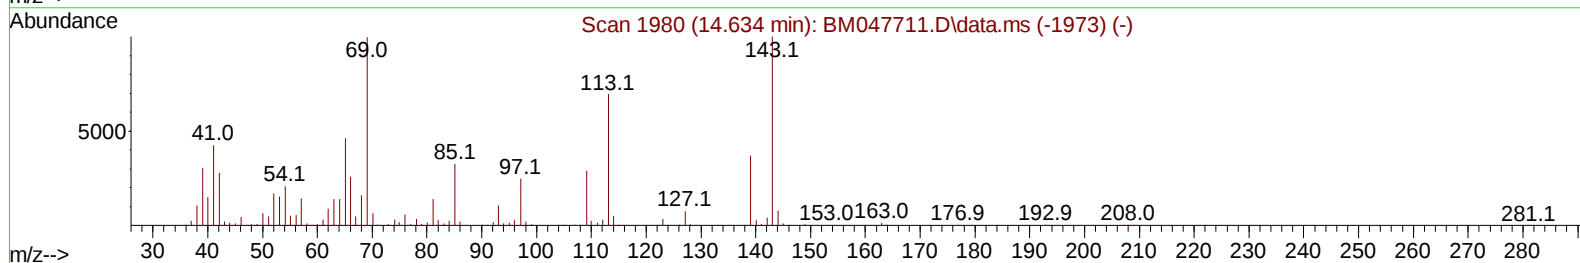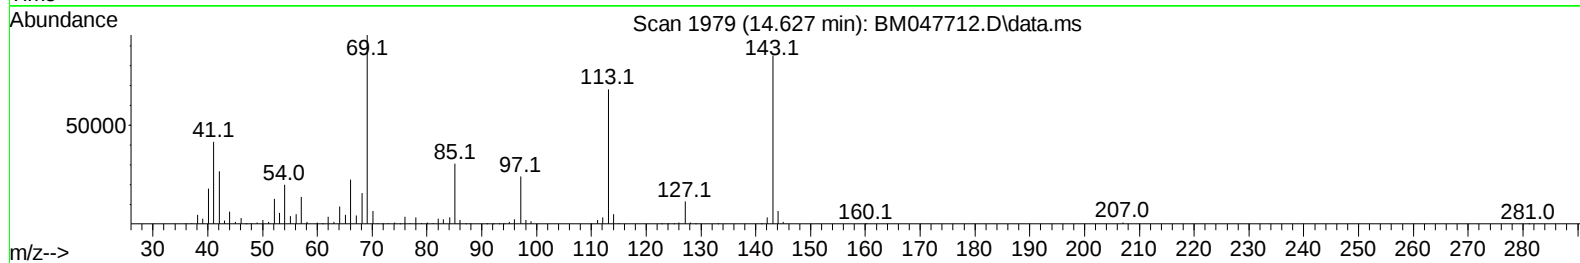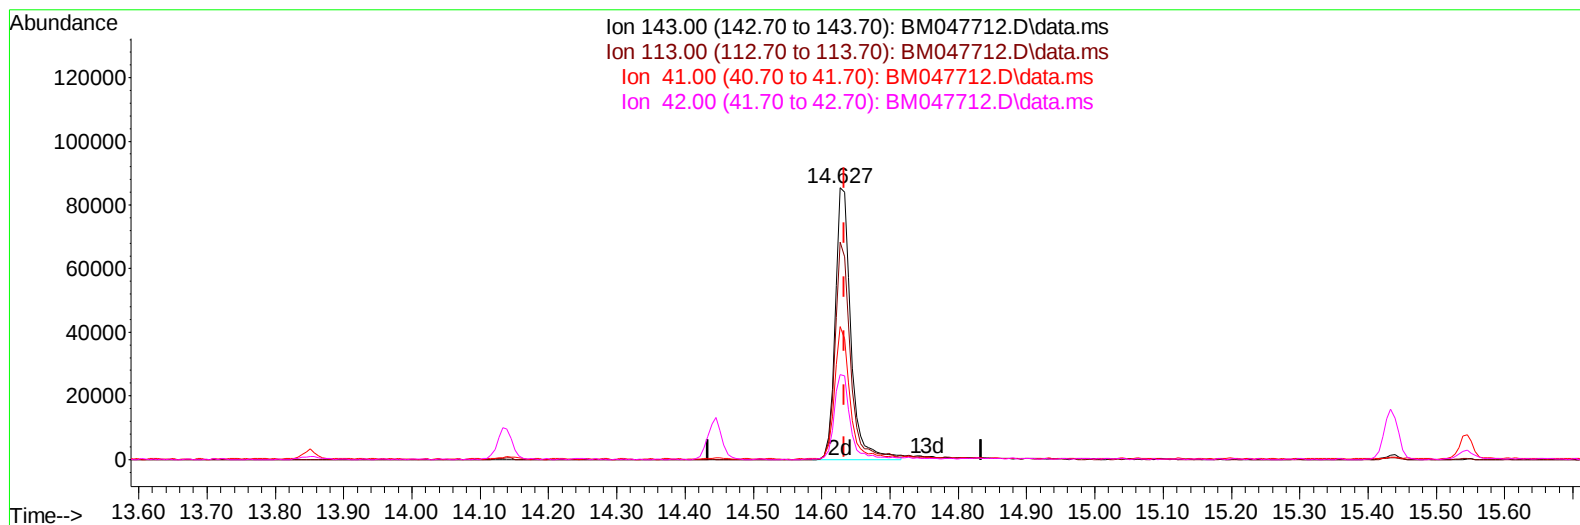

TIC: BM047712.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.627min (-0.006) 16.96 ng/ul m

response 135533

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.20	79.98
41.00	60.00	48.83
42.00	40.50	31.30#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
 Data File : BM047712.D
 Acq On : 30 Sep 2024 11:19
 Operator : RC/JU
 Sample : PB163513BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK375

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/01/2024
 Supervised By :mohammad ahmed 10/01/2024

Quant Time: Sep 30 11:55:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 02:30:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	233423	20.000	ng/ul	0.00
20) Naphthalene-d8	10.604	136	938207	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.445	164	553769	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.180	188	1095236	20.000	ng/ul	0.00
79) Chrysene-d12	21.403	240	943004	20.000	ng/ul	0.00
88) Perylene-d12	24.409	264	1058156	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	30060	4.162	ng/uL	0.00
4) Pyridine-d5	3.675	84	425623	20.125	ng/ul	0.00
7) Phenol-d5	6.975	99	455934	20.656	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	307536	19.635	ng/ul	0.00
11) 2-Chlorophenol-d4	7.345	132	375144	23.360	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113	339111	20.664	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	169615	22.706	ng/ul	0.00
24) 2-Nitrophenol-d4	9.687	143	168680	23.563	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	318713	22.287	ng/ul	0.00
31) 4-Chloroaniline-d4	10.733	131	484192	21.901	ng/ul	0.00
46) Dimethylphthalate-d6	13.851	166	936448	23.325	ng/ul	0.00
49) Acenaphthylene-d8	14.139	160	1108102	23.278	ng/ul	0.00
54) 4-Nitrophenol-d4	14.627	143	135533m	16.955	ng/ul	0.00
60) Fluorene-d10	15.433	176	794481	22.846	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.545	200	94530	14.749	ng/ul	0.00
73) Anthracene-d10	17.280	188	1213785	22.538	ng/ul	0.00
81) Pyrene-d10	19.568	212	1314725	24.565	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.203	264	1235649	22.507	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047712.D
Acq On : 30 Sep 2024 11:19
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK375

Manual IntegrationsAPPROVED

Quant Time: Sep 30 11:55:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/01/2024
Supervised By :mohammad ahmed 10/01/2024

