




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047726.D
Acq On : 30 Sep 2024 21:12
Operator : RC/JU
Sample : P4018-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCF5

Manual IntegrationsAPPROVED

Quant Time: Sep 30 23:16:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/01/2024
Supervised By :mohammad ahmed 10/01/2024

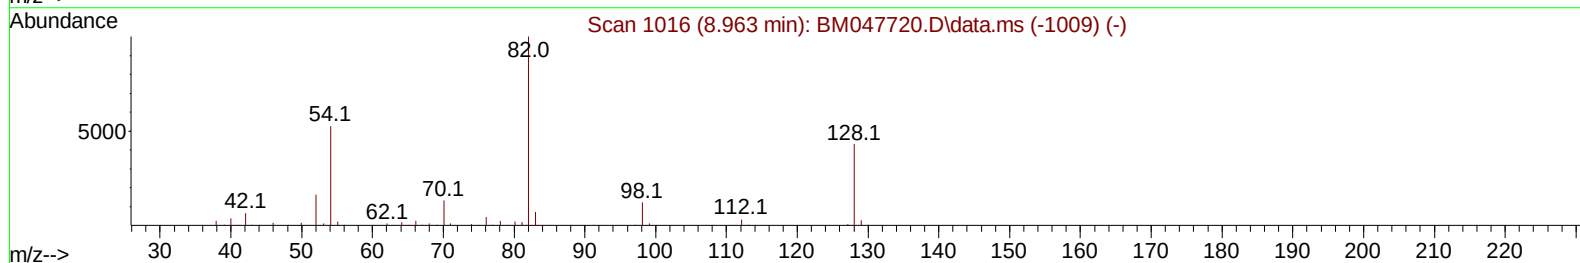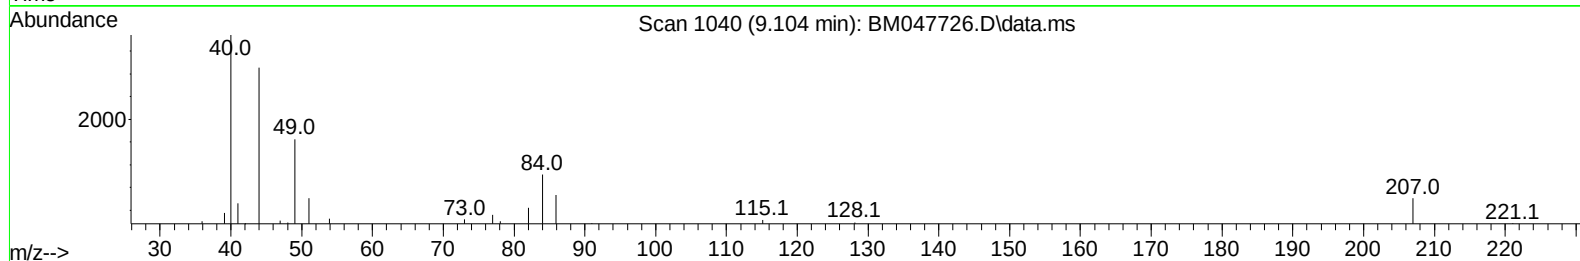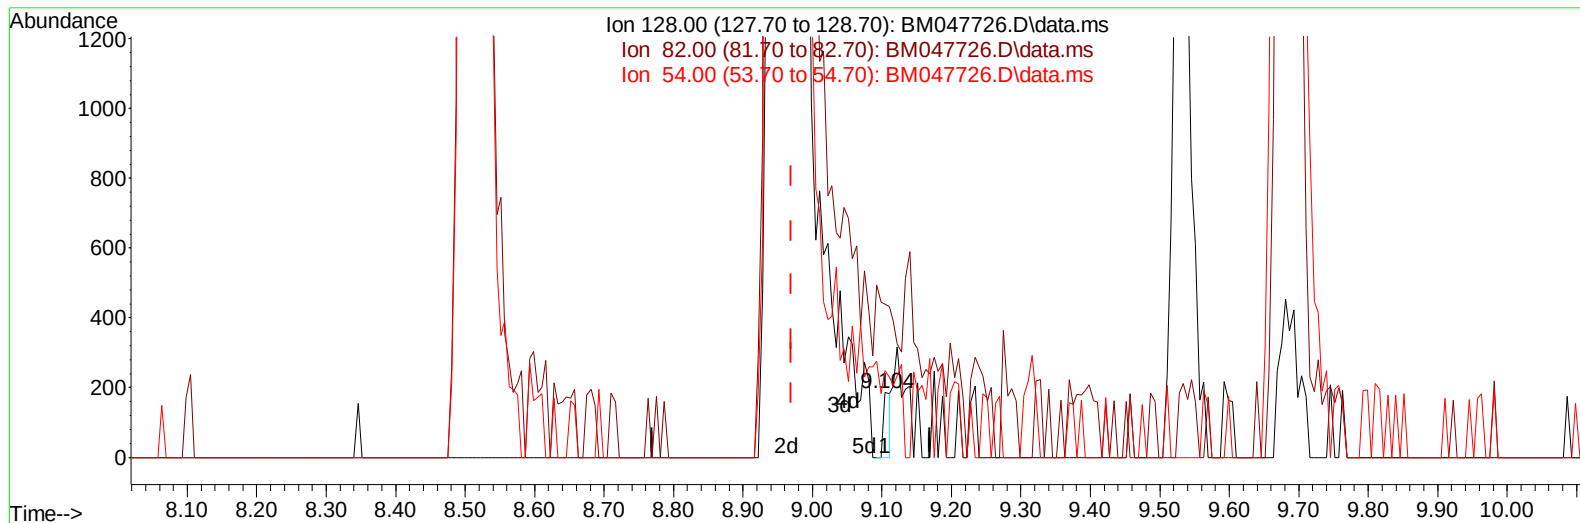

TIC: BM047726.D\data.ms

(21) Nitrobenzene-d5 (S)

9.104min (+ 0.135) 0.02 ng/u1

response 130

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	266.90	236.56
54.00	152.80	133.87
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047726.D
Acq On : 30 Sep 2024 21:12
Operator : RC/JU
Sample : P4018-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCF5

Manual IntegrationsAPPROVED

Quant Time: Sep 30 23:16:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/01/2024
Supervised By :mohammad ahmed 10/01/2024

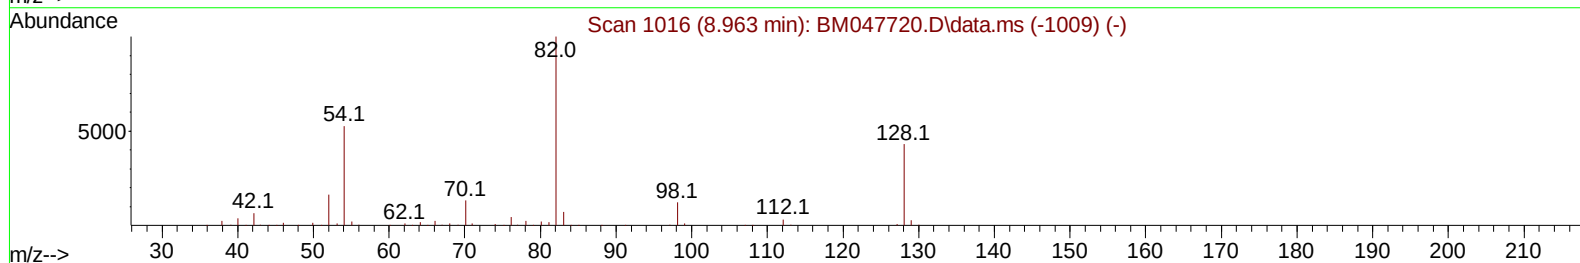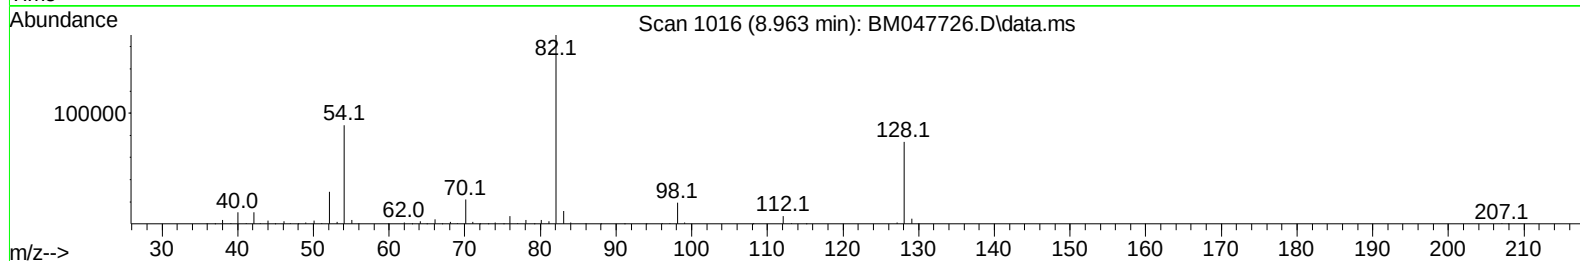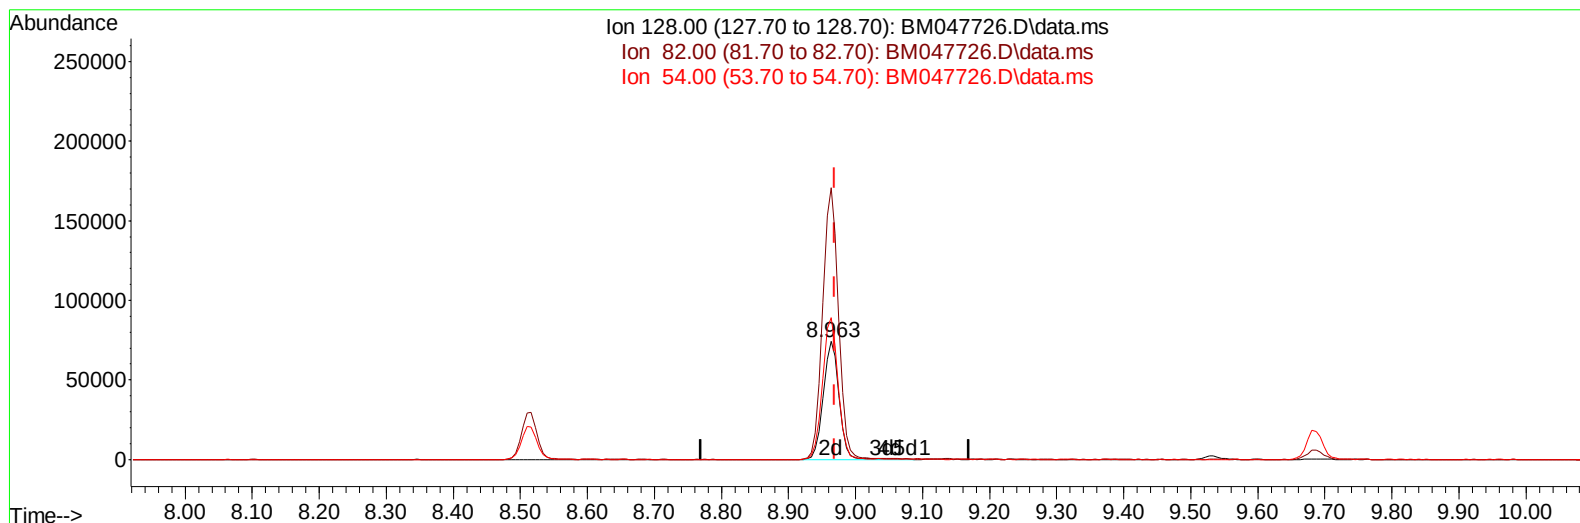

TIC: BM047726.D\data.ms

(21) Nitrobenzene-d5 (S)

8.963min (-0.006) 16.12 ng/ul m

response 120894

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	266.90	230.25
54.00	152.80	120.40#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
 Data File : BM047726.D
 Acq On : 30 Sep 2024 21:12
 Operator : RC/JU
 Sample : P4018-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCF5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/01/2024
 Supervised By :mohammad ahmed 10/01/2024

Quant Time: Sep 30 23:26:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 02:30:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	231876	20.000	ng/ul	0.00
20) Naphthalene-d8	10.604	136	942161	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.445	164	585546	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.180	188	1194057	20.000	ng/ul	0.00
79) Chrysene-d12	21.404	240	1106997	20.000	ng/ul	0.00
88) Perylene-d12	24.403	264	1300768	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	20277	2.826	ng/uL	0.00
4) Pyridine-d5	3.675	84	232621	11.072	ng/ul	0.00
7) Phenol-d5	6.975	99	306014	13.957	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	198742	12.774	ng/ul	0.00
11) 2-Chlorophenol-d4	7.346	132	253604	15.897	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113	249613	15.312	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	120894m	16.116	ng/ul	0.00
24) 2-Nitrophenol-d4	9.687	143	117904	16.401	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	238406	16.602	ng/ul	0.00
31) 4-Chloroaniline-d4	10.734	131	355514	16.013	ng/ul	0.00
46) Dimethylphthalate-d6	13.851	166	776434	18.290	ng/ul	0.00
49) Acenaphthylene-d8	14.134	160	890547	17.693	ng/ul	0.00
54) 4-Nitrophenol-d4	14.633	143	87256	10.323	ng/ul	0.00
60) Fluorene-d10	15.433	176	686136	18.660	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.545	200	60629	8.677	ng/ul	0.00
73) Anthracene-d10	17.280	188	1067369	18.179	ng/ul	0.00
81) Pyrene-d10	19.563	212	1225887	19.512	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.198	264	1278009	18.936	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047726.D
Acq On : 30 Sep 2024 21:12
Operator : RC/JU
Sample : P4018-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCF5

Manual IntegrationsAPPROVED

Quant Time: Sep 30 23:26:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/01/2024
Supervised By :mohammad ahmed 10/01/2024

