




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047729.D
Acq On : 30 Sep 2024 23:10
Operator : RC/JU
Sample : P4018-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCB8

Manual IntegrationsAPPROVED

Quant Time: Oct 01 00:26:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/01/2024
Supervised By :mohammad ahmed 10/01/2024

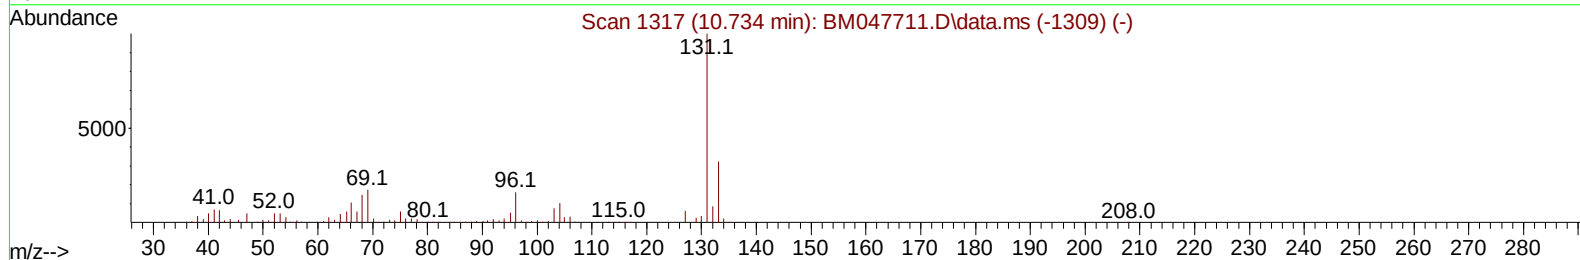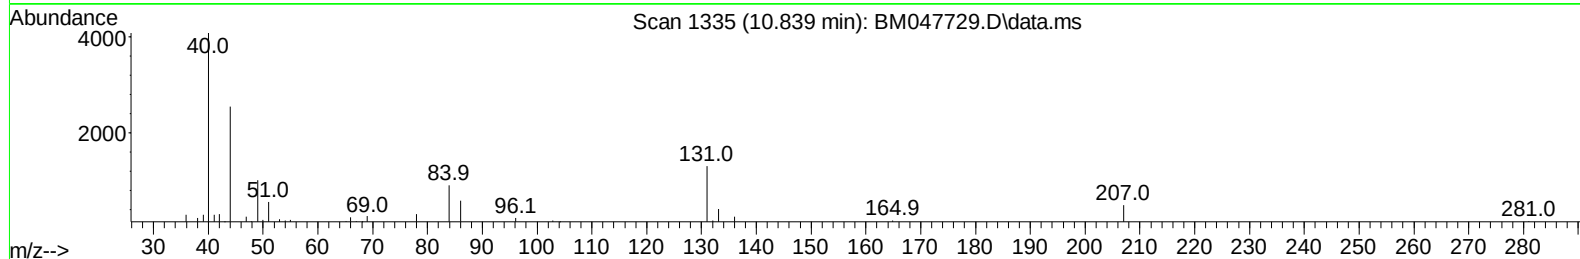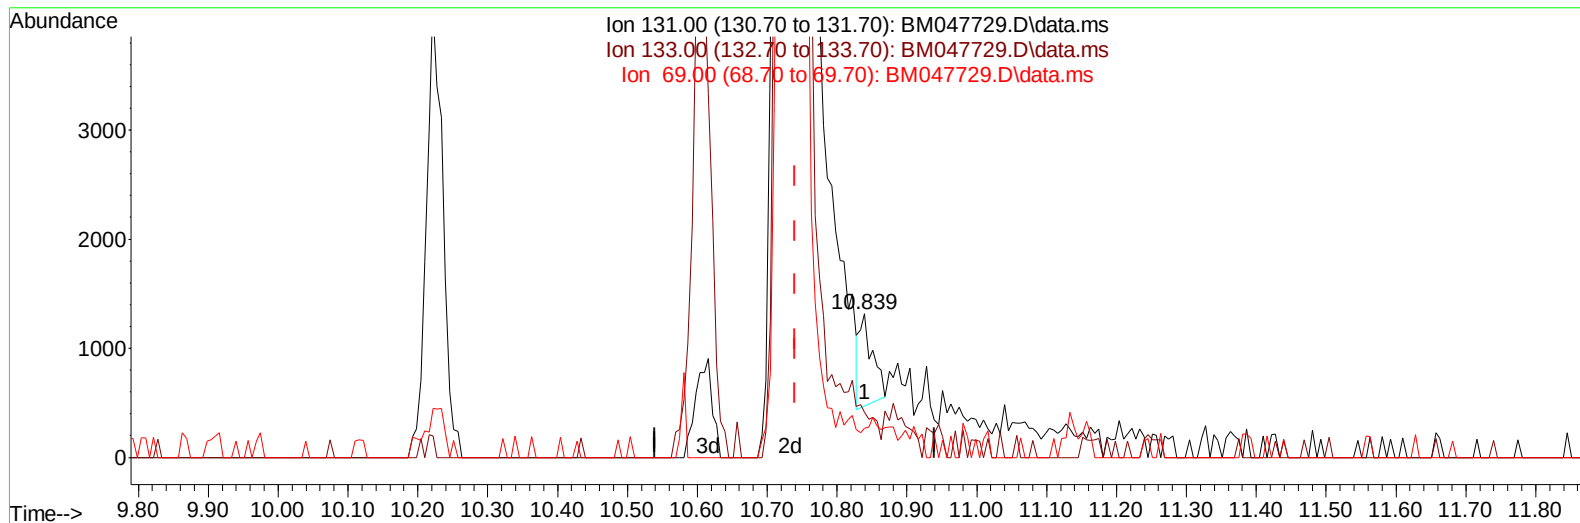

TIC: BM047729.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.839min (+ 0.100) 0.04 ng/u1

response 1088

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	34.00	31.36
69.00	20.90	20.35
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047729.D
Acq On : 30 Sep 2024 23:10
Operator : RC/JU
Sample : P4018-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCB8

Manual IntegrationsAPPROVED

Quant Time: Oct 01 00:26:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/01/2024
Supervised By :mohammad ahmed 10/01/2024

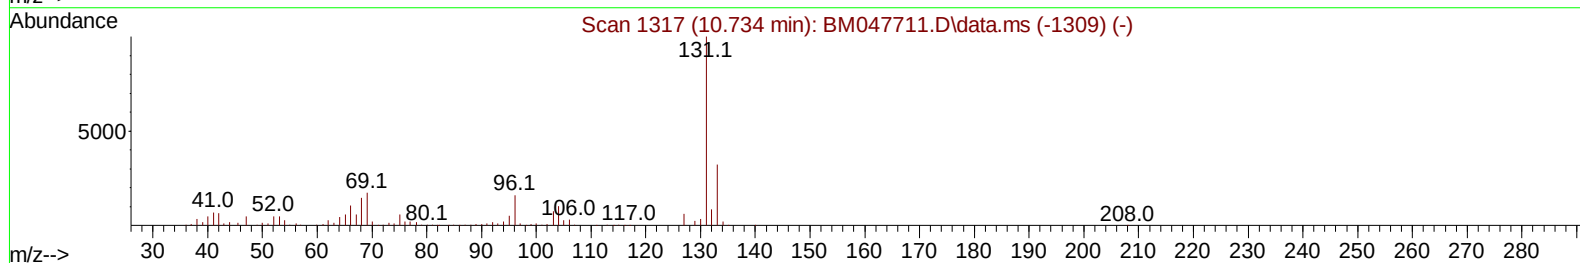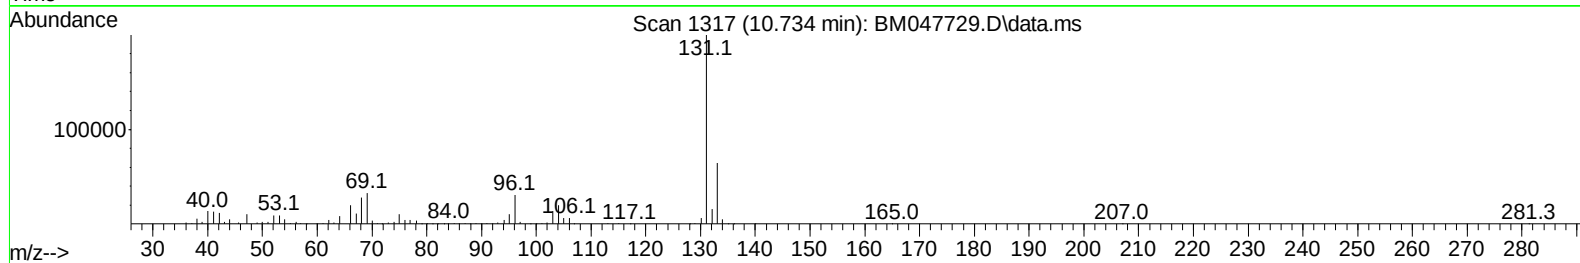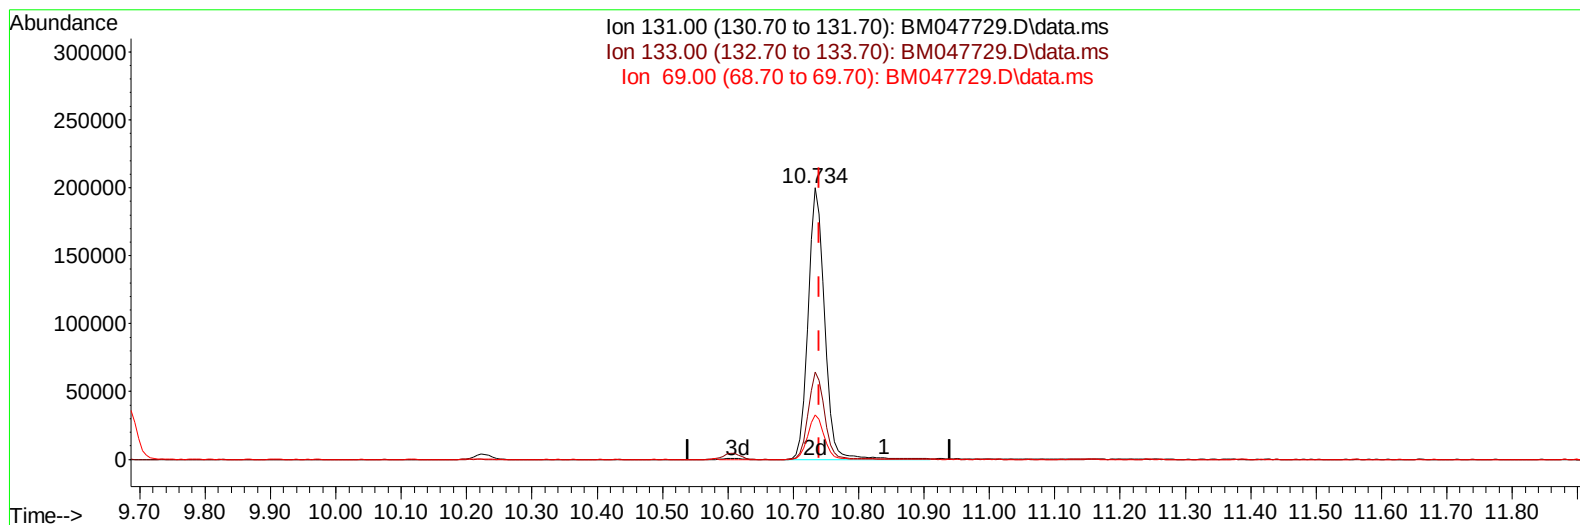

TIC: BM047729.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.734min (-0.006) 13.79 ng/ul m

response 350771

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	34.00	32.24
69.00	20.90	16.43#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
 Data File : BM047729.D
 Acq On : 30 Sep 2024 23:10
 Operator : RC/JU
 Sample : P4018-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCB8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/01/2024
 Supervised By :mohammad ahmed 10/01/2024

Quant Time: Oct 01 00:30:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 02:30:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	266281	20.000	ng/ul	0.00
20) Naphthalene-d8	10.604	136	1079673	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.445	164	668492	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.180	188	1339924	20.000	ng/ul	0.00
79) Chrysene-d12	21.403	240	1243261	20.000	ng/ul	0.00
88) Perylene-d12	24.409	264	1438940	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	16567	2.011	ng/uL	0.00
4) Pyridine-d5	3.675	84	230386	9.549	ng/ul	0.00
7) Phenol-d5	6.975	99	280657	11.146	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	190871	10.683	ng/ul	0.00
11) 2-Chlorophenol-d4	7.346	132	234362	12.793	ng/ul	0.00
15) 4-Methylphenol-d8	8.510	113	234622	12.533	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	114949	13.372	ng/ul	0.00
24) 2-Nitrophenol-d4	9.687	143	113375	13.763	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	221121	13.437	ng/ul	0.00
31) 4-Chloroaniline-d4	10.734	131	350771m	13.787	ng/ul	0.00
46) Dimethylphthalate-d6	13.851	166	736120	15.188	ng/ul	0.00
49) Acenaphthylene-d8	14.139	160	849401	14.781	ng/ul	0.00
54) 4-Nitrophenol-d4	14.633	143	28440	2.947	ng/ul	0.00
60) Fluorene-d10	15.433	176	637709	15.191	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.545	200	18738	2.390	ng/ul	0.00
73) Anthracene-d10	17.280	188	987771	14.992	ng/ul	0.00
81) Pyrene-d10	19.562	212	1150612	16.307	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.197	264	1173650	15.720	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047729.D
Acq On : 30 Sep 2024 23:10
Operator : RC/JU
Sample : P4018-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCB8

Manual IntegrationsAPPROVED

Quant Time: Oct 01 00:30:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/01/2024
Supervised By :mohammad ahmed 10/01/2024

