

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
 Data File : BM047712.D
 Acq On : 30 Sep 2024 11:19
 Operator : RC/JU
 Sample : PB163375BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK375

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047712.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	42	46	52	rBV	67105	83544	2.43%	0.184%
2	3.669	112	116	136	rBV	794310	1225220	35.67%	2.704%
3	4.005	170	173	180	rVB3	16436	23029	0.67%	0.051%
4	5.787	475	476	482	rBV6	2927	3952	0.12%	0.009%
5	6.975	671	678	690	rVV	836558	1307249	38.06%	2.885%
6	7.140	700	706	716	rVB	689882	1071144	31.18%	2.364%
7	7.345	733	741	750	rBV	850447	1344746	39.15%	2.968%
8	7.681	795	798	802	rVB6	3045	5772	0.17%	0.013%
9	7.810	813	820	830	rBV	865621	1390099	40.47%	3.068%
10	8.516	932	940	954	rBV	936162	1532909	44.63%	3.383%
11	8.963	1007	1016	1030	rBV	768264	1259639	36.67%	2.780%
12	9.234	1059	1062	1066	rVB5	3519	4260	0.12%	0.009%
13	9.687	1129	1139	1150	rBV	563038	931563	27.12%	2.056%
14	10.222	1223	1230	1242	rBV	880466	1490101	43.38%	3.288%
15	10.328	1247	1248	1253	rVB3	3085	3435	0.10%	0.008%
16	10.604	1288	1295	1304	rBV	1140029	1915153	55.76%	4.226%
17	10.734	1308	1317	1333	rBV	902517	1592777	46.37%	3.515%
18	10.969	1356	1357	1362	rVB3	3040	3975	0.12%	0.009%
19	12.192	1559	1565	1572	rBV3	13921	25673	0.75%	0.057%
20	12.416	1599	1603	1605	rVB4	3055	3501	0.10%	0.008%
21	13.610	1803	1806	1810	rBV6	2545	3555	0.10%	0.008%
22	13.851	1841	1847	1857	rBV	1502598	2042941	59.48%	4.508%
23	14.139	1889	1896	1910	rBV	1724729	2550689	74.26%	5.629%
24	14.445	1940	1948	1956	rBV	1691161	2411750	70.21%	5.322%
25	14.627	1974	1979	1993	rBV	600575	955385	27.81%	2.108%
26	15.433	2109	2116	2129	rBV	2083794	3003682	87.45%	6.629%
27	15.545	2129	2135	2143	rBV	564109	758266	22.08%	1.673%
28	15.668	2151	2156	2163	rVB7	7724	15279	0.44%	0.034%
29	16.004	2210	2213	2217	rVB5	2202	3596	0.10%	0.008%
30	16.627	2315	2319	2322	rBV3	2570	3673	0.11%	0.008%
31	16.963	2371	2376	2377	rBV5	2787	3965	0.12%	0.009%
32	17.180	2407	2413	2423	rBV	1917014	2689231	78.29%	5.935%
33	17.280	2423	2430	2445	rVV	2286903	3144837	91.56%	6.940%
34	18.080	2563	2566	2567	rBV3	3890	3746	0.11%	0.008%
35	18.904	2704	2706	2707	rBV2	4443	3496	0.10%	0.008%
36	19.133	2741	2745	2750	rBV5	23754	36228	1.05%	0.080%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047712.D
Acq On : 30 Sep 2024 11:19
Operator : RC/JU
Sample : PB163375BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK375

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	19.198	2754	2756	2762	rVB	18442	25772	0.75%	0.057%
38	19.568	2813	2819	2832	rBV	2557422	3434877	100.00%	7.580%
39	21.403	3126	3131	3140	rBV	1838775	2699834	78.60%	5.958%
40	24.203	3599	3607	3622	rVB2	1342620	3309308	96.34%	7.303%
41	24.409	3634	3642	3659	rVB	1158783	2995823	87.22%	6.611%




Sum of corrected areas: 45313674

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047712.D
Acq On : 30 Sep 2024 11:19
Operator : RC/JU
Sample : PB163375BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK375

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

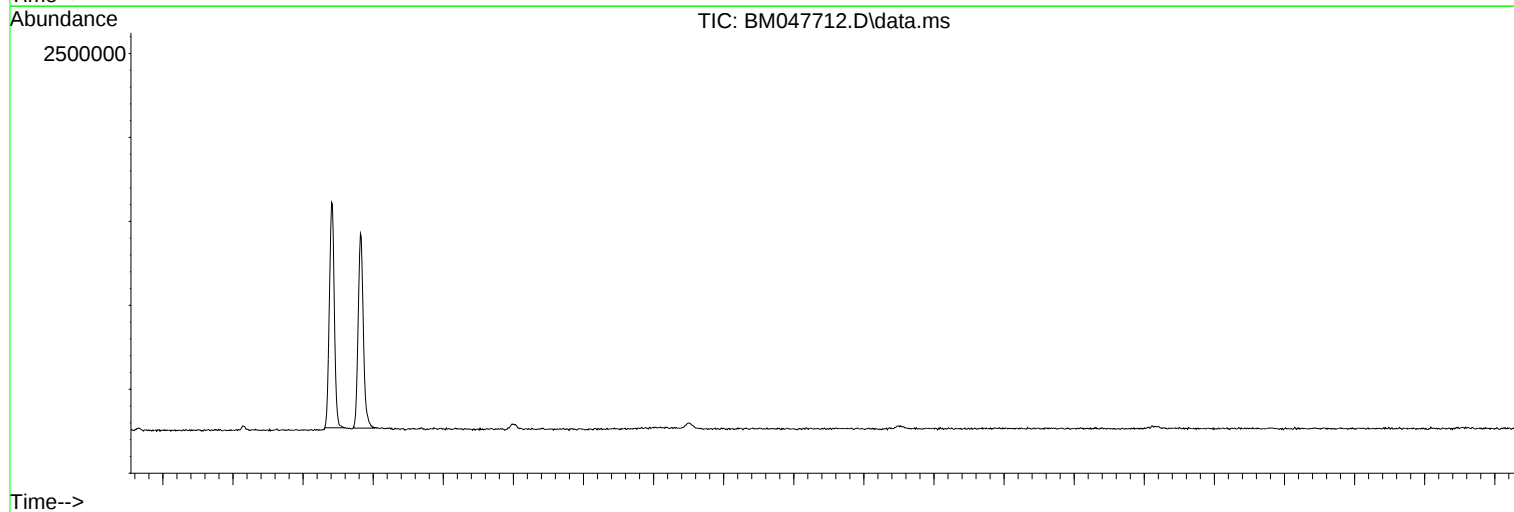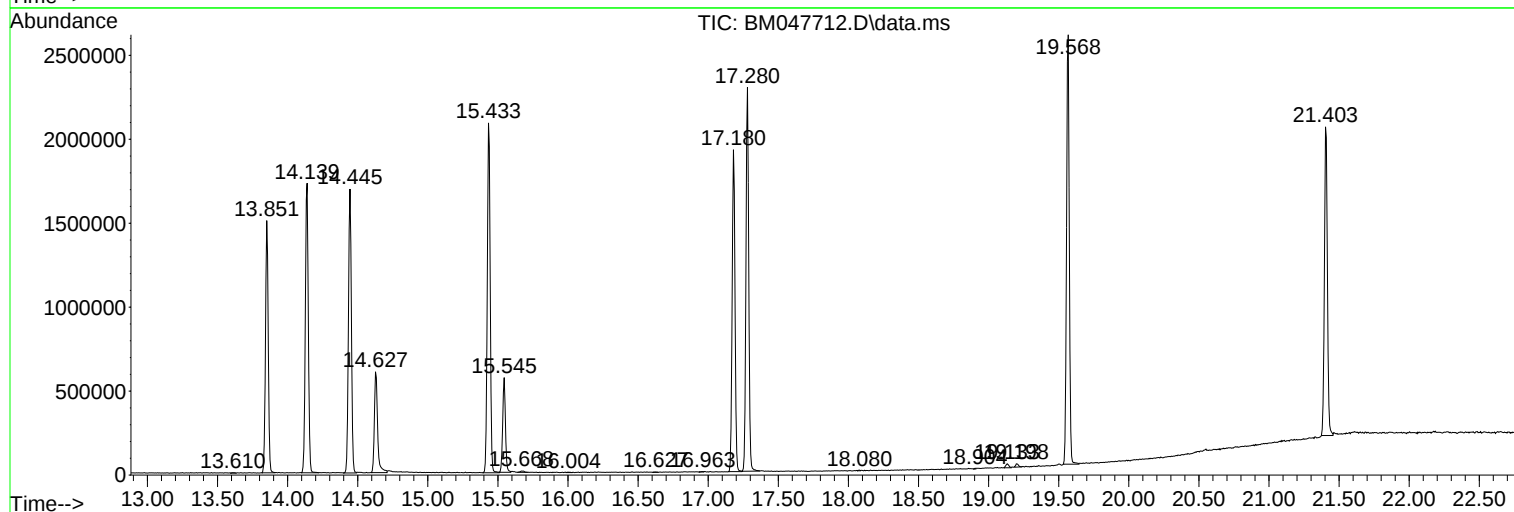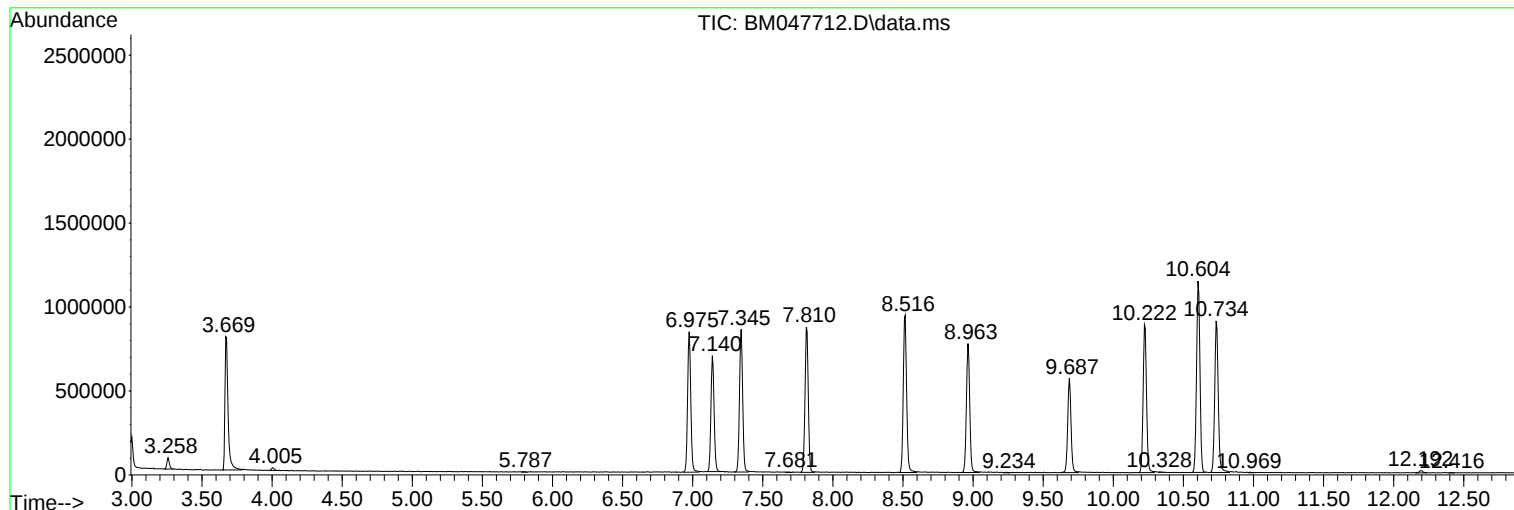

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047712.D
Acq On : 30 Sep 2024 11:19
Operator : RC/JU
Sample : PB163375BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK375

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047712.D
Acq On : 30 Sep 2024 11:19
Operator : RC/JU
Sample : PB163375BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK375

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc