

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
 Data File : BM047721.D
 Acq On : 30 Sep 2024 17:54
 Operator : RC/JU
 Sample : PB163513BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK513

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047721.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	42	46	54	rVB	73420	100114	2.19%	0.180%
2	3.675	112	117	131	rBV	907597	1382277	30.24%	2.490%
3	4.005	169	173	180	rVB3	19364	28971	0.63%	0.052%
4	4.593	270	273	276	rBV4	3705	5177	0.11%	0.009%
5	6.975	671	678	693	rBV	957673	1490994	32.62%	2.686%
6	7.140	697	706	717	rVV	783748	1208149	26.43%	2.176%
7	7.346	734	741	755	rVB	975520	1522946	33.31%	2.743%
8	7.810	813	820	832	rBV	978104	1579769	34.56%	2.846%
9	8.516	932	940	949	rBV	1113639	1789923	39.15%	3.224%
10	8.963	1007	1016	1026	rBV	884560	1429856	31.28%	2.576%
11	9.281	1066	1070	1076	rVB5	2640	4929	0.11%	0.009%
12	9.687	1127	1139	1151	rBV	673935	1123453	24.58%	2.024%
13	9.816	1159	1161	1168	rVB6	3605	5807	0.13%	0.010%
14	10.222	1223	1230	1248	rBV	1070049	1797307	39.32%	3.237%
15	10.604	1288	1295	1307	rBV	1336352	2249550	49.21%	4.052%
16	10.734	1310	1317	1330	rBV	1070196	1853452	40.54%	3.339%
17	10.816	1330	1331	1336	rVB4	6384	6896	0.15%	0.012%
18	12.198	1560	1566	1573	rVB2	17398	32836	0.72%	0.059%
19	13.851	1841	1847	1857	rBV	1714196	2378659	52.03%	4.285%
20	14.139	1888	1896	1908	rBV	2042679	3060007	66.94%	5.512%
21	14.445	1941	1948	1957	rBV	2011088	2907414	63.60%	5.237%
22	14.533	1960	1963	1967	rVB4	4029	4696	0.10%	0.008%
23	14.633	1973	1980	1999	rBV	737362	1193785	26.11%	2.150%
24	15.433	2110	2116	2125	rBV	2550839	3605604	78.87%	6.495%
25	15.545	2129	2135	2144	rVV	673342	927938	20.30%	1.671%
26	15.621	2146	2148	2153	rVV6	4048	7565	0.17%	0.014%
27	15.674	2153	2157	2161	rVB2	13547	16467	0.36%	0.030%
28	16.833	2350	2354	2357	rBV6	8893	10540	0.23%	0.019%
29	16.968	2375	2377	2382	rVB5	5201	7793	0.17%	0.014%
30	17.180	2407	2413	2423	rVV	2358855	3281873	71.79%	5.911%
31	17.280	2423	2430	2441	rVV	2709778	3817732	83.51%	6.877%
32	18.074	2563	2565	2569	rVB5	7172	8566	0.19%	0.015%
33	18.210	2584	2588	2590	rBV5	5338	7921	0.17%	0.014%
34	19.133	2741	2745	2748	rBV2	33682	47921	1.05%	0.086%
35	19.204	2752	2757	2760	rBV	32693	46805	1.02%	0.084%
36	19.562	2812	2818	2826	rBV	3204443	4349767	95.15%	7.835%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047721.D
Acq On : 30 Sep 2024 17:54
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK513

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	21.403	3125	3131	3140	rBV2	2376380	3524680	77.10%	6.349%
38	24.203	3598	3607	3618	rBV2	1874017	4571429	100.00%	8.234%
39	24.409	3634	3642	3657	rVB	1526595	4127199	90.28%	7.434%




Sum of corrected areas: 55516767

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047721.D
Acq On : 30 Sep 2024 17:54
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

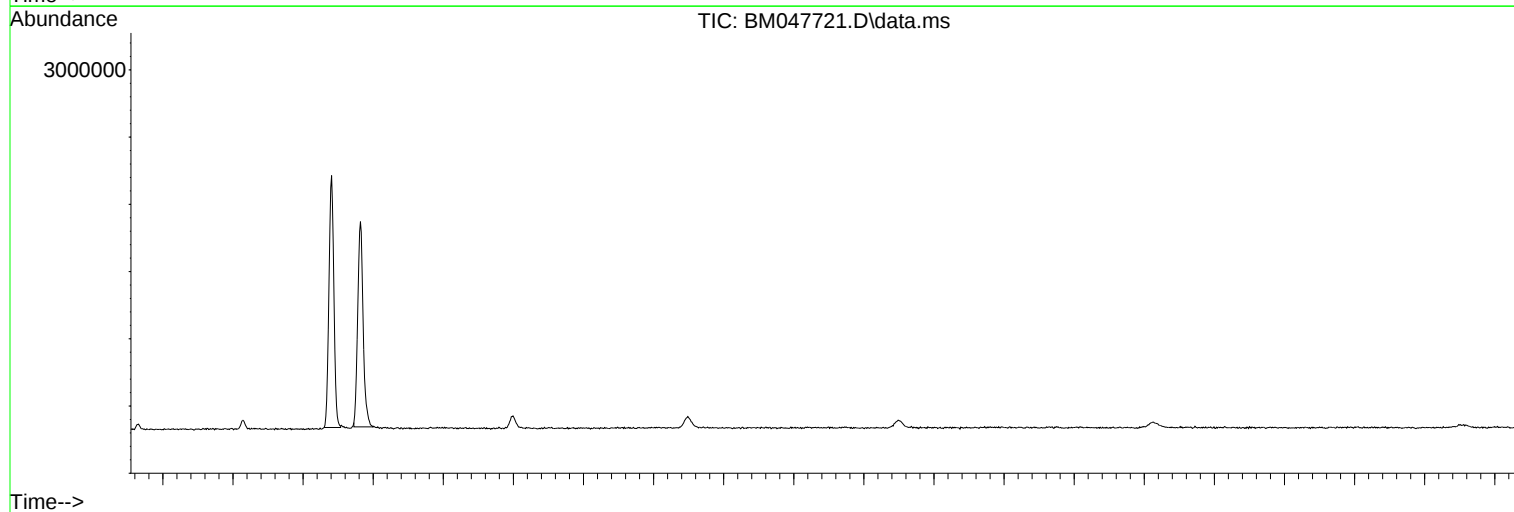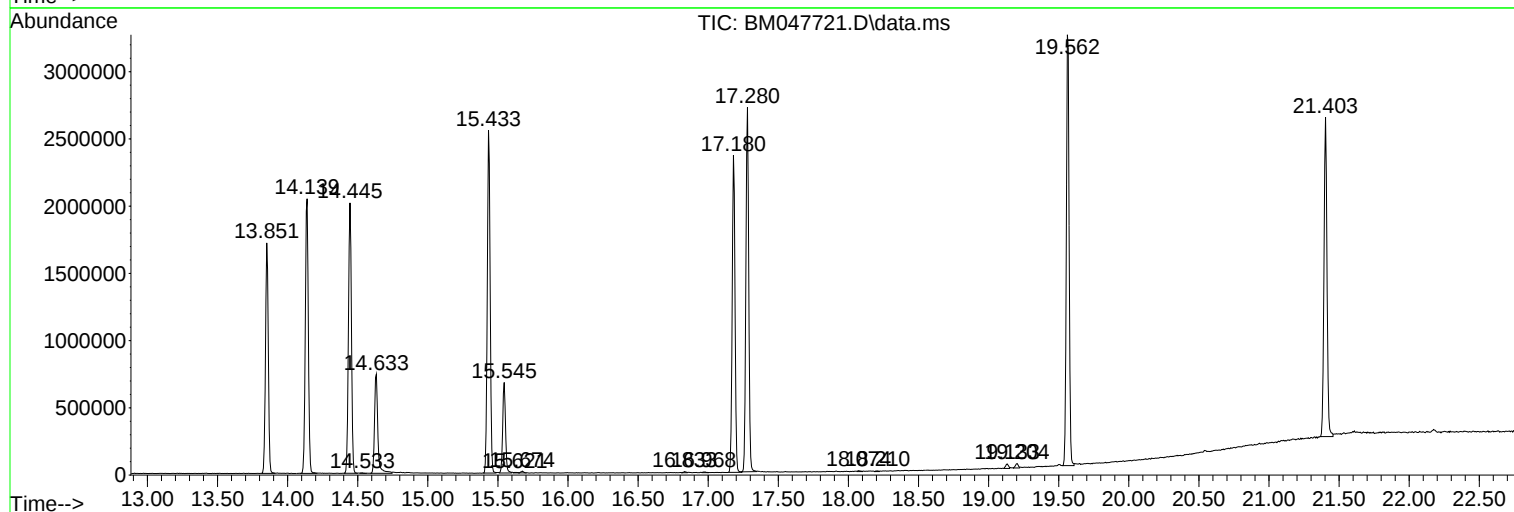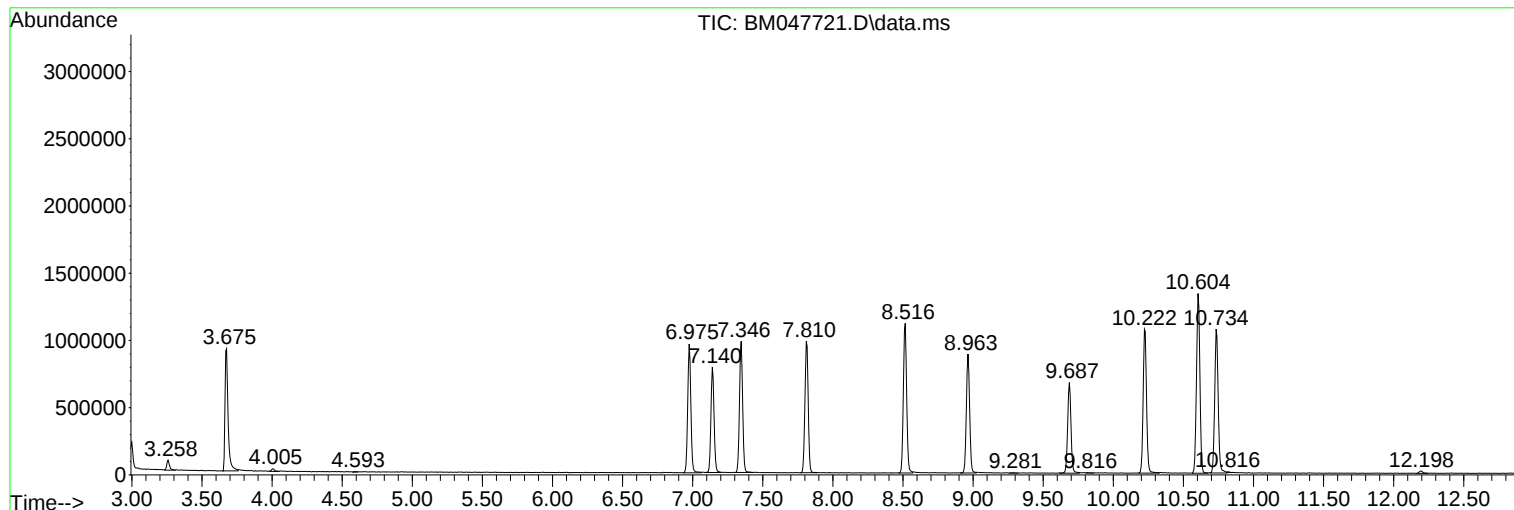

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047721.D
Acq On : 30 Sep 2024 17:54
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM093024\
Data File : BM047721.D
Acq On : 30 Sep 2024 17:54
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------