

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM100115\
 Data File : BM002819.D
 Acq On : 02 Oct 2015 00:27
 Operator : UM/IZ
 Sample : G3839-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC2W5

Quant Time: Oct 02 06:03:39 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 05:57:21 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.69	152	70121	20.00	ng/ul	0.00
18) Naphthalene-d8	11.55	136	294880	20.00	ng/ul	0.00
36) Acenaphthene-d10	15.28	164	150521	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.99	188	306829	20.00	ng/ul	0.00
78) Chrysene-d12	22.08	240	335186	20.00	ng/ul	0.00
86) Perylene-d12	24.66	264	342108	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.76	96	7027	4.65	ng/uL	0.00
5) Phenol-d5	7.80	99	135630	25.53	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.97	67	76578	25.62	ng/ul	0.00
9) 2-Chlorophenol-d4	8.20	132	126365	25.55	ng/ul	0.00
13) 4-Methylphenol-d8	9.39	113	114193	26.07	ng/ul	0.00
19) Nitrobenzene-d5	9.88	128	57983	25.78	ng/ul	0.00
22) 2-Nitrophenol-d4	10.61	143	60592	25.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	11.15	165	102279	24.66	ng/ul	0.00
29) 4-Chloroaniline-d4	11.67	131	124720	24.98	ng/ul	0.00
44) Dimethylphthalate-d6	14.66	166	307603	27.16	ng/ul	0.00
47) Acenaphthylene-d8	14.99	160	398087	26.34	ng/ul	0.00
52) 4-Nitrophenol-d4	15.46	143	48684	24.21	ng/ul	0.00
58) Fluorene-d10	16.26	176	265616	26.04	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	16.38	200	26680	17.83	ng/ul	0.00
71) Anthracene-d10	18.09	188	405094	27.66	ng/ul	0.00
79) Pyrene-d10	20.32	212	422286	26.99	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.50	264	484223	27.67	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.70	163	150988	13.12	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM100115\
Data File : BM002819.D
Acq On : 02 Oct 2015 00:27
Operator : UM/IZ
Sample : G3839-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC2W5

Quant Time: Oct 02 06:03:39 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092915.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 05:57:21 2015
Response via : Initial Calibration

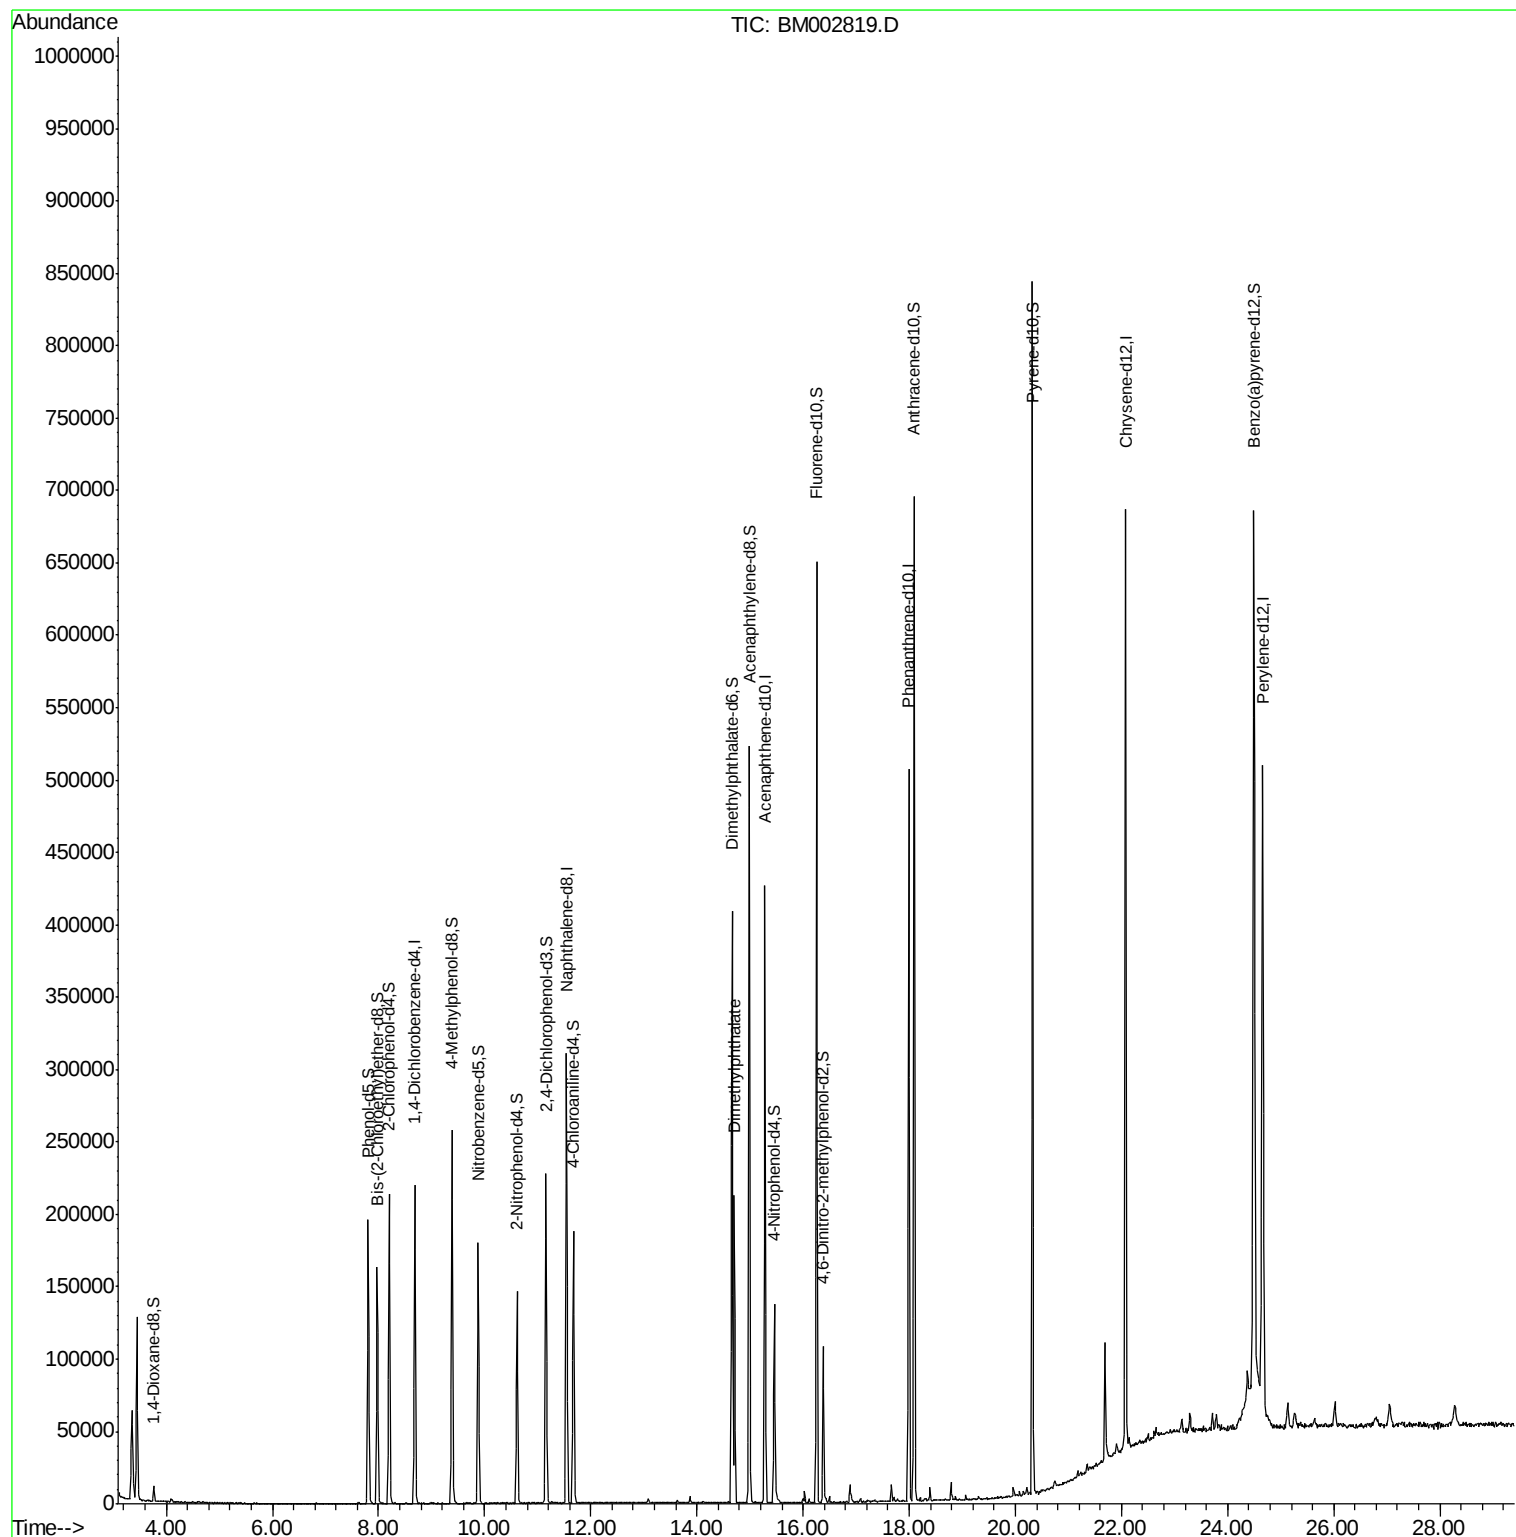

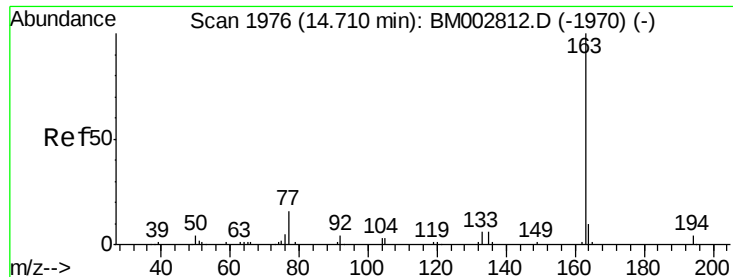

#45

Dimethylphthalate

Concen: 13.12 ng/ul

RT: 14.70 min Scan# 1975

Delta R.T. -0.01 min

Lab File: BM002819.D


Acq: 02 Oct 2015 00:27

Instrument :

BNA_M

ClientSampleId :

BC2W5

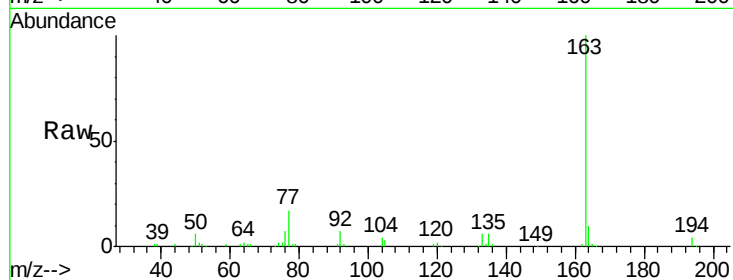


Tgt Ion:163 Resp: 150988

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 9.8 8.1 12.1

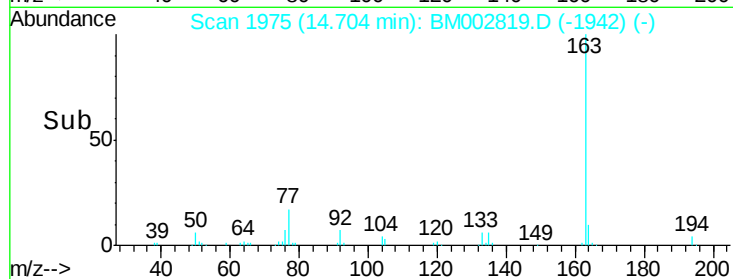

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

