

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM100115\
 Data File : BM002820.D
 Acq On : 02 Oct 2015 01:03
 Operator : UM/IZ
 Sample : G3800-19
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C03H6

Quant Time: Oct 02 06:03:48 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 05:57:21 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.69	152	75259	20.00	ng/ul	0.00
18) Naphthalene-d8	11.55	136	316972	20.00	ng/ul	0.00
36) Acenaphthene-d10	15.28	164	166394	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.99	188	349615	20.00	ng/ul	0.00
78) Chrysene-d12	22.08	240	381009	20.00	ng/ul	0.00
86) Perylene-d12	24.66	264	384883	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.76	96	2214	1.37	ng/uL	0.00
5) Phenol-d5	7.80	99	44702	7.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.98	67	91333	28.47	ng/ul	0.00
9) 2-Chlorophenol-d4	8.20	132	131169	24.71	ng/ul	0.00
13) 4-Methylphenol-d8	9.39	113	82192	17.48	ng/ul	0.00
19) Nitrobenzene-d5	9.88	128	72717	30.08	ng/ul	0.00
22) 2-Nitrophenol-d4	10.61	143	75384	29.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	11.15	165	122348	27.44	ng/ul	0.00
29) 4-Chloroaniline-d4	11.67	131	25934	4.83	ng/ul	0.00
44) Dimethylphthalate-d6	14.66	166	390118	31.16	ng/ul	0.00
47) Acenaphthylene-d8	14.99	160	501662	30.03	ng/ul	0.00
52) 4-Nitrophenol-d4	15.46	143	15655	7.04	ng/ul	0.00
58) Fluorene-d10	16.26	176	335583	29.76	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	16.38	200	41913	24.58	ng/ul	0.00
71) Anthracene-d10	18.09	188	502810	30.13	ng/ul	0.00
79) Pyrene-d10	20.32	212	530525	29.83	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.50	264	601705	30.56	ng/ul	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.45	88	4096	2.29	ng/uL#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM100115\
Data File : BM002820.D
Acq On : 02 Oct 2015 01:03
Operator : UM/IZ
Sample : G3800-19
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C03H6

Quant Time: Oct 02 06:03:48 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092915.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 05:57:21 2015
Response via : Initial Calibration

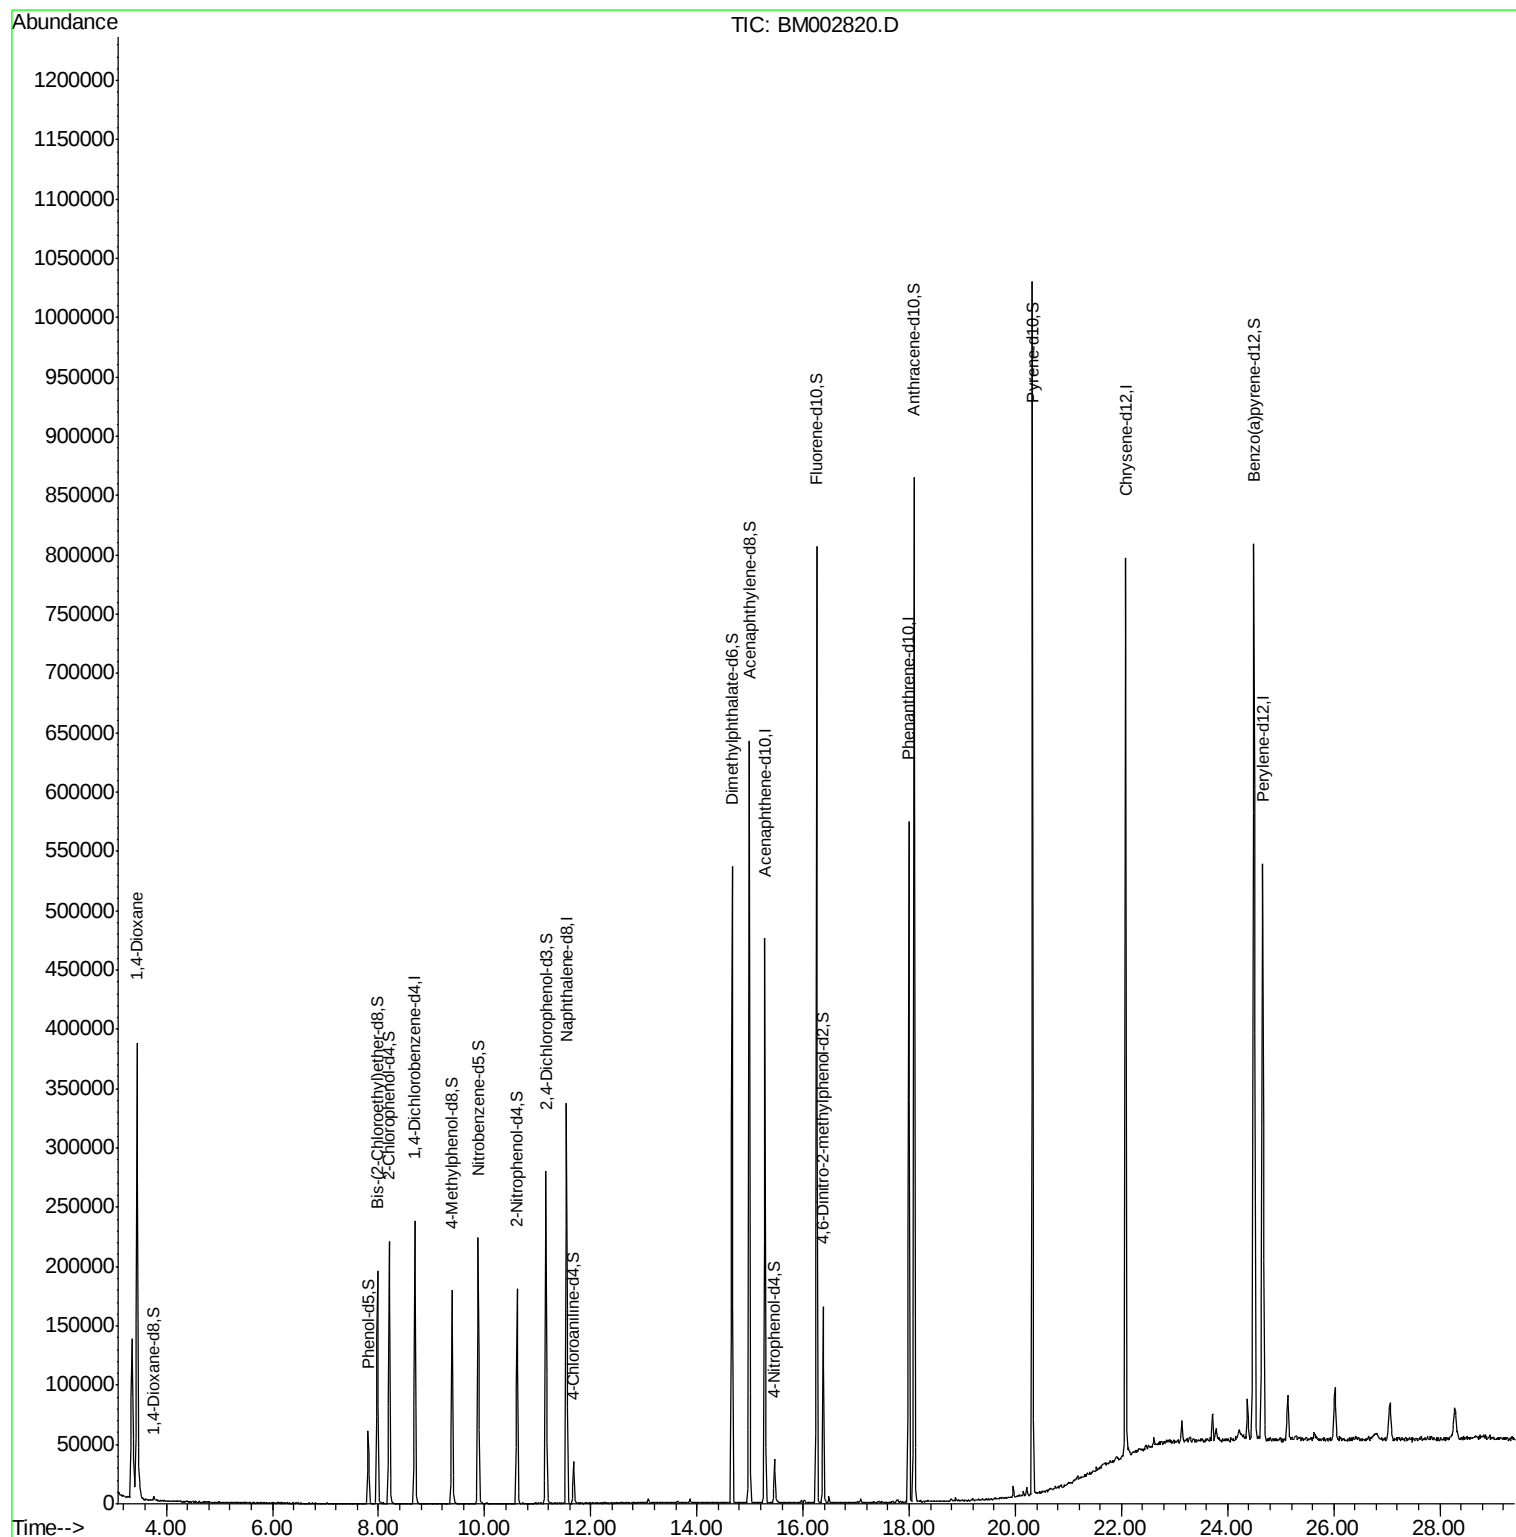

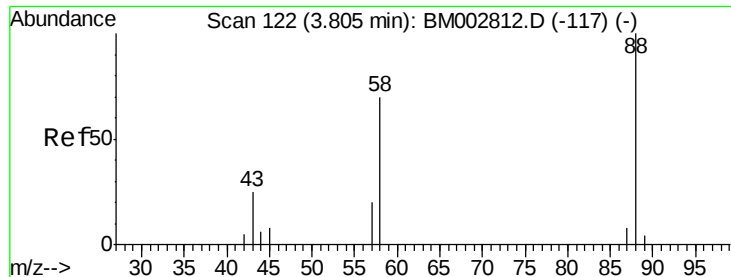

#2
 1,4-Dioxane
 Concen: 2.29 ng/uL
 RT: 3.45 min Scan# 61
 Delta R.T. -0.36 min
 Lab File: BM002820.D
 Acq: 02 Oct 2015 01:03

Instrument :
 BNA_M
 ClientSampleId :
 C03H6

Tgt Ion: 88 Resp: 4096
 Ion Ratio Lower Upper
 88 100
 43 2374.3 26.2 39.4#
 58 15.6 58.5 87.7#

