

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM100115\
 Data File : BM002818.D
 Acq On : 01 Oct 2015 23:51
 Operator : UM/IZ
 Sample : G3839-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC2W6

Quant Time: Oct 02 05:59:07 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 05:57:21 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.69	152	65734	20.00	ng/ul	0.00
18) Naphthalene-d8	11.55	136	276930	20.00	ng/ul	0.00
36) Acenaphthene-d10	15.28	164	143567	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.99	188	301031	20.00	ng/ul	0.00
78) Chrysene-d12	22.08	240	332411	20.00	ng/ul	0.00
86) Perylene-d12	24.66	264	338198	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.76	96	4562	3.22	ng/uL	0.00
5) Phenol-d5	7.80	99	85964	17.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.98	67	49927	17.82	ng/ul	0.00
9) 2-Chlorophenol-d4	8.20	132	81073	17.49	ng/ul	0.00
13) 4-Methylphenol-d8	9.39	113	73140	17.81	ng/ul	0.00
19) Nitrobenzene-d5	9.88	128	36591	17.33	ng/ul	0.00
22) 2-Nitrophenol-d4	10.61	143	37951	17.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	11.16	165	63823	16.39	ng/ul	0.00
29) 4-Chloroaniline-d4	11.67	131	77732	16.58	ng/ul	0.00
44) Dimethylphthalate-d6	14.66	166	200789	18.59	ng/ul	0.00
47) Acenaphthylene-d8	14.99	160	258426	17.93	ng/ul	0.00
52) 4-Nitrophenol-d4	15.46	143	26963	14.06	ng/ul	0.00
58) Fluorene-d10	16.26	176	173266	17.81	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	16.38	200	13534	9.22	ng/ul	0.00
71) Anthracene-d10	18.09	188	261870	18.23	ng/ul	0.00
79) Pyrene-d10	20.32	212	276193	17.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.50	264	316657	18.30	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.70	163	103679	9.44	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM100115\
Data File : BM002818.D
Acq On : 01 Oct 2015 23:51
Operator : UM/IZ
Sample : G3839-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC2W6

Quant Time: Oct 02 05:59:07 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092915.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 05:57:21 2015
Response via : Initial Calibration

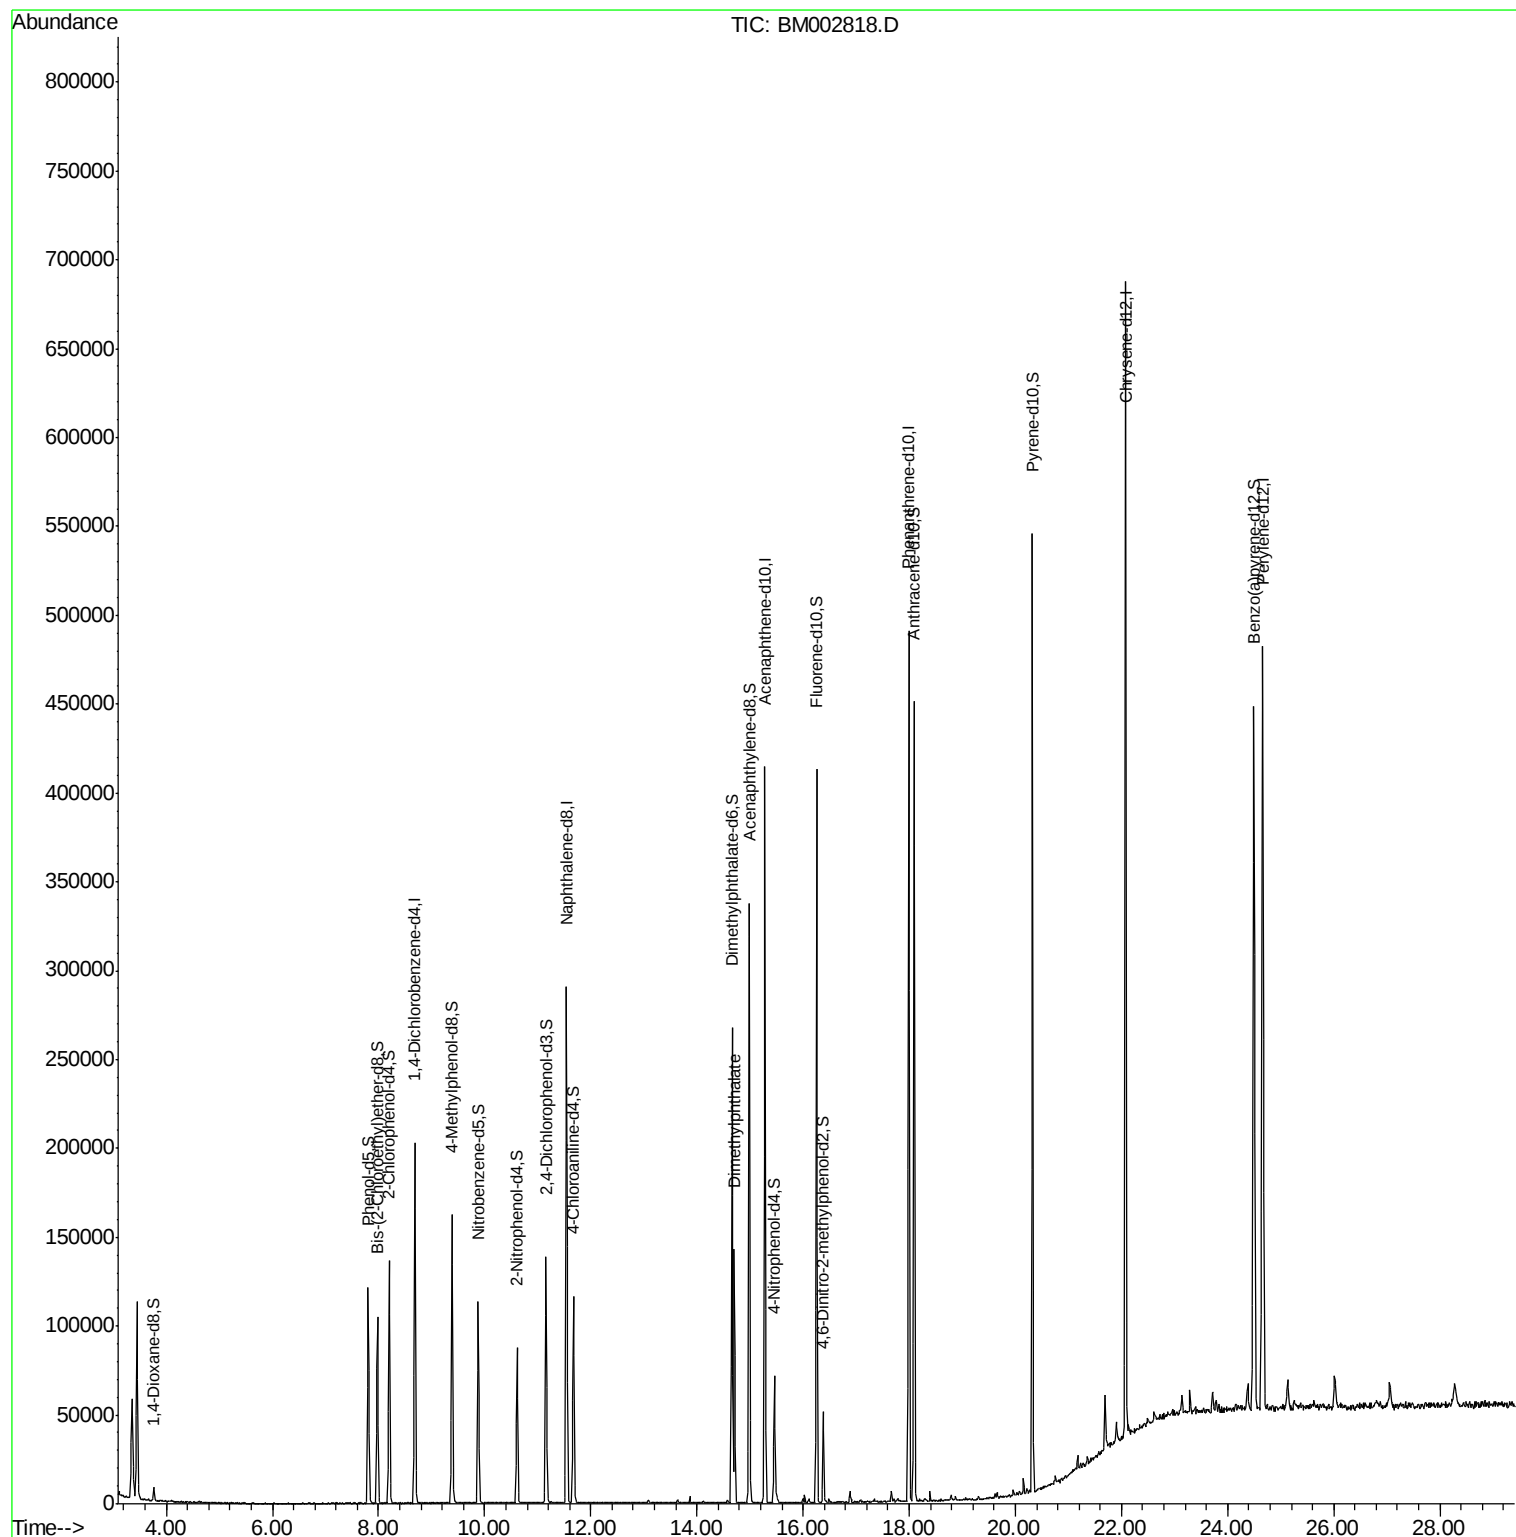

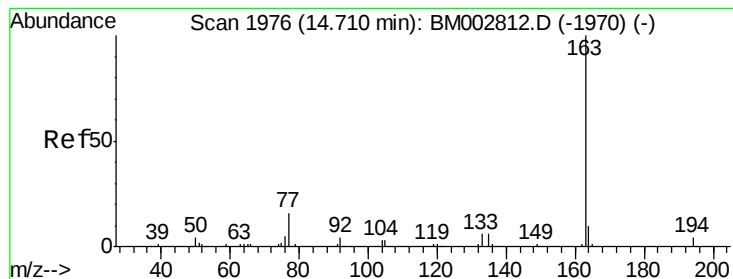

#45

Dimethylphthalate

Concen: 9.44 ng/ul

RT: 14.70 min Scan# 1975

Delta R.T. -0.01 min

Lab File: BM002818.D


Acq: 01 Oct 2015 23:51

Instrument :

BNA_M

ClientSampleId :

BC2W6

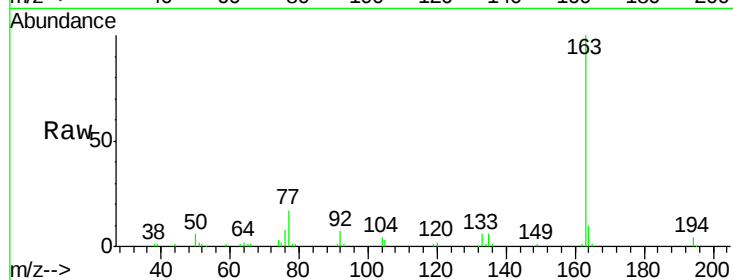

Tgt Ion:	163	Resp:	103679
Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.2	4.8
164	10.0	8.1	12.1

