


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM100115\
Data File : BM002802.D
Acq On : 01 Oct 2015 10:07
Operator : UM/IZ
Sample : DFTPP19
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP19

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092915.M
Title : SVOA CALIBRATION
Last Update : Fri Oct 02 05:57:21 2015

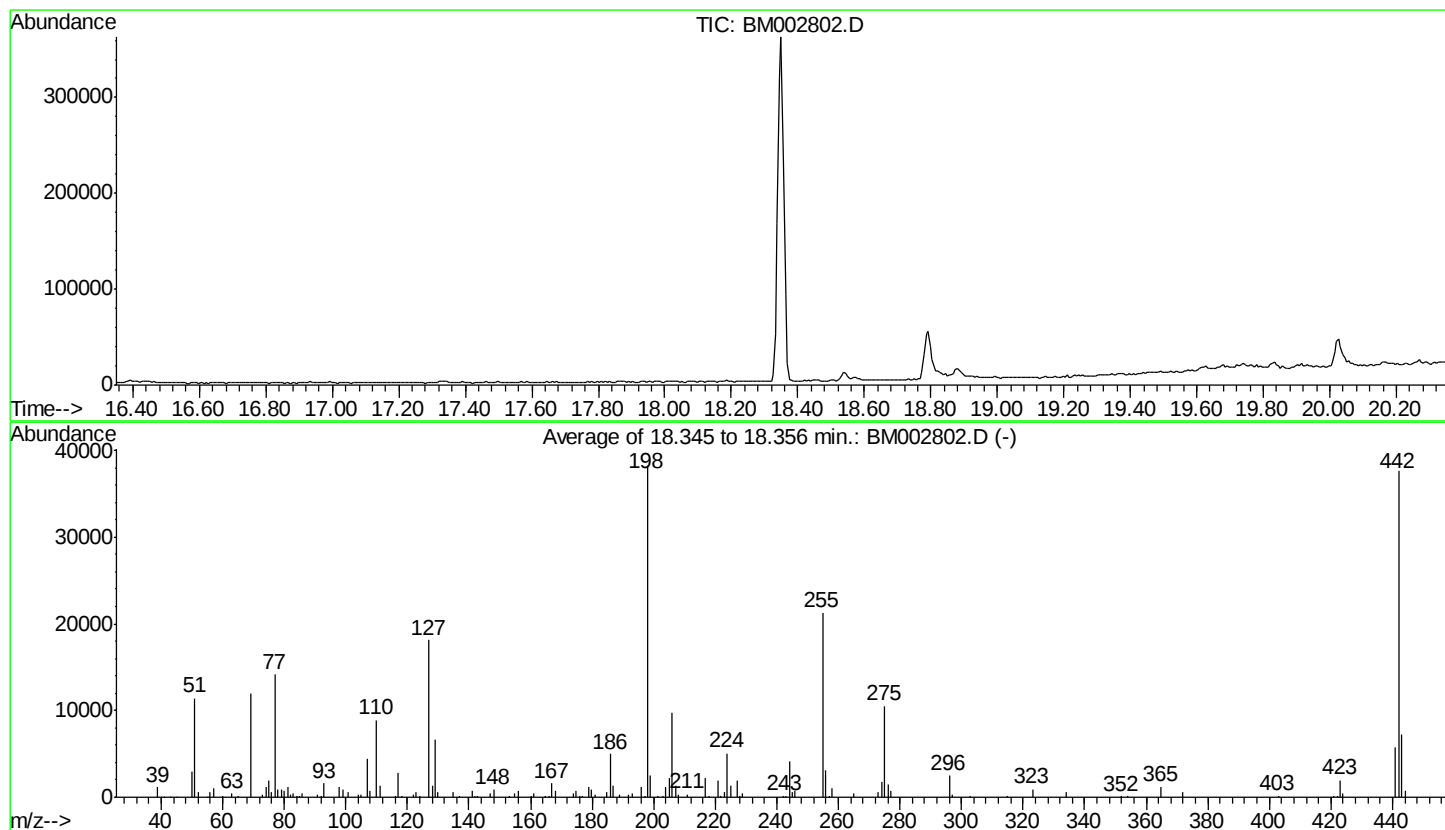

AutoFind: Scans 2594, 2595, 2596; Background Corrected with Scan 2589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	11375	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.3	11985	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.3	18109	PASS
197	198	0.00	2	0.3	105	PASS
198	198	100	100	100.0	38245	PASS
199	198	5	9	6.8	2587	PASS
275	198	10	60	27.5	10503	PASS
365	198	1	100	3.2	1216	PASS
441	443	0.01	100	80.0	5748	PASS
442	198	50	100	98.6	37717	PASS
443	442	15	24	19.1	7186	PASS

Scan 2589 (18.315 min): BM002802.D
DFTPP19

m/z	Abundance
40.00	317.0
41.00	460.0
43.00	818.0
44.00	1349.0
45.00	334.0
55.00	401.0
207.00	354.0

Instrument :
BNA_M
ClientSampleId :
DFTPP19

m/z	Abundance
39.00	1291.0
39.90	370.0
41.00	491.0
43.00	816.0
44.00	1304.0
45.00	348.0
50.00	3436.0
51.00	13861.0
52.00	746.0
55.00	433.0
56.00	576.0
57.00	1236.0
63.00	568.0
65.00	333.0
69.00	13764.0
72.90	330.0
74.00	1340.0
75.00	2376.0
76.00	755.0
77.00	16315.0
78.00	1130.0
79.00	1046.0
79.90	794.0
81.00	1316.0
82.00	447.0
83.00	436.0
85.00	347.0
86.00	478.0
91.00	375.0
91.90	315.0
93.00	1901.0
98.00	1452.0
99.00	1071.0
100.90	733.0
103.90	430.0
104.90	446.0
107.00	5006.0
108.00	765.0
110.00	10202.0
110.90	1485.0
115.90	301.0
117.00	3237.0
118.00	305.0
121.90	367.0
122.90	539.0
127.00	20632.0
128.00	1567.0
129.00	7371.0
130.00	758.0
135.00	672.0
137.00	344.0
141.00	881.0
146.90	401.0
147.90	1002.0
152.90	300.0
155.00	613.0
156.00	799.0
161.00	446.0
165.00	340.0
166.00	321.0
167.00	1698.0
168.00	804.0
173.90	455.0
175.00	793.0
176.00	380.0
178.90	1281.0
180.00	886.0
181.00	418.0
184.90	649.0
186.00	5306.0
187.00	1425.0
188.90	345.0
191.90	468.0
193.00	473.0
196.00	1170.0
197.10	315.0
198.00	41216.0
199.00	2642.0
204.00	1196.0
205.00	2236.0
206.00	9996.0
207.00	1677.0
208.00	306.0
210.90	390.0
216.90	2263.0
218.00	318.0
221.00	2067.0
221.70	476.0
222.90	611.0
224.00	5185.0
225.00	1306.0

Instrument :
BNA_M
ClientSampleId :
DFTPP19

227.00	1974.0
229.00	517.0
242.00	306.0
242.90	336.0
244.00	4014.0
245.00	586.0
245.90	706.0
255.00	20904.0
256.00	3274.0
257.00	334.0
257.90	1008.0
265.00	442.0
273.00	652.0
274.00	1647.0
275.00	10365.0
276.00	1399.0
277.00	763.0
296.00	2510.0
297.00	325.0
323.00	849.0
334.00	468.0
364.90	1094.0
371.90	438.0
423.00	1636.0
423.90	356.0
441.00	4907.0
442.00	31792.0
443.00	6040.0
444.00	617.0

Instrument :
BNA_M
ClientSampleId :
DFTPP19

m/z	Abundance
39.00	1267.0
40.00	382.0
41.10	436.0
43.00	781.0
44.00	1329.0
44.90	389.0
50.00	3227.0
51.00	12934.0
52.00	662.0
55.00	492.0
56.00	537.0
57.00	1168.0
60.00	319.0
63.00	561.0
69.00	13950.0
73.00	390.0
74.00	1331.0
75.00	2234.0
76.00	756.0
77.10	16264.0
78.00	1127.0
79.00	1050.0
79.90	804.0
81.00	1267.0
82.10	300.0
83.00	477.0
84.00	306.0
85.00	317.0
86.00	360.0
90.90	384.0
91.90	309.0
93.00	1677.0
98.00	1410.0
98.90	963.0
101.00	674.0
103.90	415.0
104.90	487.0
107.00	5015.0
108.00	855.0
110.00	10347.0
111.00	1543.0
116.00	335.0
117.00	3377.0
122.00	360.0
123.00	631.0
124.00	303.0
127.00	20792.0
128.00	1538.0
129.00	7607.0
130.00	693.0
135.00	665.0
137.00	314.0
141.00	959.0
142.00	372.0
142.90	307.0
146.90	573.0
148.00	882.0
153.00	329.0
154.90	526.0
156.00	919.0
160.00	328.0
161.00	522.0
164.80	303.0
166.00	360.0
167.00	1875.0
168.00	914.0
174.00	421.0
174.90	795.0
177.00	426.0
178.90	1541.0
179.90	1149.0
181.00	543.0
184.90	738.0
186.00	5902.0
187.00	1609.0
189.00	388.0
192.00	479.0
193.00	595.0
196.00	1533.0
198.00	44544.0
199.00	3245.0
201.40	312.0
202.90	307.0
204.00	1420.0
205.00	2497.0
206.00	11596.0
207.00	1907.0
208.00	415.0
211.00	513.0
217.00	2594.0
218.00	324.0

Instrument :
BNA_M
ClientSampleId :
DFTPP19

221.00	2192.0
223.00	732.0
224.00	5908.0
225.00	1575.0
227.00	2130.0
227.90	316.0
228.90	496.0
241.90	309.0
243.00	341.0
244.00	4787.0
245.00	664.0
245.90	777.0
255.00	25112.0
256.00	3430.0
258.00	1228.0
265.00	575.0
273.00	728.0
274.00	2083.0
275.00	12374.0
276.00	1620.0
276.90	968.0
296.00	2988.0
296.90	484.0
303.00	319.0
315.00	362.0
323.00	1200.0
334.00	686.0
352.00	338.0
364.90	1492.0
372.00	621.0
403.00	341.0
421.00	306.0
422.00	332.0
423.00	2499.0
424.00	518.0
441.00	6925.0
442.00	44776.0
443.00	8890.0
444.00	794.0

Instrument :
BNA_M
ClientSampleId :
DFTPP19

m/z	Abundance
39.00	798.0
39.90	321.0
41.00	479.0
43.00	863.0
44.00	1407.0
45.00	334.0
50.00	2035.0
51.00	7332.0
52.00	406.0
55.00	412.0
56.00	508.0
57.00	699.0
60.00	354.0
69.00	8241.0
73.00	347.0
74.00	834.0
75.00	1287.0
76.00	489.0
77.10	9764.0
78.00	606.0
79.00	665.0
79.90	445.0
81.00	826.0
81.90	307.0
83.10	335.0
85.90	302.0
91.00	319.0
93.00	1098.0
98.00	877.0
99.00	635.0
101.00	465.0
107.00	3102.0
108.00	493.0
110.00	6117.0
111.00	1053.0
117.00	1968.0
123.00	399.0
127.00	12905.0
128.00	985.0
129.00	4767.0
129.90	390.0
135.00	430.0
140.90	568.0
146.90	350.0
147.90	648.0
154.90	327.0
156.00	435.0
160.90	334.0
167.00	1148.0
167.90	514.0
174.00	357.0
175.00	561.0
179.00	831.0
180.00	697.0
184.90	466.0
186.00	3795.0
187.00	1066.0
188.90	305.0
192.90	344.0
195.90	858.0
197.90	28976.0
199.00	1876.0
204.00	885.0
205.00	1765.0
206.00	7546.0
207.00	1402.0
208.00	339.0
216.90	1767.0
221.00	1510.0
222.90	460.0
224.00	4109.0
225.00	923.0
227.00	1684.0
228.90	376.0
244.00	3504.0
244.90	420.0
246.00	597.0
255.00	17824.0
256.00	2444.0
257.90	956.0
264.90	362.0
273.00	483.0
274.00	1486.0
275.00	8770.0
276.00	1228.0
277.00	664.0
296.00	1982.0
297.00	309.0
323.00	782.0
334.00	546.0
353.90	325.0

Instrument :
BNA_M
ClientSampleId :
DFTPP19

364.90	1064.0
372.00	521.0
403.00	304.0
423.00	1795.0
424.00	427.0
441.00	5414.0
442.00	36584.0
443.00	6628.0
444.00	676.0

Instrument :
BNA_M
ClientSampleId :
DFTPP19