

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100117\
 Data File : BM011807.D
 Acq On : 01 Oct 2017 14:07
 Operator : SJ/JU
 Sample : PB102763BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK63

Quant Time: Oct 02 02:27:05 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM092717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 02 02:22:21 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	114448	20.00	ng/ul	0.00
18) Naphthalene-d8	10.69	136	520730	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.52	164	320789	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.26	188	778838	20.00	ng/ul	0.00
75) Chrysene-d12	21.43	240	913124	20.00	ng/ul	0.00
83) Perylene-d12	23.76	264	1054412	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	15212	5.93	ng/uL	0.00
5) Phenol-d5	7.03	99	293332	26.06	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.21	67	244904	30.00	ng/ul	0.00
9) 2-Chlorophenol-d4	7.41	132	244654	29.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.58	113	242725	27.53	ng/ul	0.00
19) Nitrobenzene-d5	9.05	128	122453	30.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.77	143	135042	31.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.30	165	234666	28.38	ng/ul	0.00
29) 4-Chloroaniline-d4	10.82	131	350293	38.32	ng/ul	0.00
43) Dimethylphthalate-d6	13.93	166	924338	33.59	ng/ul	0.00
46) Acenaphthylene-d8	14.22	160	1008255	30.30	ng/ul	0.00
51) 4-Nitrophenol-d4	14.72	143	114456	24.34	ng/ul	0.00
57) Fluorene-d10	15.52	176	741768	31.31	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.63	200	132715	25.16	ng/ul	0.00
70) Anthracene-d10	17.36	188	1254920	31.66	ng/ul	0.00
76) Pyrene-d10	19.65	212	1572780	36.09	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.61	264	1646483	32.61	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) 2,6-Dinitrotoluene	13.93	165	5058	1.044	ng/ul#	23




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100117\
Data File : BM011807.D
Acq On : 01 Oct 2017 14:07
Operator : SJ/JU
Sample : PB102763BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK63

Quant Time: Oct 02 02:27:05 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM092717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 02 02:22:21 2017
Response via : Initial Calibration

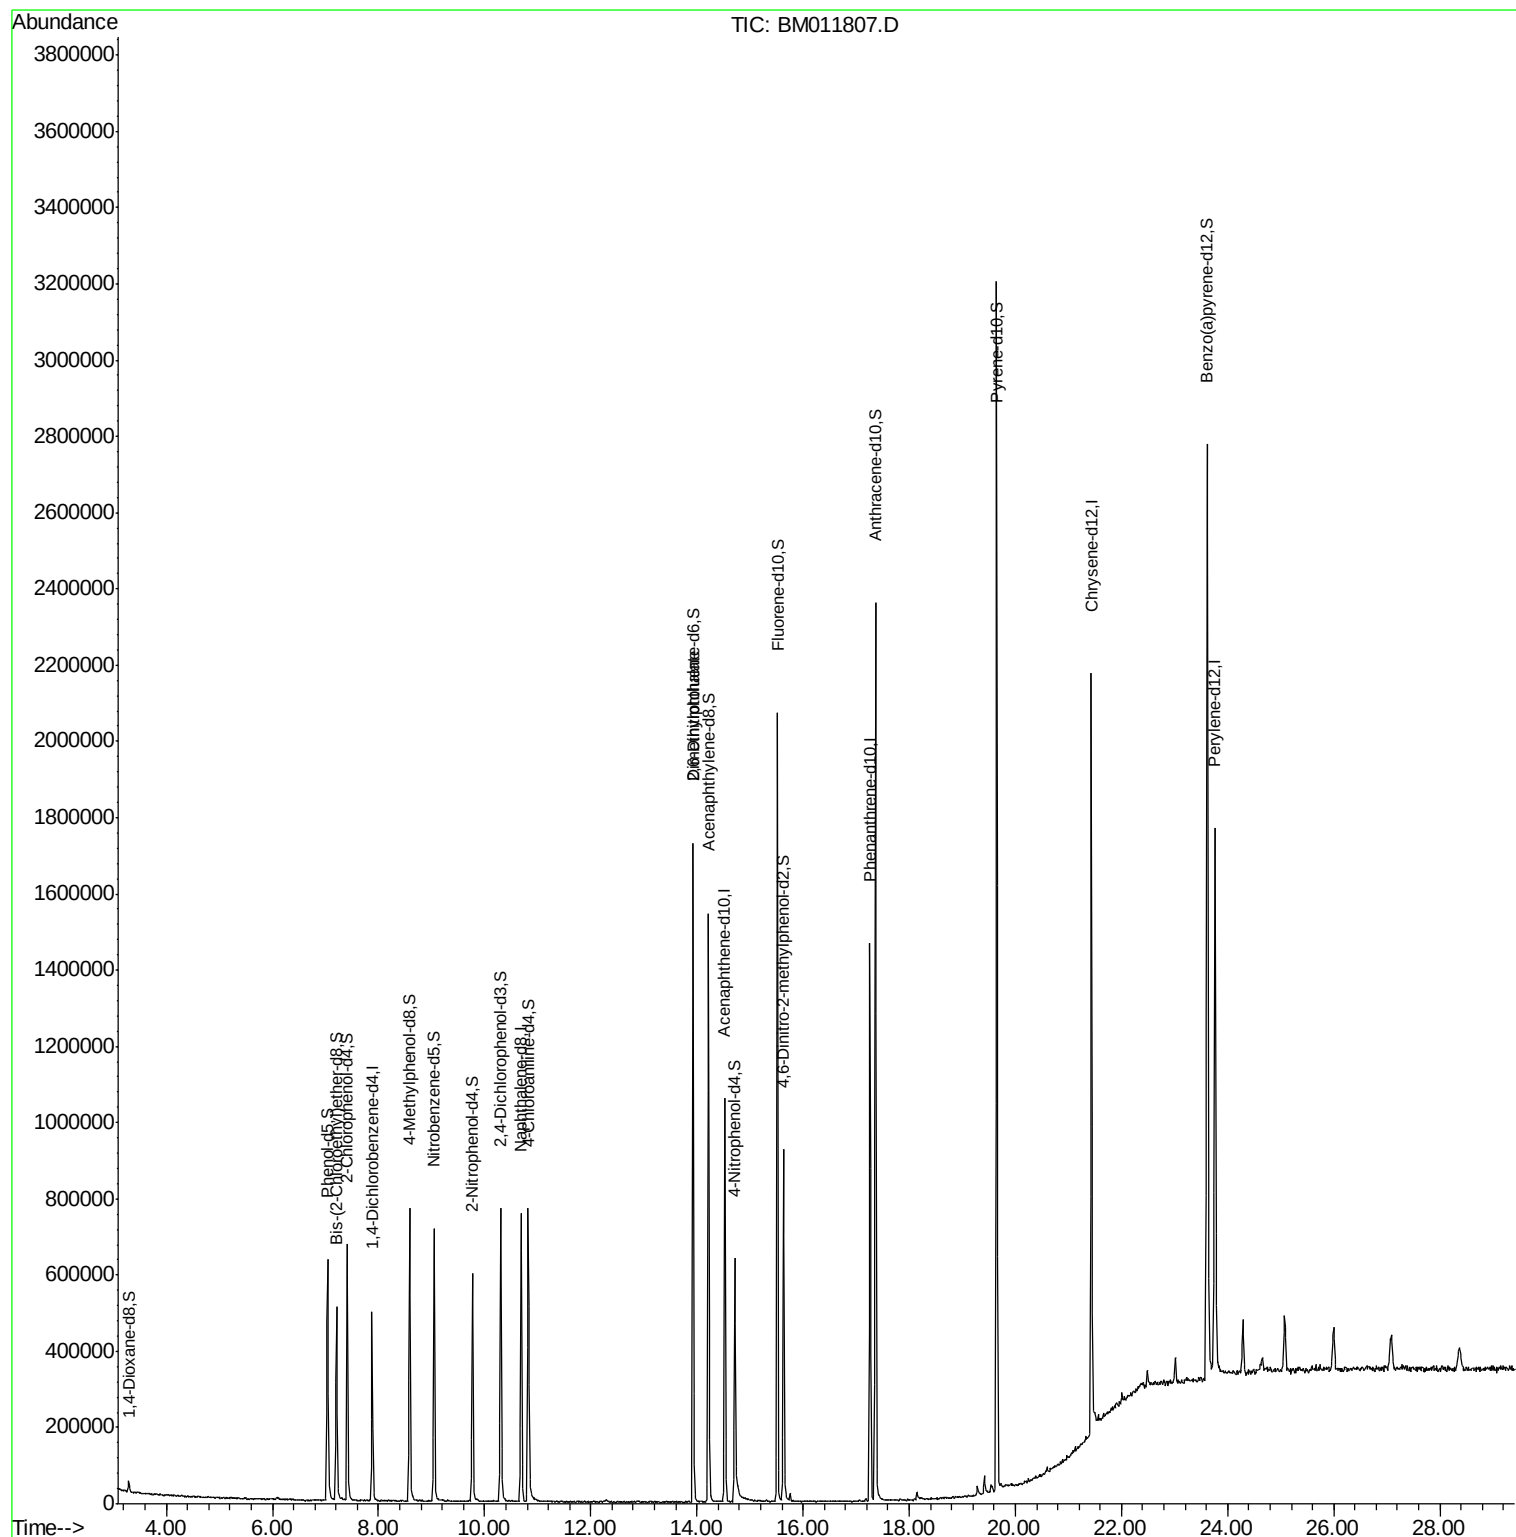

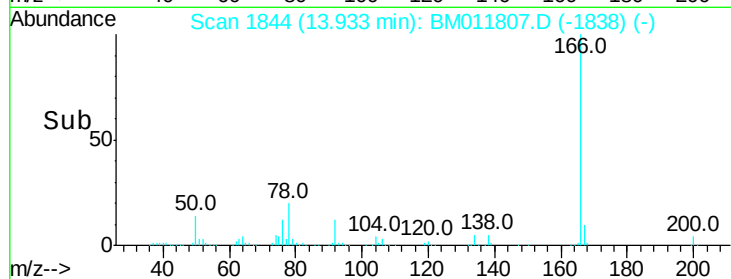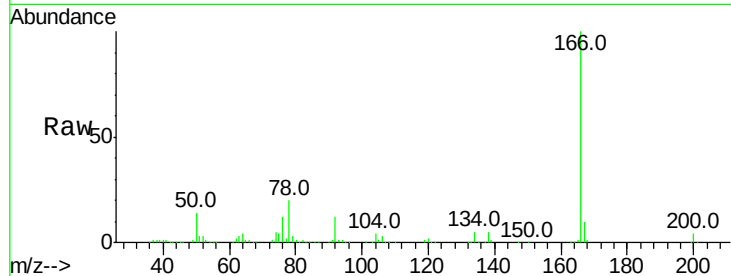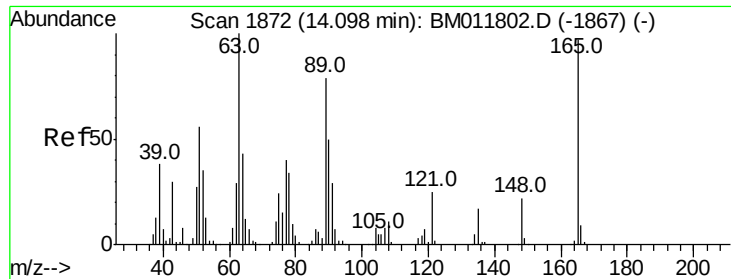

#45

2,6-Dinitrotoluene

Concen: 1.044 ng/ul

RT: 13.93 min Scan# 1844

Delta R.T. -0.16 min

Lab File: BM011807.D

Acq: 01 Oct 2017 14:07

Instrument :

BNA_M

ClientSampleId :

SBLK63

Tot Ion:165 Resp: 5058

Ion Ratio Lower Upper

165 100

89 0.0 52.6 79.0#

121 43.2 14.6 22.0#

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

