

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100117\
 Data File : BM011821.D
 Acq On : 01 Oct 2017 22:34
 Operator : SJ/JU
 Sample : I5458-14
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG8

Quant Time: Oct 02 05:11:44 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM092717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 02 04:55:04 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	103219	20.00	ng/ul	0.00
18) Naphthalene-d8	10.69	136	484659	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.52	164	295094	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.26	188	724468	20.00	ng/ul	0.00
75) Chrysene-d12	21.43	240	888773	20.00	ng/ul	0.00
83) Perylene-d12	23.76	264	1006053	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	11905	5.14	ng/uL	0.00
5) Phenol-d5	7.04	99	64980	6.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.20	67	226371	30.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.41	132	192774	25.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.58	113	127663	16.05	ng/ul	0.00
19) Nitrobenzene-d5	9.05	128	115936	30.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.77	143	125962	31.24	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.30	165	210567	27.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.84	131	16947	1.99	ng/ul	0.02
43) Dimethylphthalate-d6	13.93	166	878154	34.70	ng/ul	0.00
46) Acenaphthylene-d8	14.22	160	990261	32.35	ng/ul	0.00
51) 4-Nitrophenol-d4	14.72	143	15321	3.54	ng/ul	0.00
57) Fluorene-d10	15.52	176	743653	34.12	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.63	200	133031	27.11	ng/ul	0.00
70) Anthracene-d10	17.36	188	1243771	33.74	ng/ul	0.00
76) Pyrene-d10	19.65	212	1582954	37.32	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.61	264	1658247	34.42	ng/ul	0.00


Target Compounds				Ovalue	
45) 2,6-Dinitrotoluene	13.93	165	5096	1.143	ng/ul# 26




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100117\
Data File : BM011821.D
Acq On : 01 Oct 2017 22:34
Operator : SJ/JU
Sample : I5458-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG8

Quant Time: Oct 02 05:11:44 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM092717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 02 04:55:04 2017
Response via : Initial Calibration

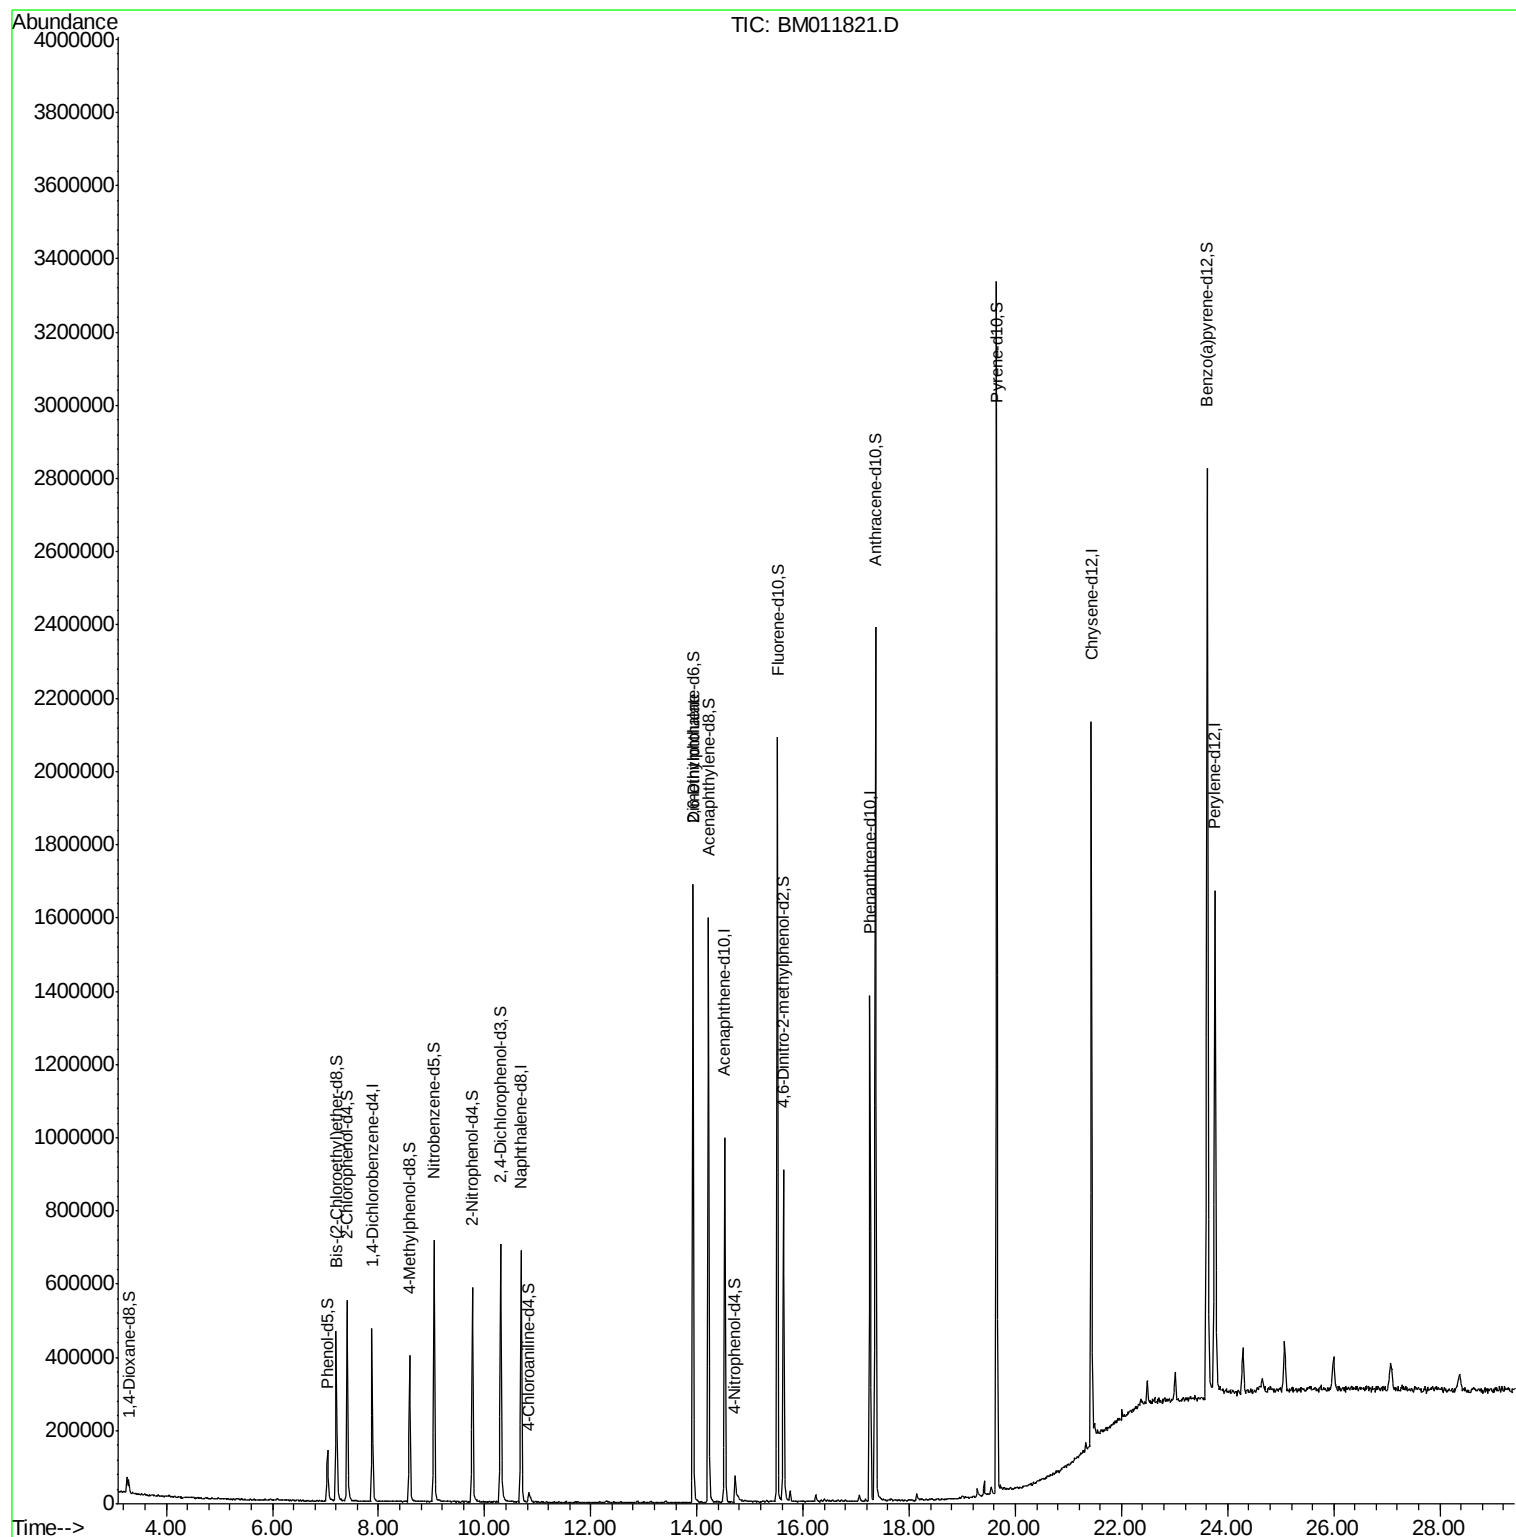

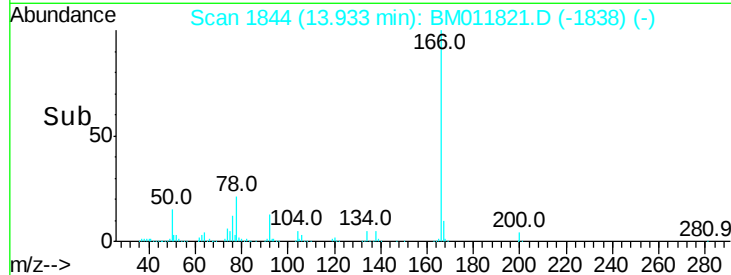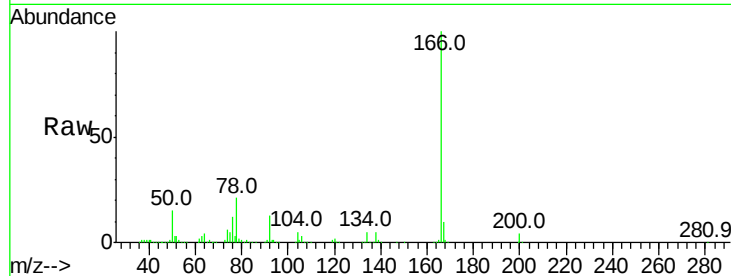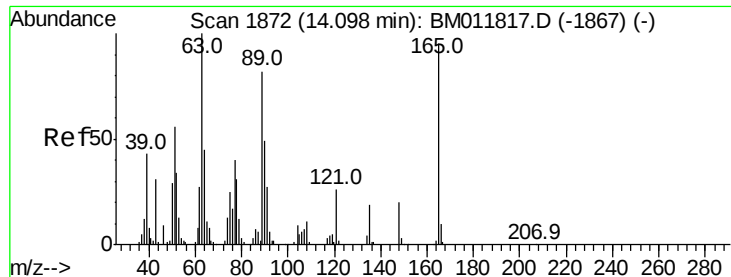

#45

2,6-Dinitrotoluene

Concen: 1.143 ng/ul

RT: 13.93 min Scan# 1844

Delta R.T. -0.16 min

Lab File: BM011821.D

Acq: 01 Oct 2017 22:34

Instrument :

BNA_M

ClientSampleId :

C0AG8

Tot Ion:165 Resp: 5096

Ion Ratio Lower Upper

165 100

89 0.0 52.6 79.0#

121 37.3 14.6 22.0#

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

