

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100117\
 Data File : BM011808.D
 Acq On : 01 Oct 2017 14:44
 Operator : SJ/JU
 Sample : I5477-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET243

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.039	665	672	683	rBV	122827	222782	5.41%	0.619%
2	7.210	695	701	715	rBV	410661	697266	16.94%	1.937%
3	7.410	728	735	752	rBV	467317	813848	19.77%	2.261%
4	7.881	809	815	826	rBV	491350	881291	21.41%	2.449%
5	8.586	927	935	947	rBV	334987	621988	15.11%	1.728%
6	9.045	1005	1013	1027	rBV	594805	1064012	25.85%	2.956%
7	9.769	1129	1136	1149	rBV	515519	904170	21.97%	2.512%
8	10.304	1220	1227	1241	rBV	615205	1126431	27.37%	3.130%
9	10.686	1285	1292	1307	rVB	743212	1269522	30.85%	3.527%
10	13.927	1836	1843	1861	rBV	1379010	1959920	47.62%	5.446%
11	14.215	1886	1892	1905	rBV	1338315	2015406	48.97%	5.600%
12	14.527	1938	1945	1955	rBV2	1052403	1694329	41.17%	4.708%
13	14.721	1971	1978	1986	rBV2	58628	129827	3.15%	0.361%
14	15.515	2106	2113	2120	rBV	1833398	2561672	62.24%	7.118%
15	15.633	2127	2133	2147	rBV	792607	1146468	27.86%	3.185%
16	17.268	2404	2411	2421	rBV	1449785	2116890	51.43%	5.882%
17	17.362	2421	2427	2440	rVV	2014875	2984754	72.52%	8.293%
18	18.139	2554	2559	2566	rBV	59576	92998	2.26%	0.258%
19	19.286	2749	2754	2760	rBV	23255	44055	1.07%	0.122%
20	19.415	2771	2776	2782	rBV2	122474	183077	4.45%	0.509%
21	19.545	2794	2798	2805	rBV3	21072	41500	1.01%	0.115%
22	19.650	2810	2816	2825	rBV	2799063	3713794	90.23%	10.319%
23	21.433	3114	3119	3126	rBV	2204220	2724377	66.19%	7.570%
24	23.615	3483	3490	3501	rBV2	2092181	4115739	100.00%	11.435%
25	23.768	3509	3516	3525	rVB	1423244	2865001	69.61%	7.960%


Sum of corrected areas: 35991117

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100117\
Data File : BM011808.D
Acq On : 01 Oct 2017 14:44
Operator : SJ/JU
Sample : I5477-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
ET243

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM092717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

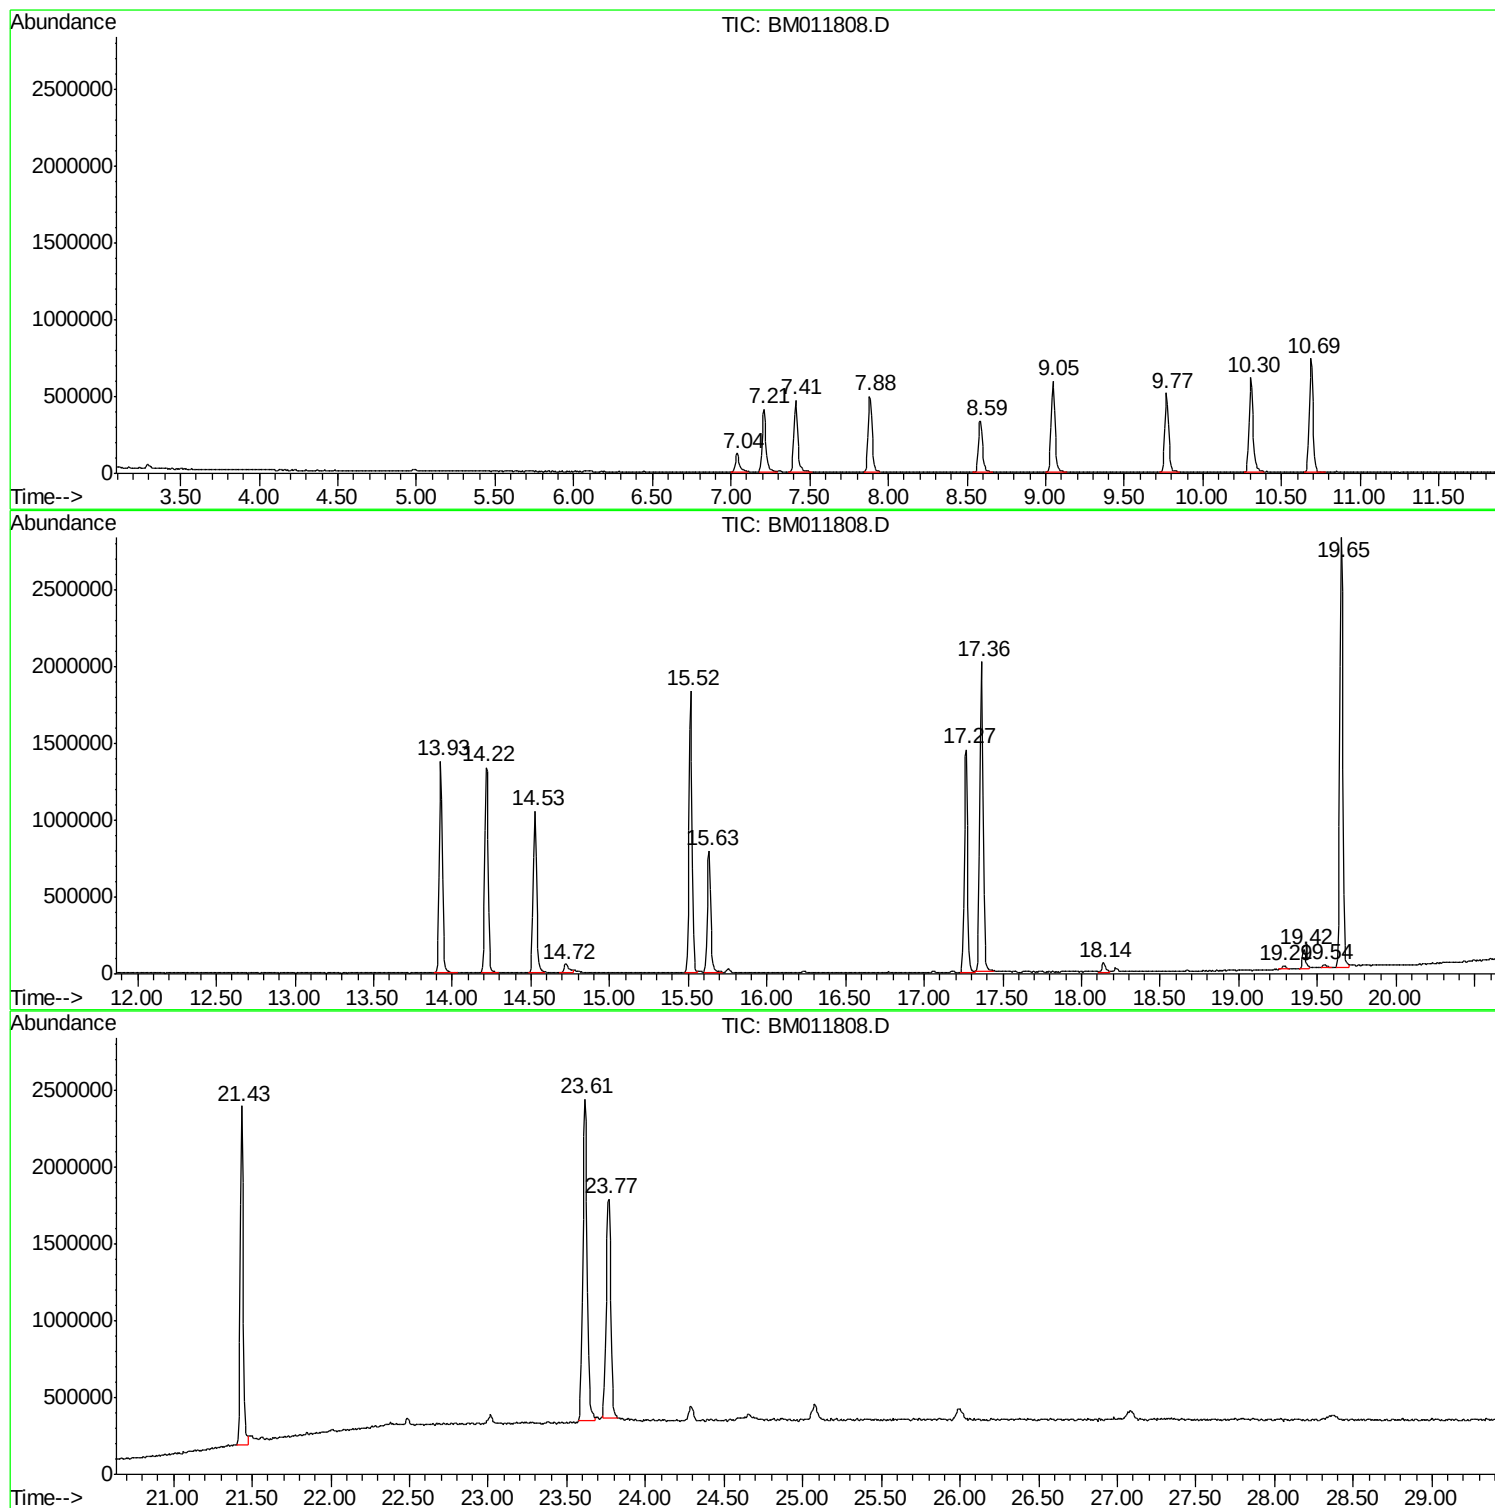

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM100117\
Data File : BM011808.D
Acq On : 01 Oct 2017 14:44
Operator : SJ/JU
Sample : I5477-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET243

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM100117\
Data File : BM011808.D
Acq On : 01 Oct 2017 14:44
Operator : SJ/JU
Sample : I5477-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET243

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc