

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100117\
 Data File : BM011834.D
 Acq On : 02 Oct 2017 06:19
 Operator : SJ/JU
 Sample : I5477-13
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET238

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	31	34	43	rVB	43626	69189	1.12%	0.133%
2	7.034	665	671	681	rBV	228312	402831	6.55%	0.774%
3	7.204	694	700	712	rBV	643277	1034565	16.81%	1.988%
4	7.410	727	735	752	rBV	739113	1303270	21.18%	2.504%
5	7.881	808	815	824	rBV	640407	1093651	17.77%	2.101%
6	8.581	927	934	944	rBV	619366	1054741	17.14%	2.027%
7	9.045	1005	1013	1026	rBV	921625	1617894	26.30%	3.109%
8	9.763	1128	1135	1150	rBV	816634	1425697	23.17%	2.739%
9	10.298	1219	1226	1244	rBV	1055583	1879127	30.54%	3.610%
10	10.680	1282	1291	1301	rBV	937786	1586581	25.79%	3.048%
11	10.833	1310	1317	1328	rBV3	38406	98678	1.60%	0.190%
12	13.927	1836	1843	1852	rBV	2071146	2958045	48.08%	5.683%
13	14.216	1886	1892	1906	rVB	2187166	3096274	50.32%	5.949%
14	14.521	1936	1944	1959	rBV2	1357052	2226029	36.18%	4.277%
15	14.715	1971	1977	1985	rBV	162582	334447	5.44%	0.643%
16	15.510	2106	2112	2120	rBV	2749115	3959284	64.35%	7.607%
17	15.627	2126	2132	2141	rBV	1352990	1947023	31.64%	3.741%
18	17.262	2404	2410	2419	rBV2	1943906	2760153	44.86%	5.303%
19	17.362	2421	2427	2441	rBV	3276843	4781739	77.72%	9.187%
20	18.139	2556	2559	2568	rBV3	108913	158037	2.57%	0.304%
21	19.415	2773	2776	2781	rVB2	219377	252224	4.10%	0.485%
22	19.650	2810	2816	2823	rBV	4783592	6152771	100.00%	11.822%
23	21.433	3114	3119	3128	rBV	2728345	3495645	56.81%	6.716%
24	23.615	3482	3490	3502	rBV	2742679	5322531	86.51%	10.226%
25	23.762	3508	3515	3528	rVB	1530568	3036790	49.36%	5.835%


Sum of corrected areas: 52047216

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100117\
Data File : BM011834.D
Acq On : 02 Oct 2017 06:19
Operator : SJ/JU
Sample : I5477-13
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
ET238

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM092717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

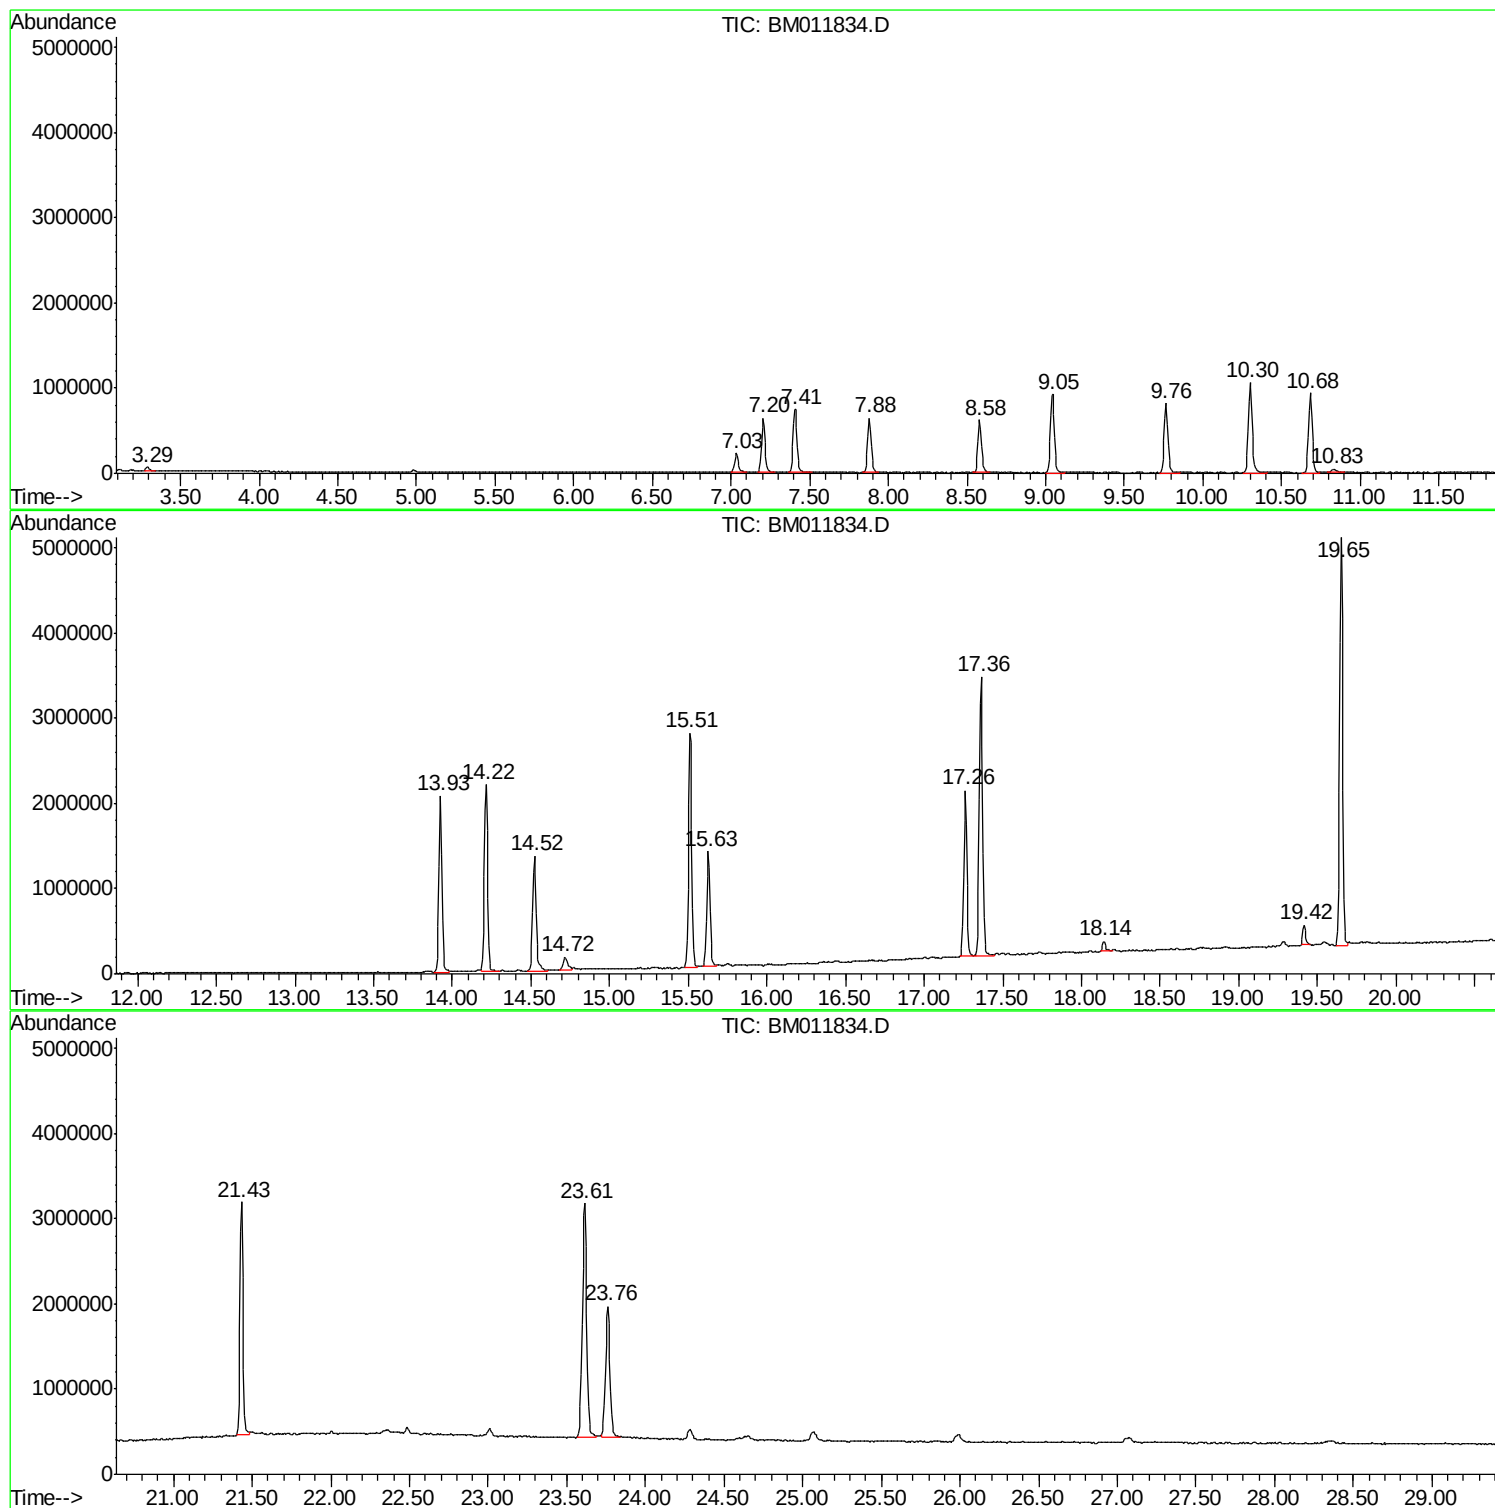

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM100117\
Data File : BM011834.D
Acq On : 02 Oct 2017 06:19
Operator : SJ/JU
Sample : I5477-13
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET238

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM100117\
Data File : BM011834.D
Acq On : 02 Oct 2017 06:19
Operator : SJ/JU
Sample : I5477-13
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET238

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc