

Quantitation Report (QT Reviewed)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100120\
 Data File : BM027572.D
 Acq On : 01 Oct 2020 14:13
 Operator : JU/CG
 Sample : PB131994BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK994

Quant Time: Oct 01 14:46:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM092920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 01 14:40:17 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 10/2/2020 12:15:06 PM

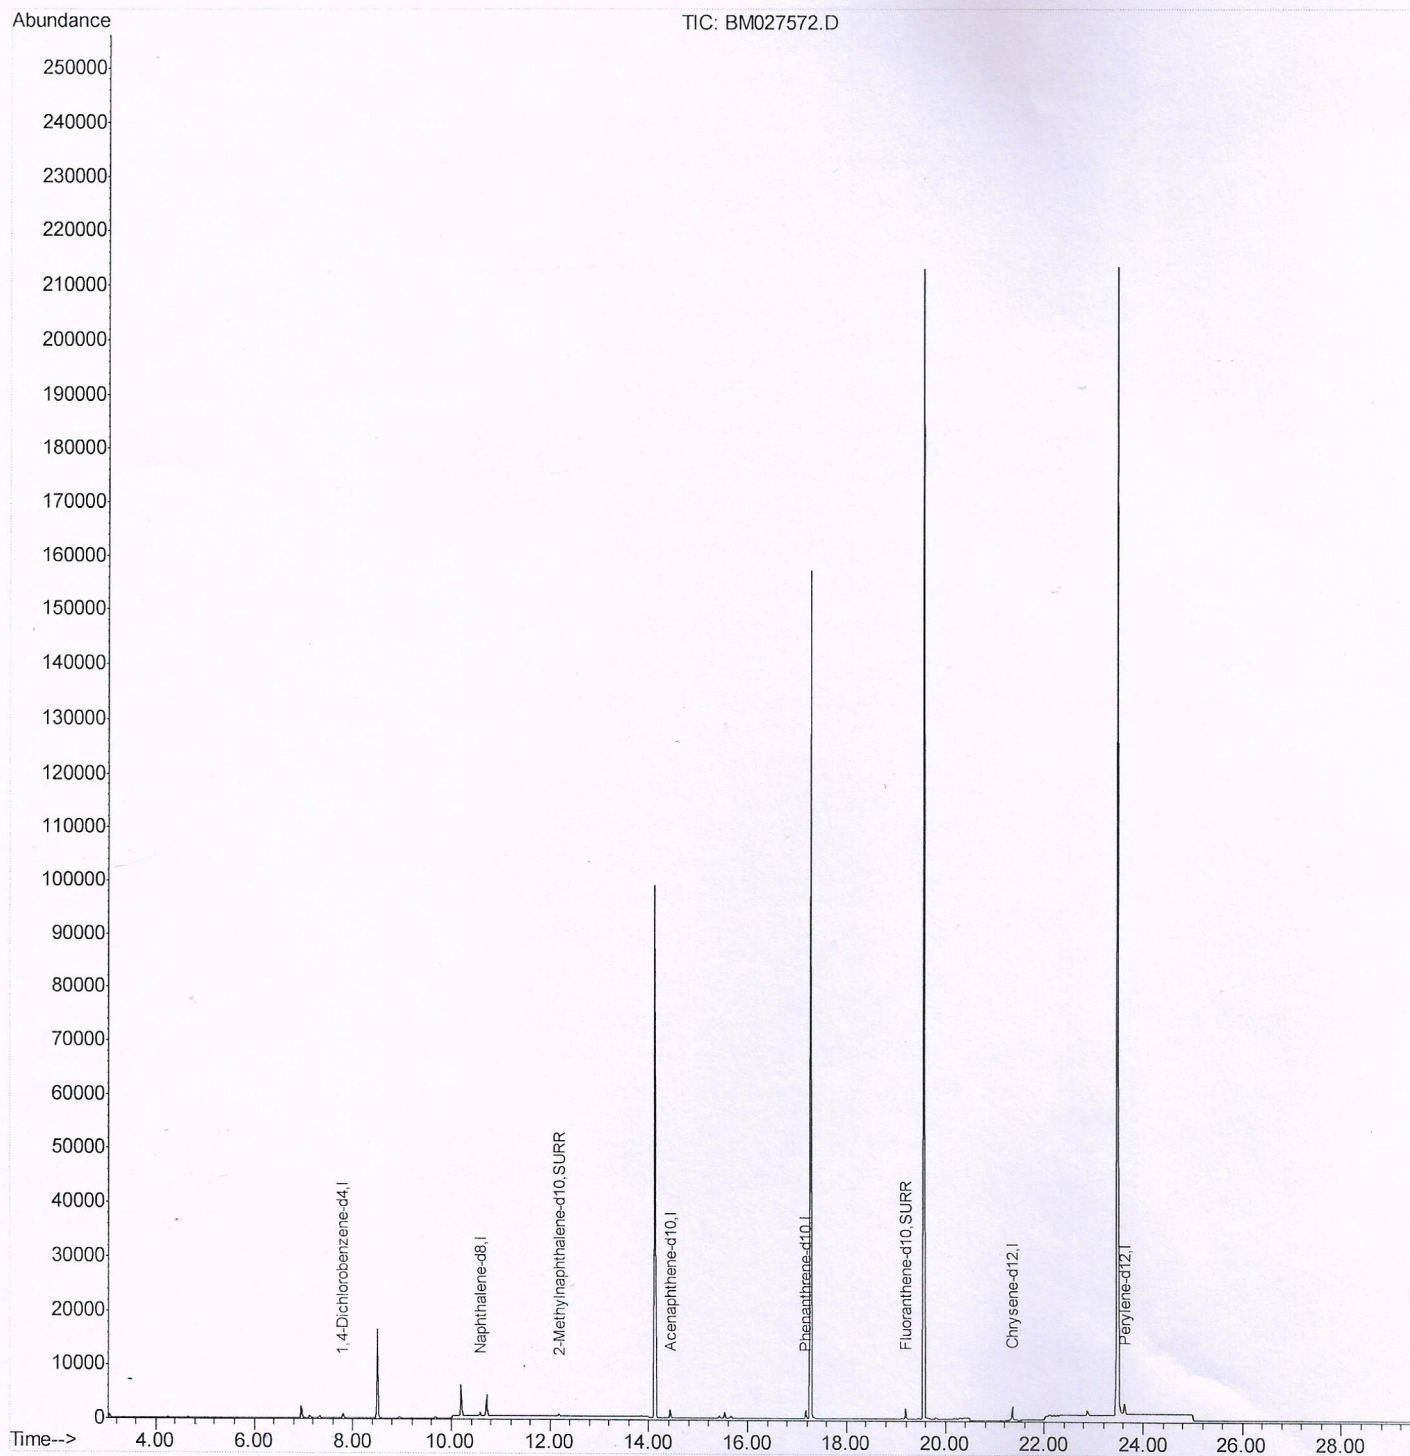

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100120\
 Data File : BM027572.D
 Acq On : 01 Oct 2020 14:13
 Operator : JU/CG
 Sample : PB131994BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK994

Quant Time: Oct 01 14:44:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM092920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 01 14:40:17 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 10/2/2020 12:15:06 PM

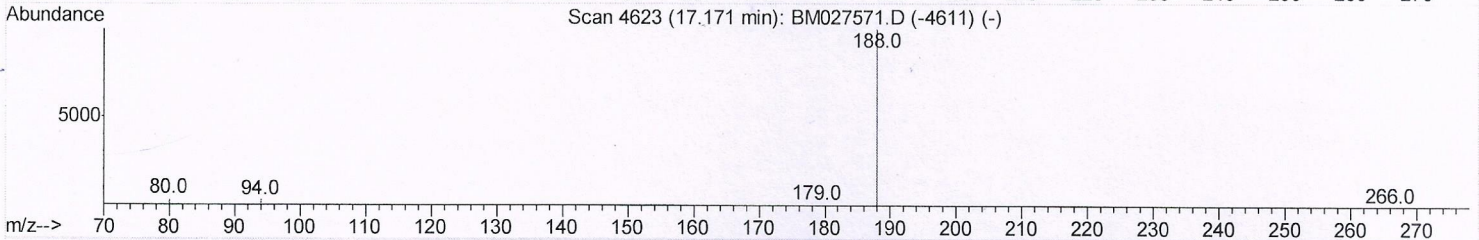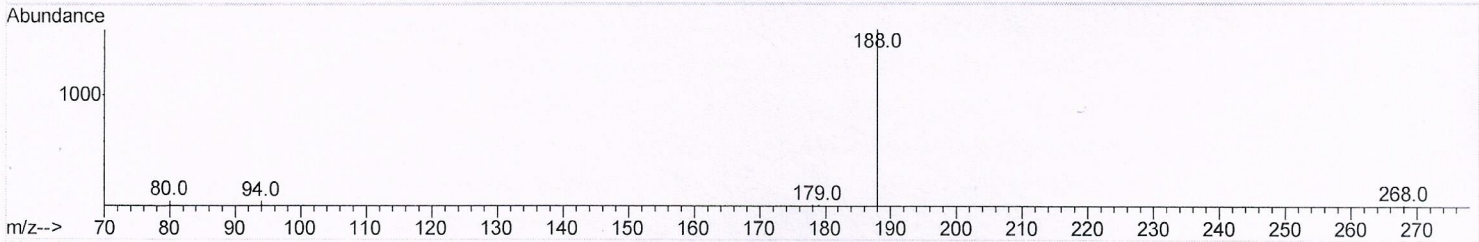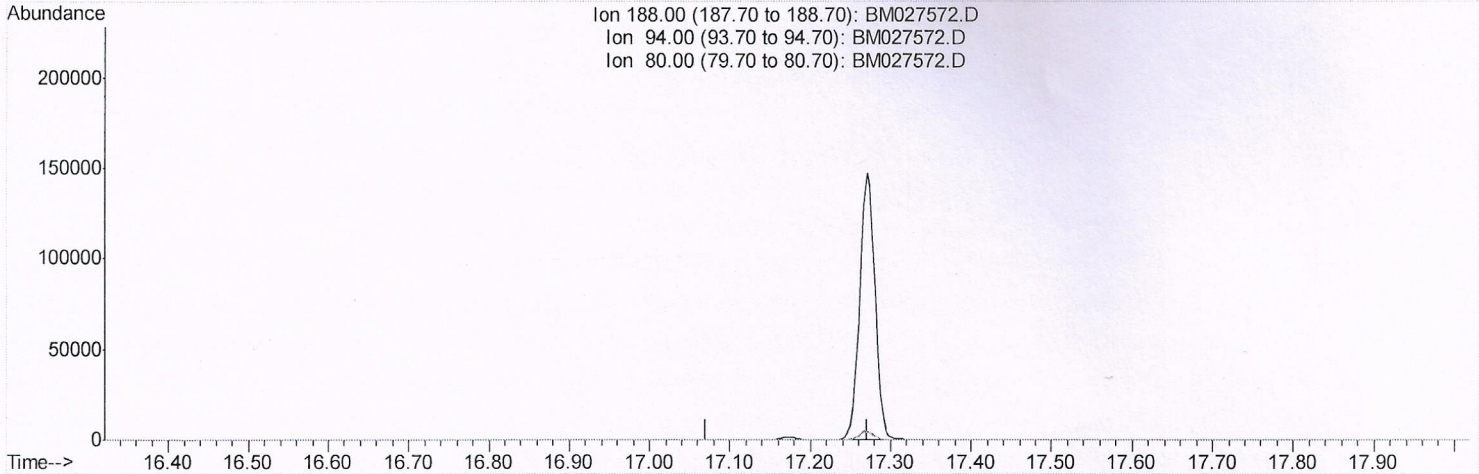

(11) Phenanthrene-d10 (I)

17.171min (-17.171) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	4.80	0.00#
80.00	5.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100120\
Data File : BM027572.D
Acq On : 01 Oct 2020 14:13
Operator : JU/CG
Sample : PB131994BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

SBLK994




Quant Time: Oct 01 14:44:28 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM092920.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Oct 01 14:40:17 2020

Response via : Initial Calibration

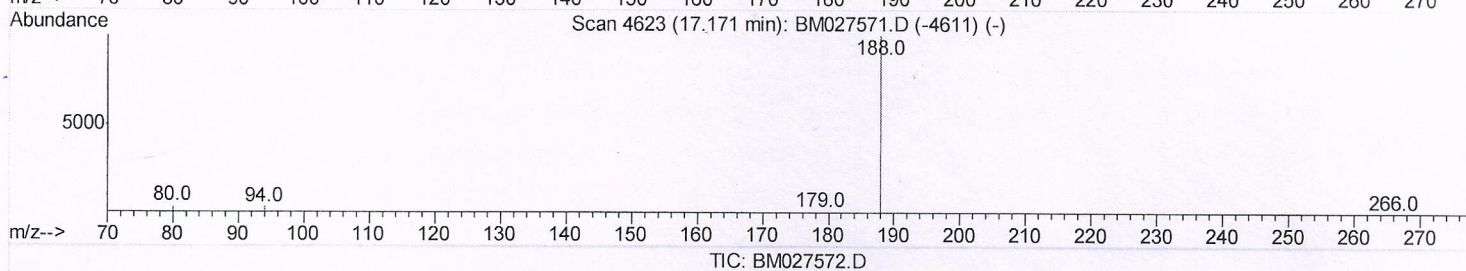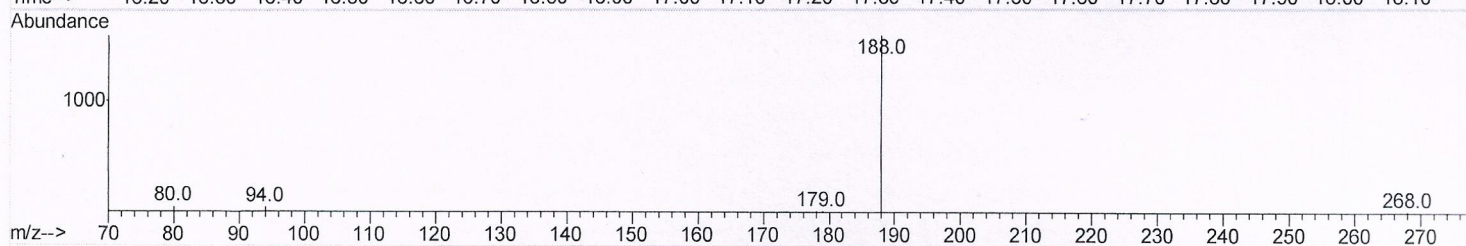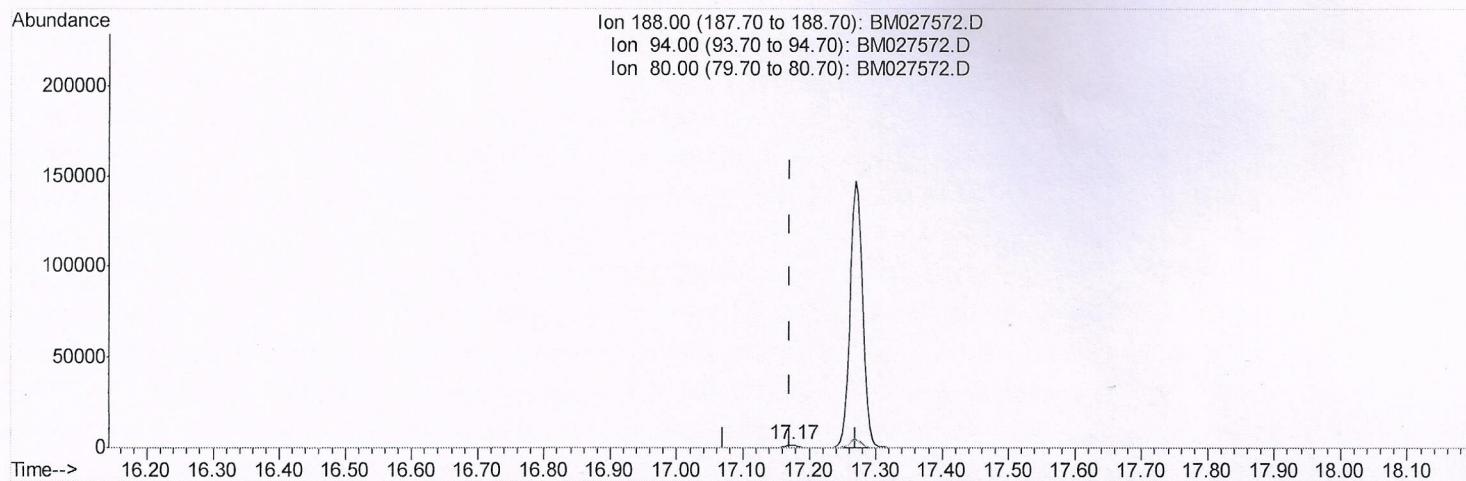Manual Integrations
APPROVEDmohammad
10/2/2020 12:15:06 PM

(11) Phenanthrene-d10 (I)

17.173min (+0.002) 0.40ng/ul m

response 2263

Ion	Exp%	Act%
188.00	100	100
94.00	4.80	5.39
80.00	5.00	5.91
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100120\
Data File : BM027572.D
Acq On : 01 Oct 2020 14:13
Operator : JU/CG
Sample : PB131994BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK994

Quant Time: Oct 01 14:46:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM092920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 01 14:40:17 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
10/2/2020 12:15:06 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	373	0.40	ng/ul	0.00
2) Naphthalene-d8	10.59	136	1006	0.40	ng/ul	0.00
7) Acenaphthene-d10	14.43	164	835	0.40	ng/ul	0.00
11) Phenanthrene-d10	17.17	188	2263m	0.40	ng/ul	0.00
17) Chrysene-d12	21.35	240	2297	0.40	ng/ul	0.00
21) Perylene-d12	23.61	264	2697	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev (Min)
4) 2-Methylnaphthalene-d10	12.18	152	647	0.32	ng/ul	0.00
15) Fluoranthene-d10	19.20	212	2362	0.31	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed