
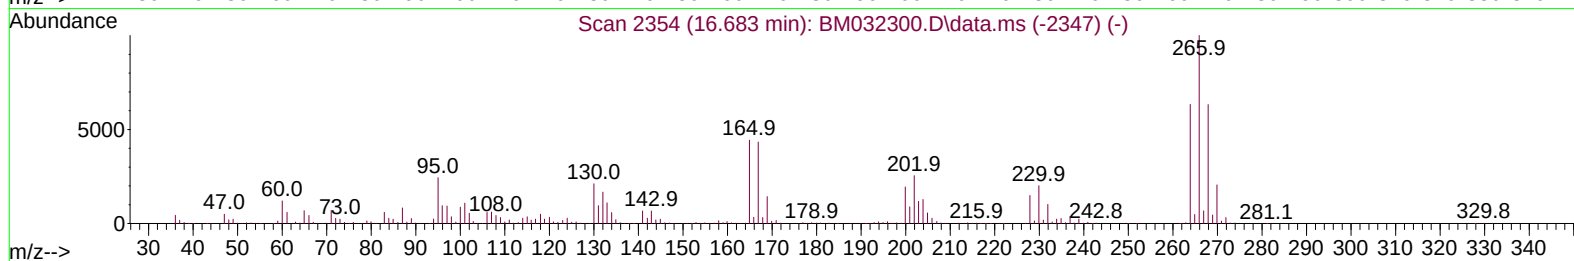
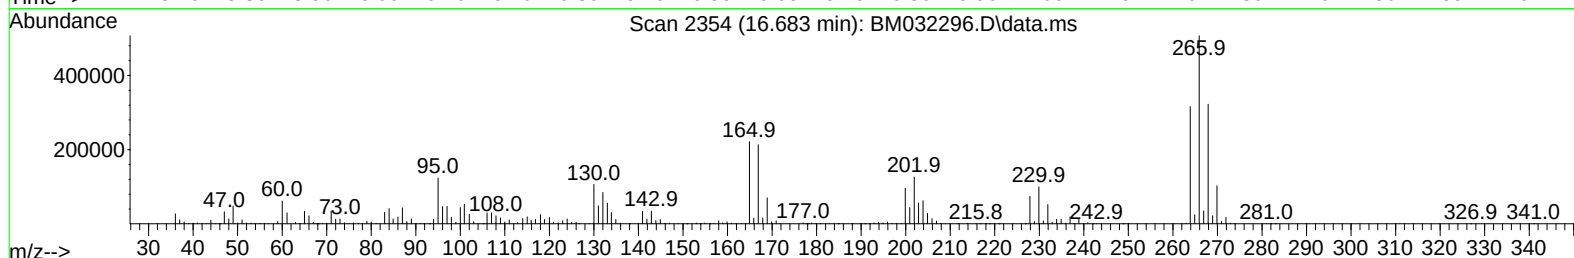


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100121\
 Data File : BM032296.D
 Acq On : 30 Sep 2021 15:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 19:17:16 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 30 19:01:58 2021
 Response via : Initial Calibration

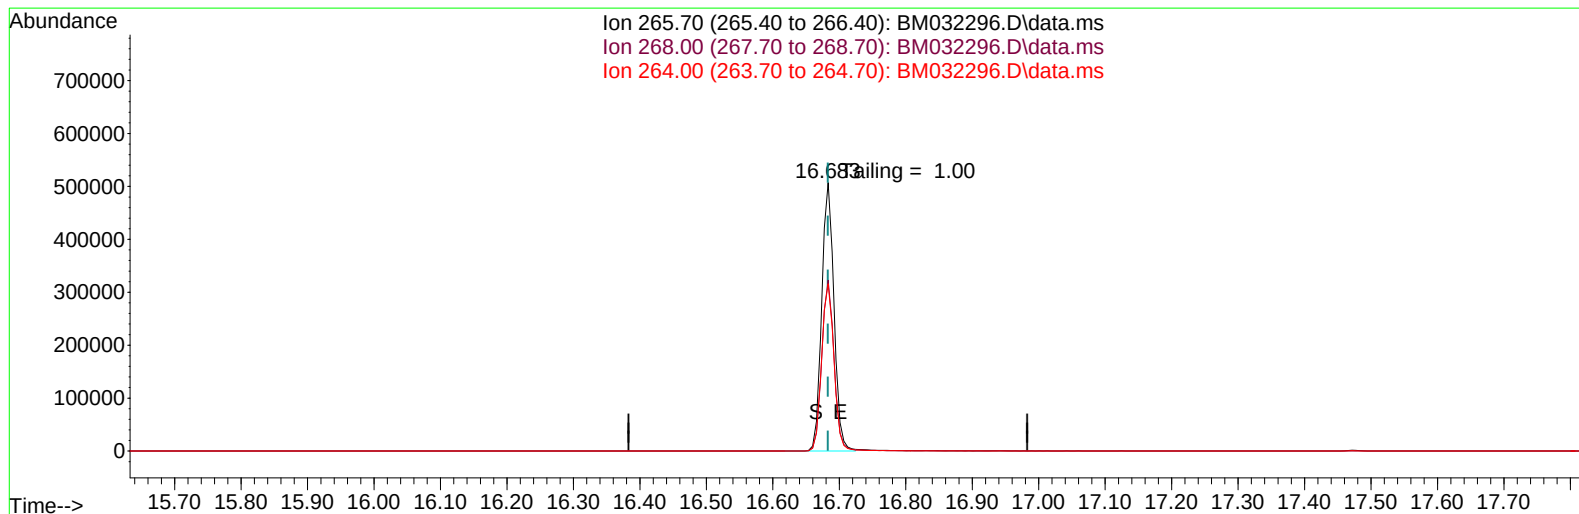

TIC: BM032296.D\data.ms

(70) Pentachlorophenol (C)




16.683min (+ 0.000) 0.00 ng

response 657619

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.62
264.00	65.10	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100121\
Data File : BM032296.D
Acq On : 30 Sep 2021 15:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 19:17:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 19:01:58 2021
Response via : Initial Calibration

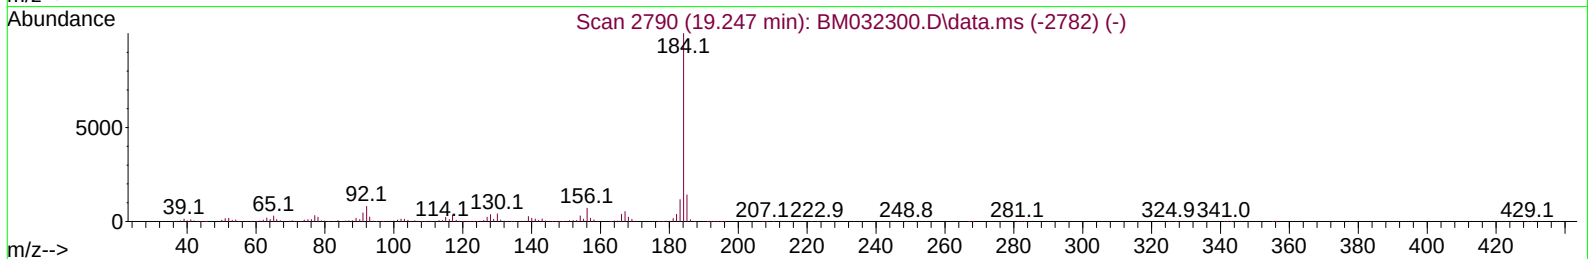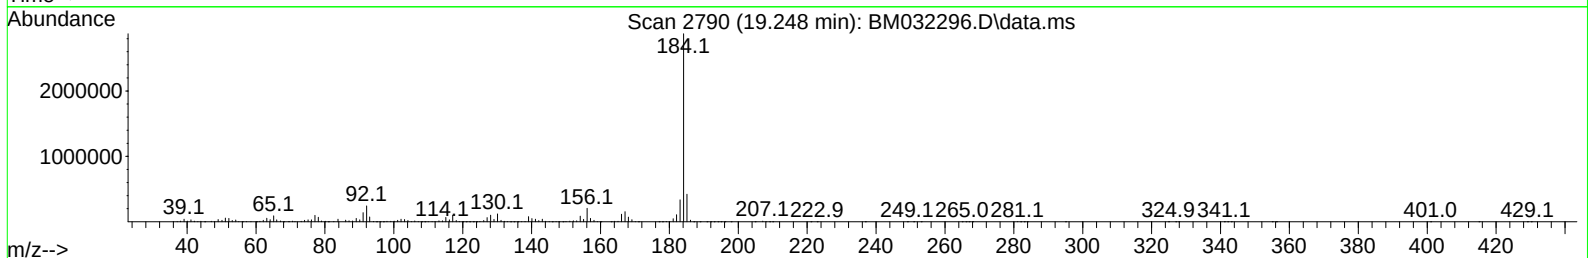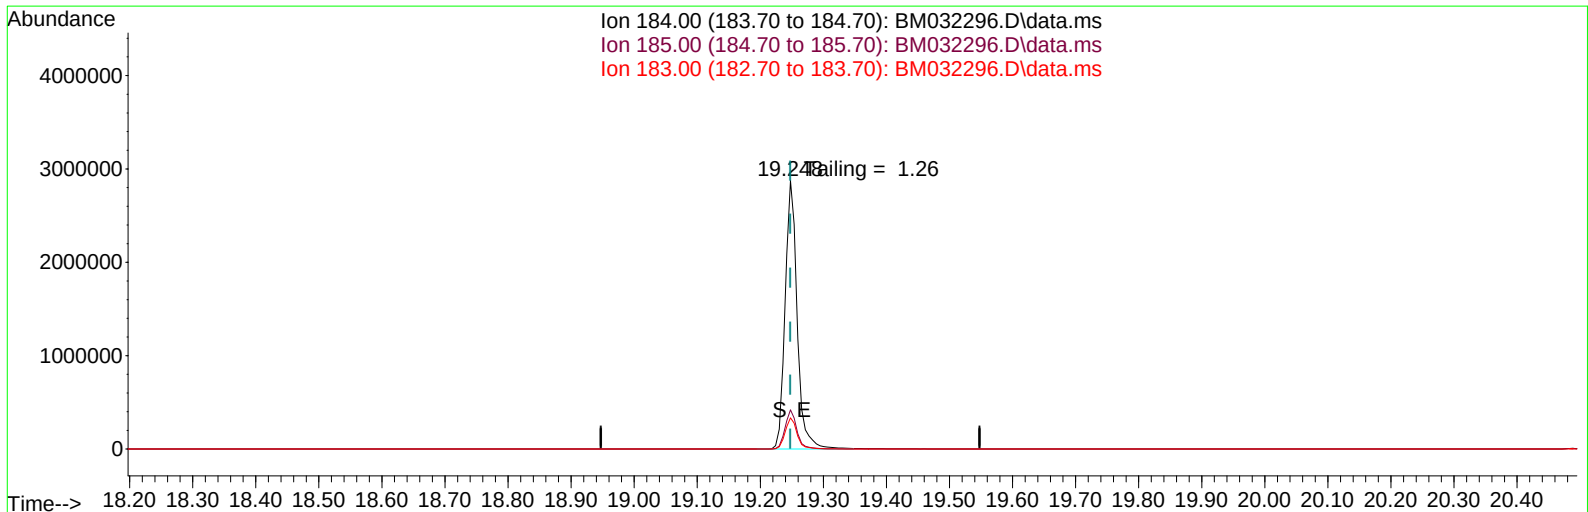

TIC: BM032296.D\data.ms

(77) Benzidine**19.248min (+ 0.000) 3305350.64 ng****response 3835494**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.62
183.00	11.20	11.67
0.00	0.00	0.00