

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100121\
 Data File : BM032305.D
 Acq On : 30 Sep 2021 21:53
 Operator : CG/JU
 Sample : PB139476BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB139476BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM032305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.213	397	404	416	rBV	6622943	9593231	56.45%	10.971%
2	6.837	672	680	693	rVB	6077576	9660890	56.85%	11.049%
3	7.642	809	817	824	rBV	1438269	2200193	12.95%	2.516%
4	8.795	1004	1013	1021	rBV	3886765	6267360	36.88%	7.168%
5	10.430	1284	1291	1301	rVB	1851616	2947117	17.34%	3.371%
6	12.907	1703	1712	1719	rBV	8876514	13258667	78.02%	15.164%
7	14.283	1940	1946	1953	rBV	2555866	3666112	21.57%	4.193%
8	15.771	2192	2199	2218	rBV	6550874	9260215	54.49%	10.591%
9	17.012	2404	2410	2421	rBV	3296954	4336103	25.51%	4.959%
10	19.630	2849	2855	2860	rBV	12581393	16995017	100.00%	19.437%
11	20.383	2980	2983	2988	rBV	160775	193076	1.14%	0.221%
12	21.177	3113	3118	3124	rBV	3899790	4620443	27.19%	5.284%
13	23.336	3478	3485	3495	rBV2	2513102	4439393	26.12%	5.077%




Sum of corrected areas: 87437817

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100121\
Data File : BM032305.D
Acq On : 30 Sep 2021 21:53
Operator : CG/JU
Sample : PB139476BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB139476BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

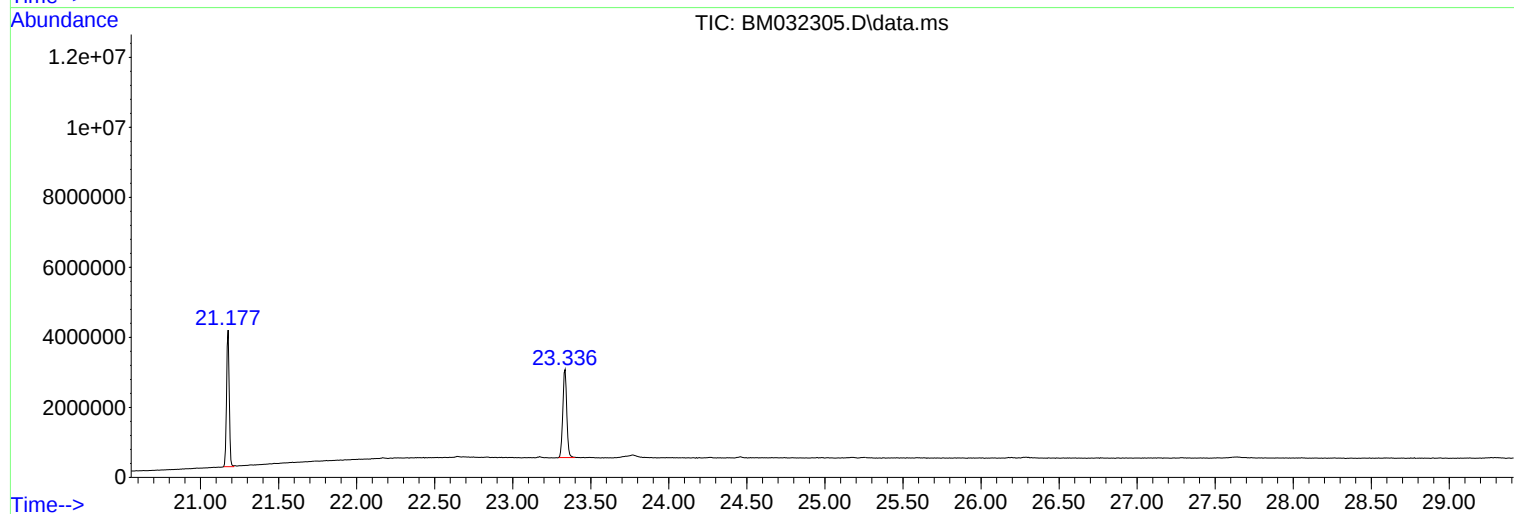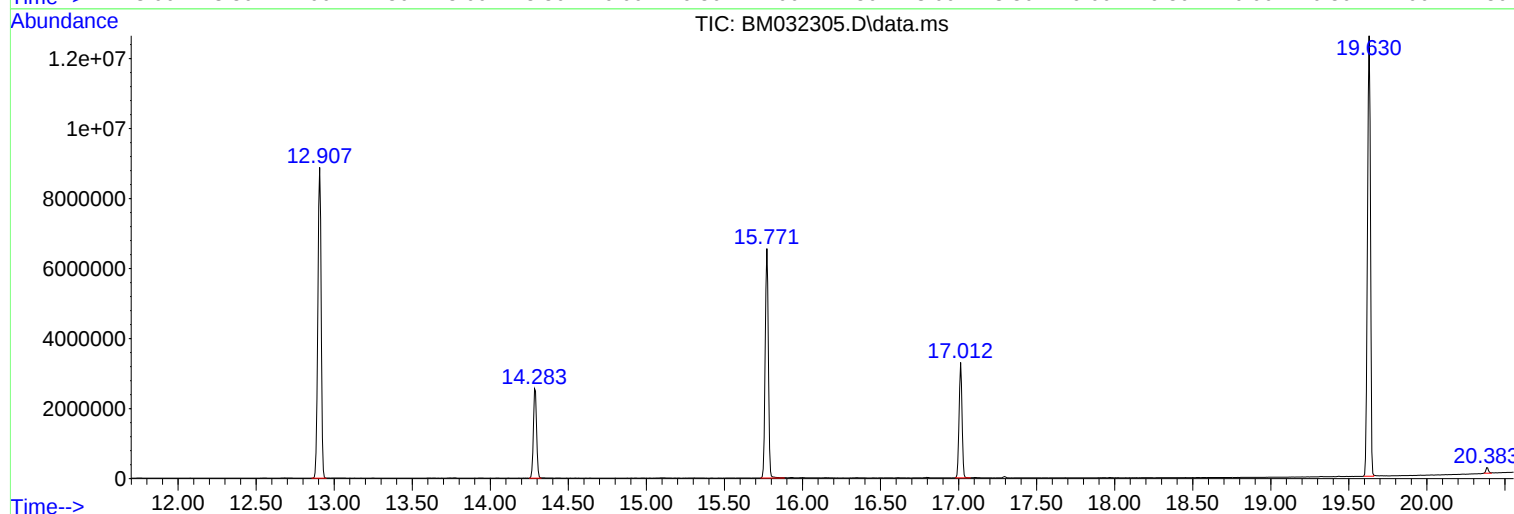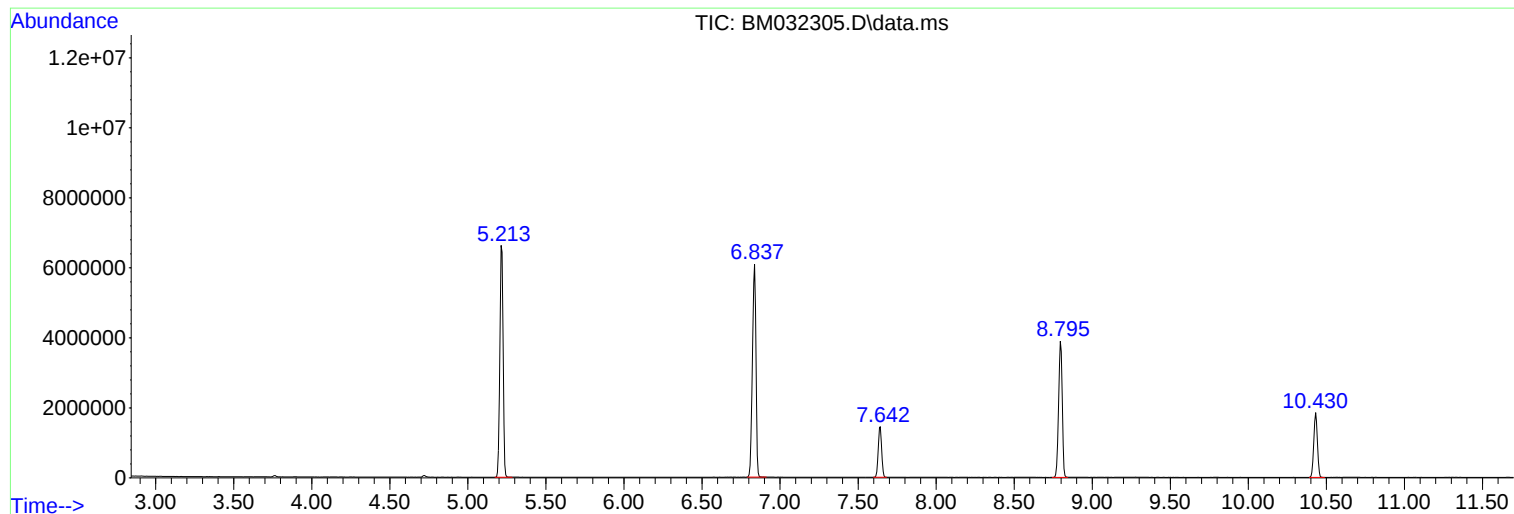

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100121\
Data File : BM032305.D
Acq On : 30 Sep 2021 21:53
Operator : CG/JU
Sample : PB139476BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB139476BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100121\
Data File : BM032305.D
Acq On : 30 Sep 2021 21:53
Operator : CG/JU
Sample : PB139476BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB139476BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------