
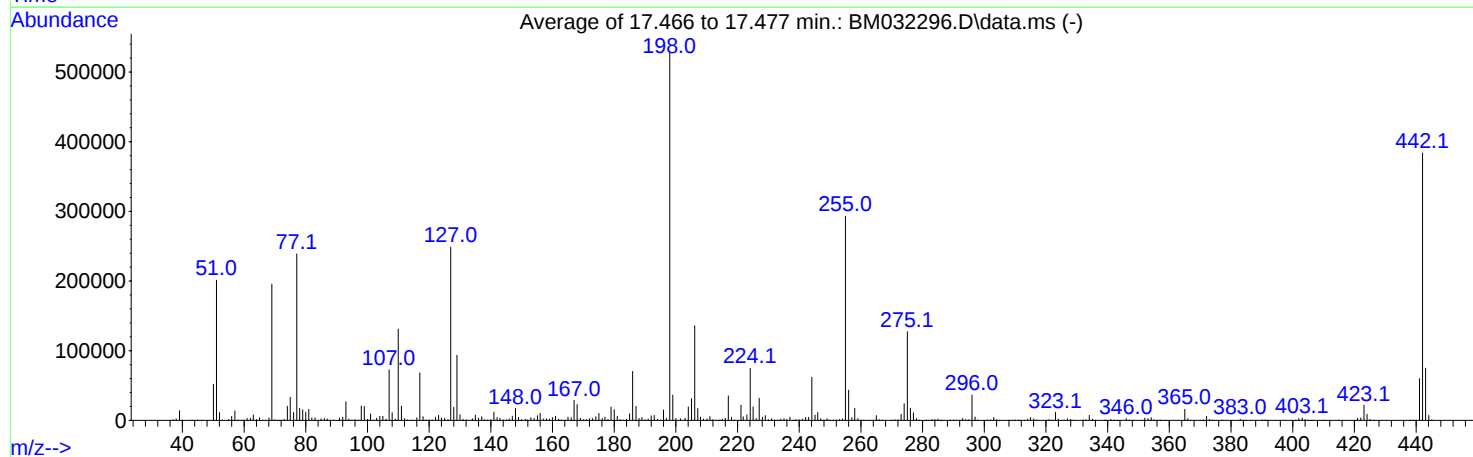


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100121\
 Data File : BM032296.D
 Acq On : 30 Sep 2021 15:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 01 10:39:43 2021

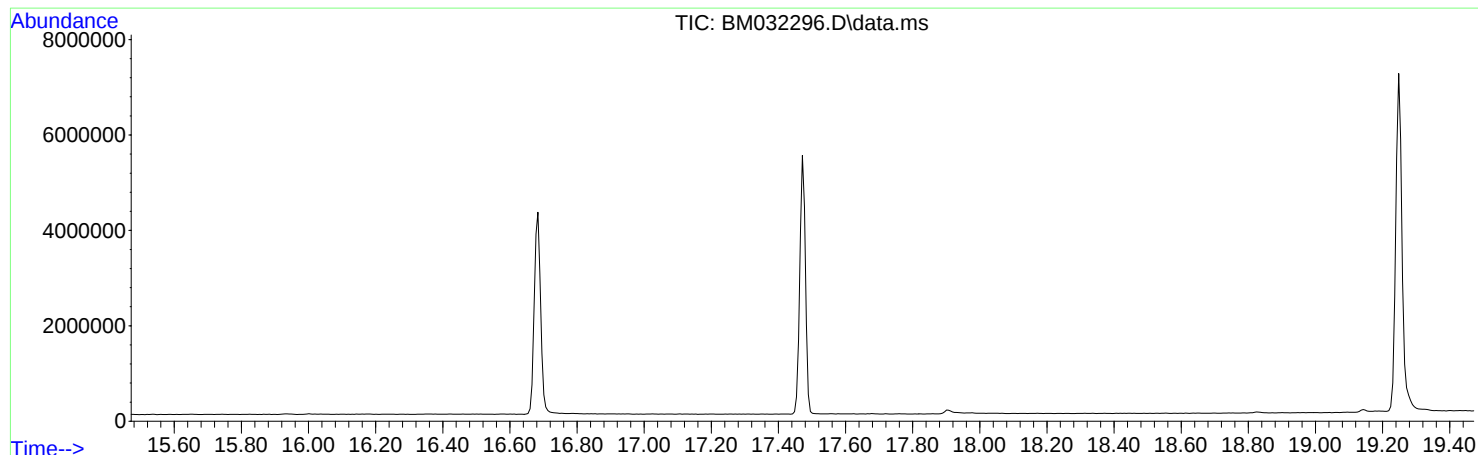




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	201263	PASS
68	69	0.00	2	1.7	3419	PASS
69	198	0.00	100	37.1	195686	PASS
70	69	0.00	2	0.5	900	PASS
127	198	10	80	47.1	248853	PASS
197	198	0.00	2	0.5	2739	PASS
198	198	100	100	100.0	528085	PASS
199	198	5	9	6.9	36248	PASS
275	198	10	60	24.1	127267	PASS
365	198	1	100	3.0	15912	PASS
441	198	0.01	100	11.3	59917	PASS
442	442	50	100	100.0	383808	PASS
443	442	15	24	19.5	74811	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100121\
 Data File : BM032296.D
 Acq On : 30 Sep 2021 15:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Sep 30 19:17:16 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 30 19:01:58 2021
 Response via : Initial Calibration

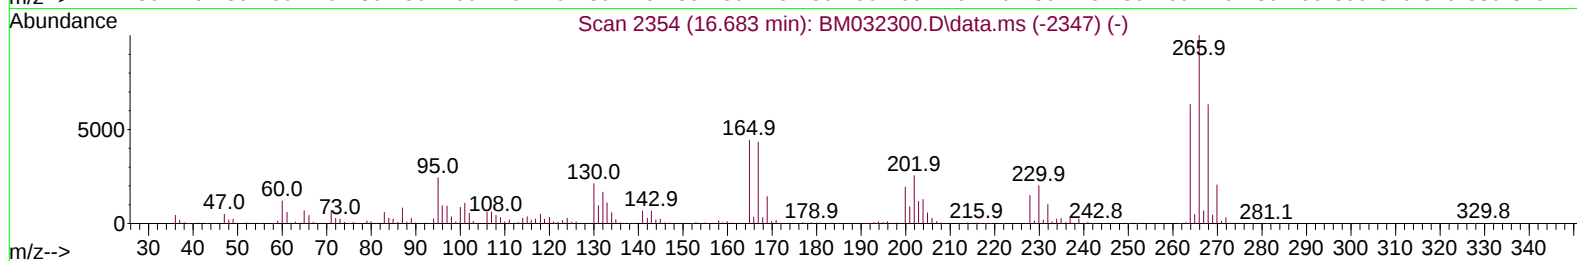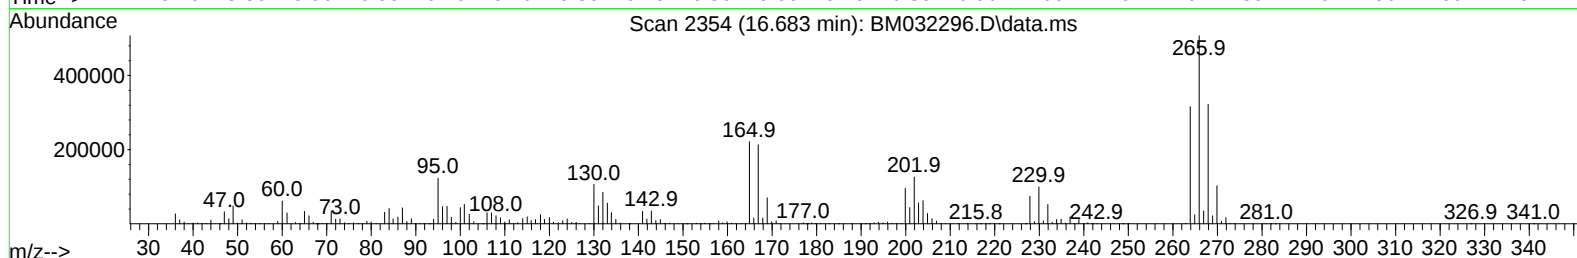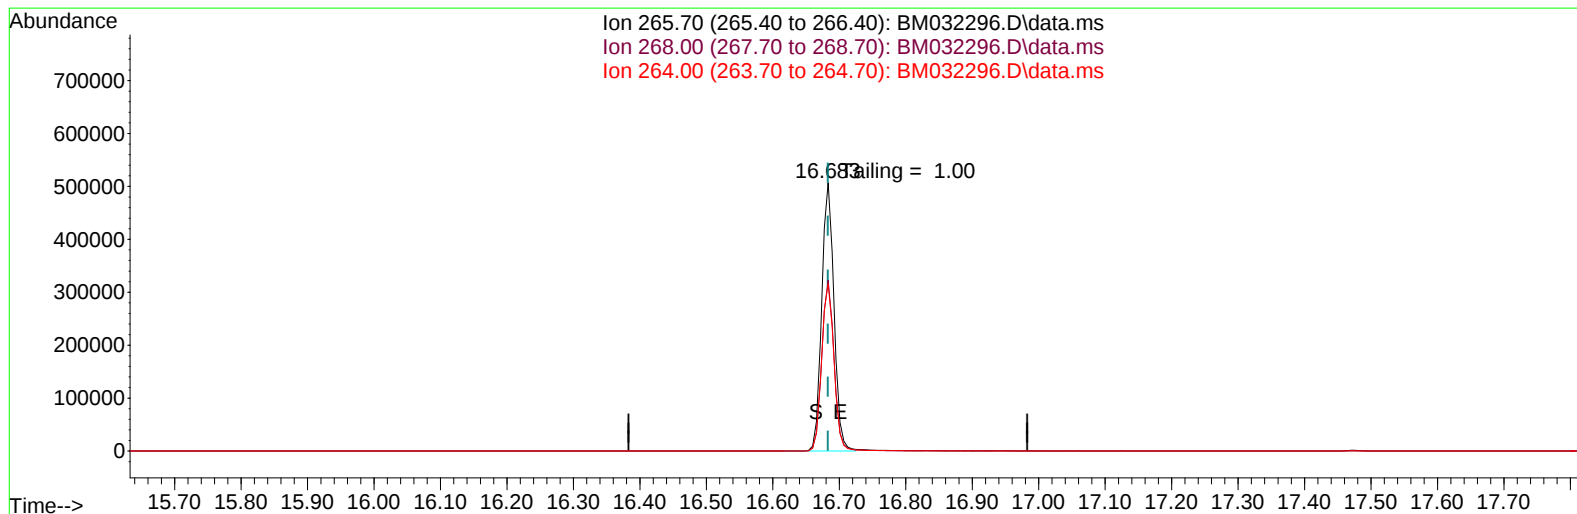

TIC: BM032296.D\data.ms

(70) Pentachlorophenol (C)

16.683min (+ 0.000) 0.00 ng




response 657619

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.62
264.00	65.10	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100121\
Data File : BM032296.D
Acq On : 30 Sep 2021 15:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 30 19:17:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 19:01:58 2021
Response via : Initial Calibration

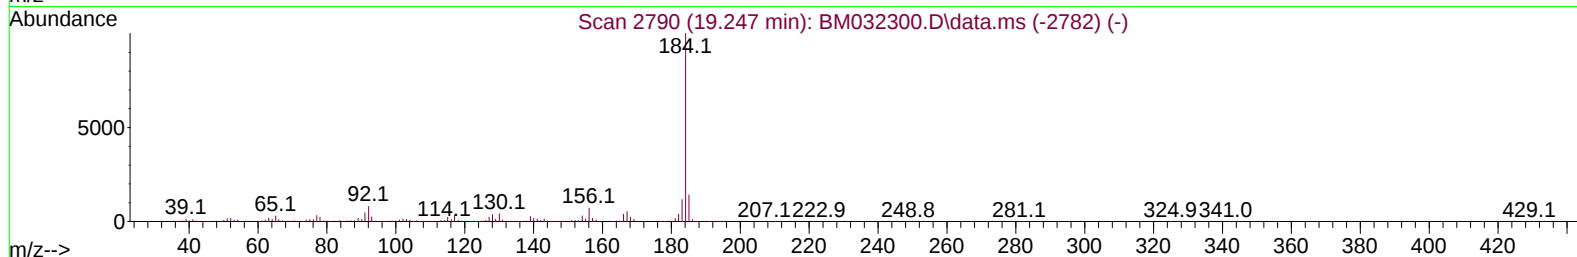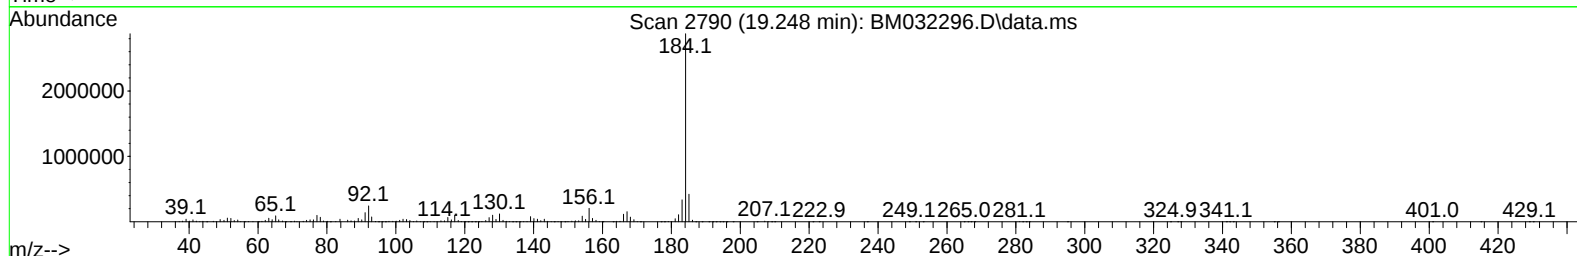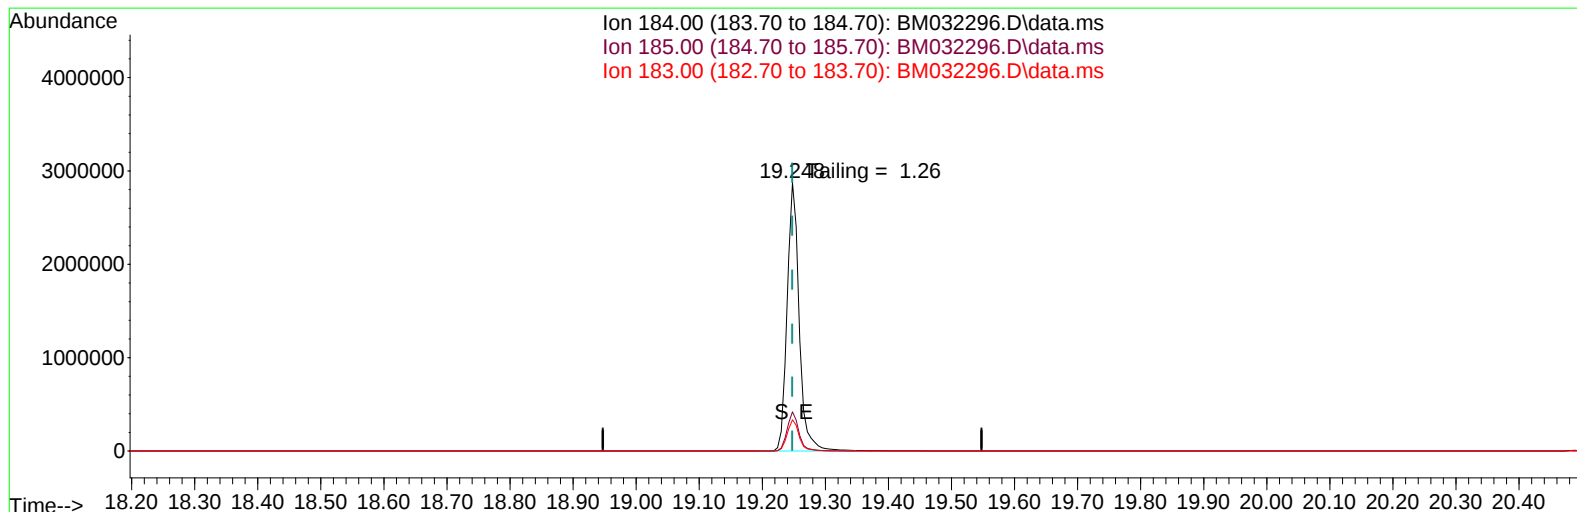

TIC: BM032296.D\data.ms

(77) Benzidine

19.248min (+ 0.000) 3305350.64 ng

response 3835494

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.62
183.00	11.20	11.67
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/1/2021	BNA_M	<u>BM032296.D</u>
Compound Name	Response	Retention Time
DDT	1583957	20.48
DDD	23565	20.04
DDE	615	19.54
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24180	1608137	1.50

Instrument :
BNA_M
ClientSampleId :
DFTPP