

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
 Data File : BM047740.D
 Acq On : 01 Oct 2024 13:05
 Operator : RC/JU
 Sample : P4018-14
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCE1

Quant Time: Oct 01 22:48:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 02:30:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	257204	20.000	ng/u1	0.00
20) Naphthalene-d8	10.604	136	1073961	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	665005	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.180	188	1322102	20.000	ng/u1	0.00
79) Chrysene-d12	21.403	240	1234870	20.000	ng/u1	0.00
88) Perylene-d12	24.409	264	1446851	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.257	96	35732	4.490	ng/uL	0.00
4) Pyridine-d5	3.669	84	558816	23.980	ng/u1	0.00
7) Phenol-d5	6.975	99	670702	27.577	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.139	67	411342	23.834	ng/u1	0.00
11) 2-Chlorophenol-d4	7.345	132	541009	30.574	ng/u1	0.00
15) 4-Methylphenol-d8	8.516	113	553417	30.605	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	268848	31.441	ng/u1	0.00
24) 2-Nitrophenol-d4	9.686	143	284530	34.723	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	528555	32.289	ng/u1	0.00
31) 4-Chloroaniline-d4	10.733	131	783488	30.959	ng/u1	0.00
46) Dimethylphthalate-d6	13.851	166	1616327	33.525	ng/u1	0.00
49) Acenaphthylene-d8	14.139	160	1889664	33.057	ng/u1	0.00
54) 4-Nitrophenol-d4	14.633	143	228249	23.778	ng/u1	0.00
60) Fluorene-d10	15.433	176	1422318	34.058	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.545	200	145682	18.830	ng/u1	0.00
73) Anthracene-d10	17.280	188	2175779	33.469	ng/u1	0.00
81) Pyrene-d10	19.568	212	2516989	35.913	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.203	264	2639486	35.161	ng/u1	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.833	266	37487	3.717	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047740.D
Acq On : 01 Oct 2024 13:05
Operator : RC/JU
Sample : P4018-14
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCE1

Quant Time: Oct 01 22:48:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

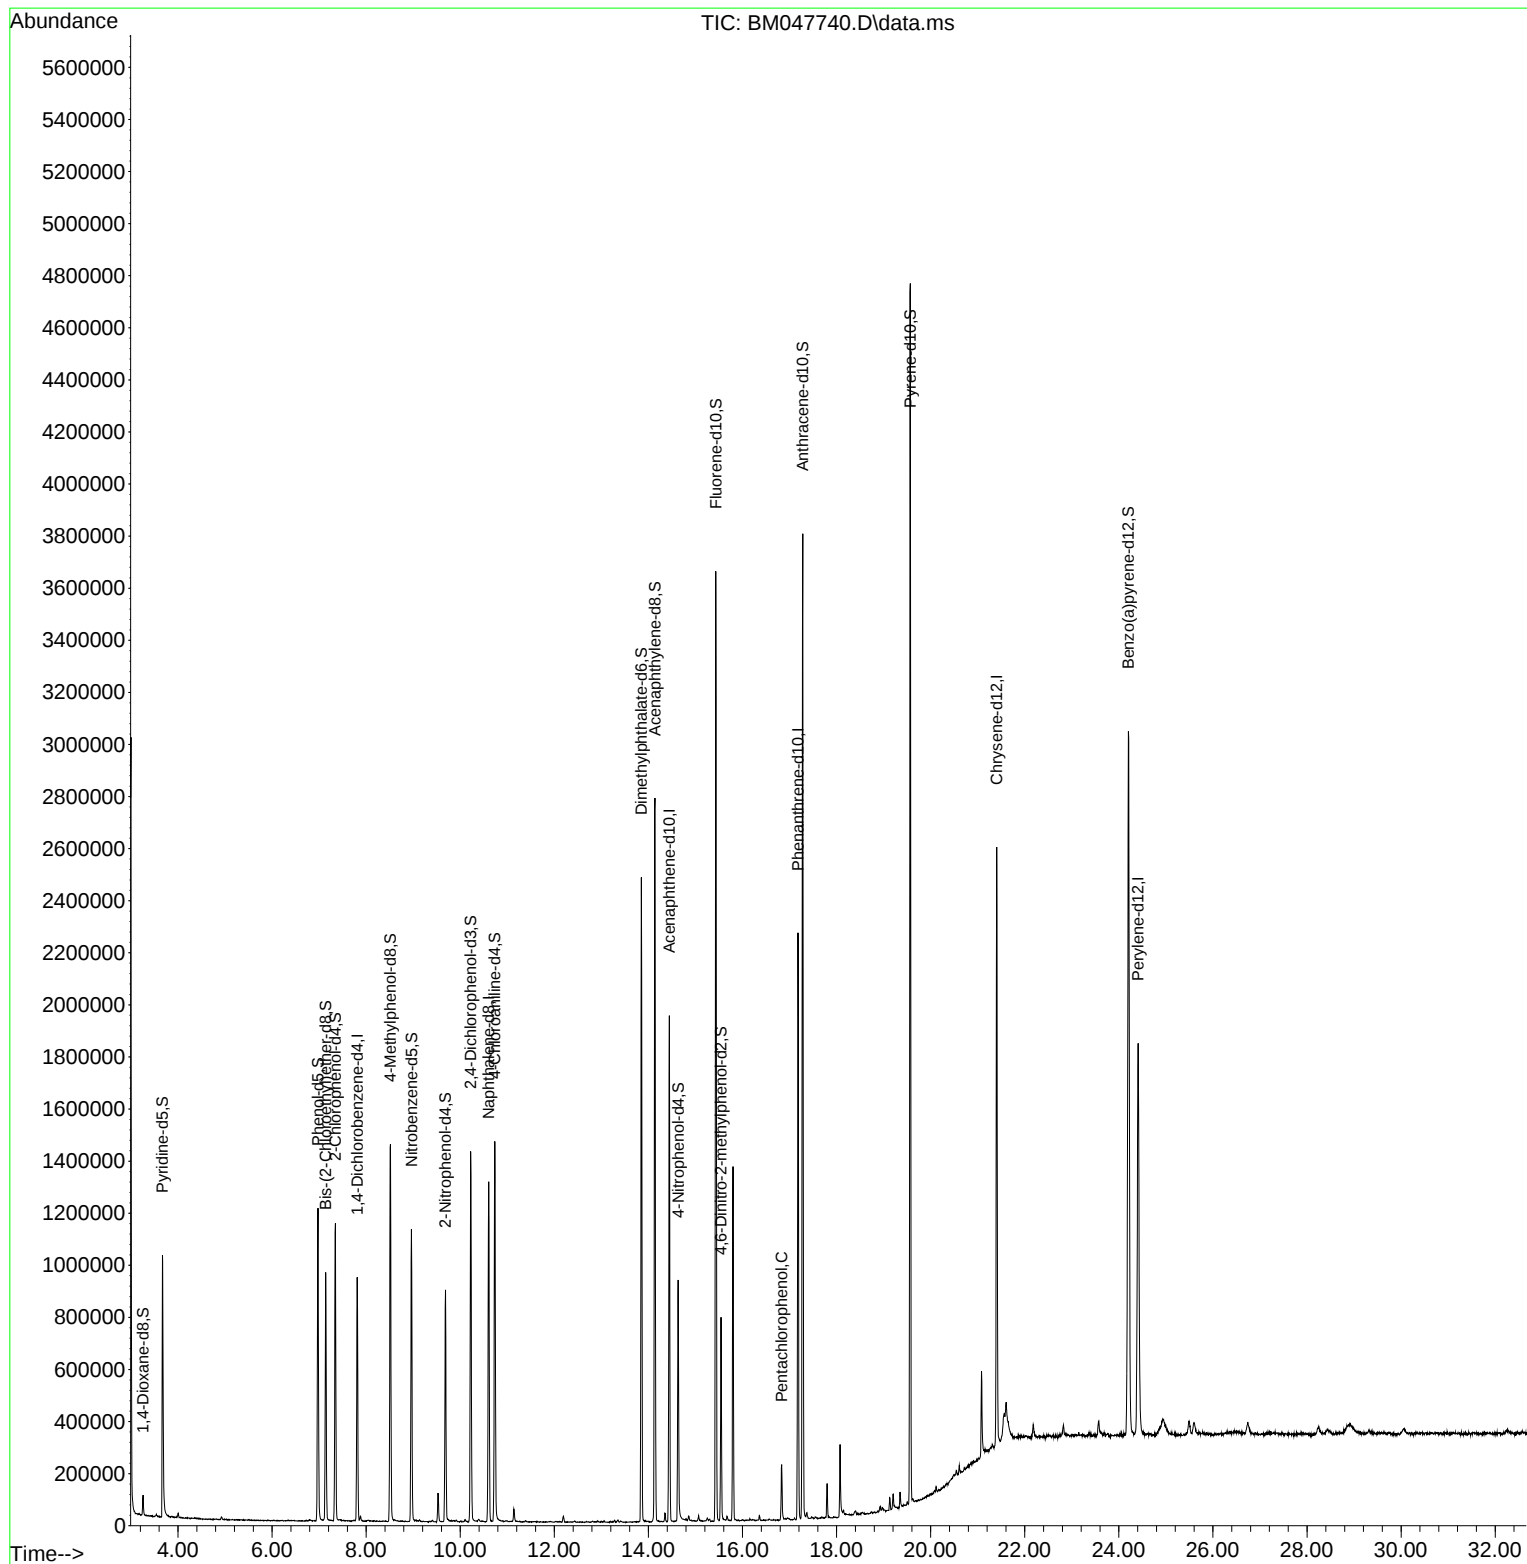

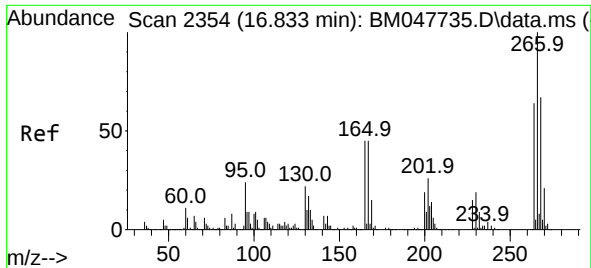

#71
Pentachlorophenol
Concen: 3.717 ng/ul
RT: 16.833 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM047740.D
Acq: 01 Oct 2024 13:05

Instrument :
BNA_M
ClientSampleId :
DDCE1

Tgt Ion:266 Resp: 37487
Ion Ratio Lower Upper
266 100
264 64.7 50.2 75.2
268 64.8 50.9 76.3

