

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
 Data File : BM047742.D
 Acq On : 01 Oct 2024 14:24
 Operator : RC/JU
 Sample : P4018-22
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCF7

Quant Time: Oct 01 22:49:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 02:30:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	281827	20.000	ng/ul	0.00
20) Naphthalene-d8	10.604	136	1166538	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.445	164	722504	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.180	188	1468866	20.000	ng/ul	0.00
79) Chrysene-d12	21.403	240	1356610	20.000	ng/ul	0.00
88) Perylene-d12	24.409	264	1590933	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	22567	2.588	ng/uL	0.00
4) Pyridine-d5	3.681	84	91322	3.576	ng/ul	0.00
7) Phenol-d5	6.975	99	369798	13.876	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	230692	12.199	ng/ul	0.00
11) 2-Chlorophenol-d4	7.346	132	310107	15.994	ng/ul	0.00
15) 4-Methylphenol-d8	8.510	113	303364	15.311	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	143922	15.495	ng/ul	0.00
24) 2-Nitrophenol-d4	9.687	143	149782	16.828	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	296018	16.648	ng/ul	0.00
31) 4-Chloroaniline-d4	10.734	131	440034	16.008	ng/ul	0.00
46) Dimethylphthalate-d6	13.851	166	944865	18.038	ng/ul	0.00
49) Acenaphthylene-d8	14.133	160	1089012	17.534	ng/ul	0.00
54) 4-Nitrophenol-d4	14.627	143	116986	11.217	ng/ul	0.00
60) Fluorene-d10	15.433	176	836933	18.446	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.545	200	86256	10.035	ng/ul	0.00
73) Anthracene-d10	17.274	188	1316975	18.234	ng/ul	-0.01
81) Pyrene-d10	19.562	212	1542130	20.029	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.203	264	1591784	19.284	ng/ul	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.833	266	12071	1.077	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047742.D
Acq On : 01 Oct 2024 14:24
Operator : RC/JU
Sample : P4018-22
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCF7


Quant Time: Oct 01 22:49:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

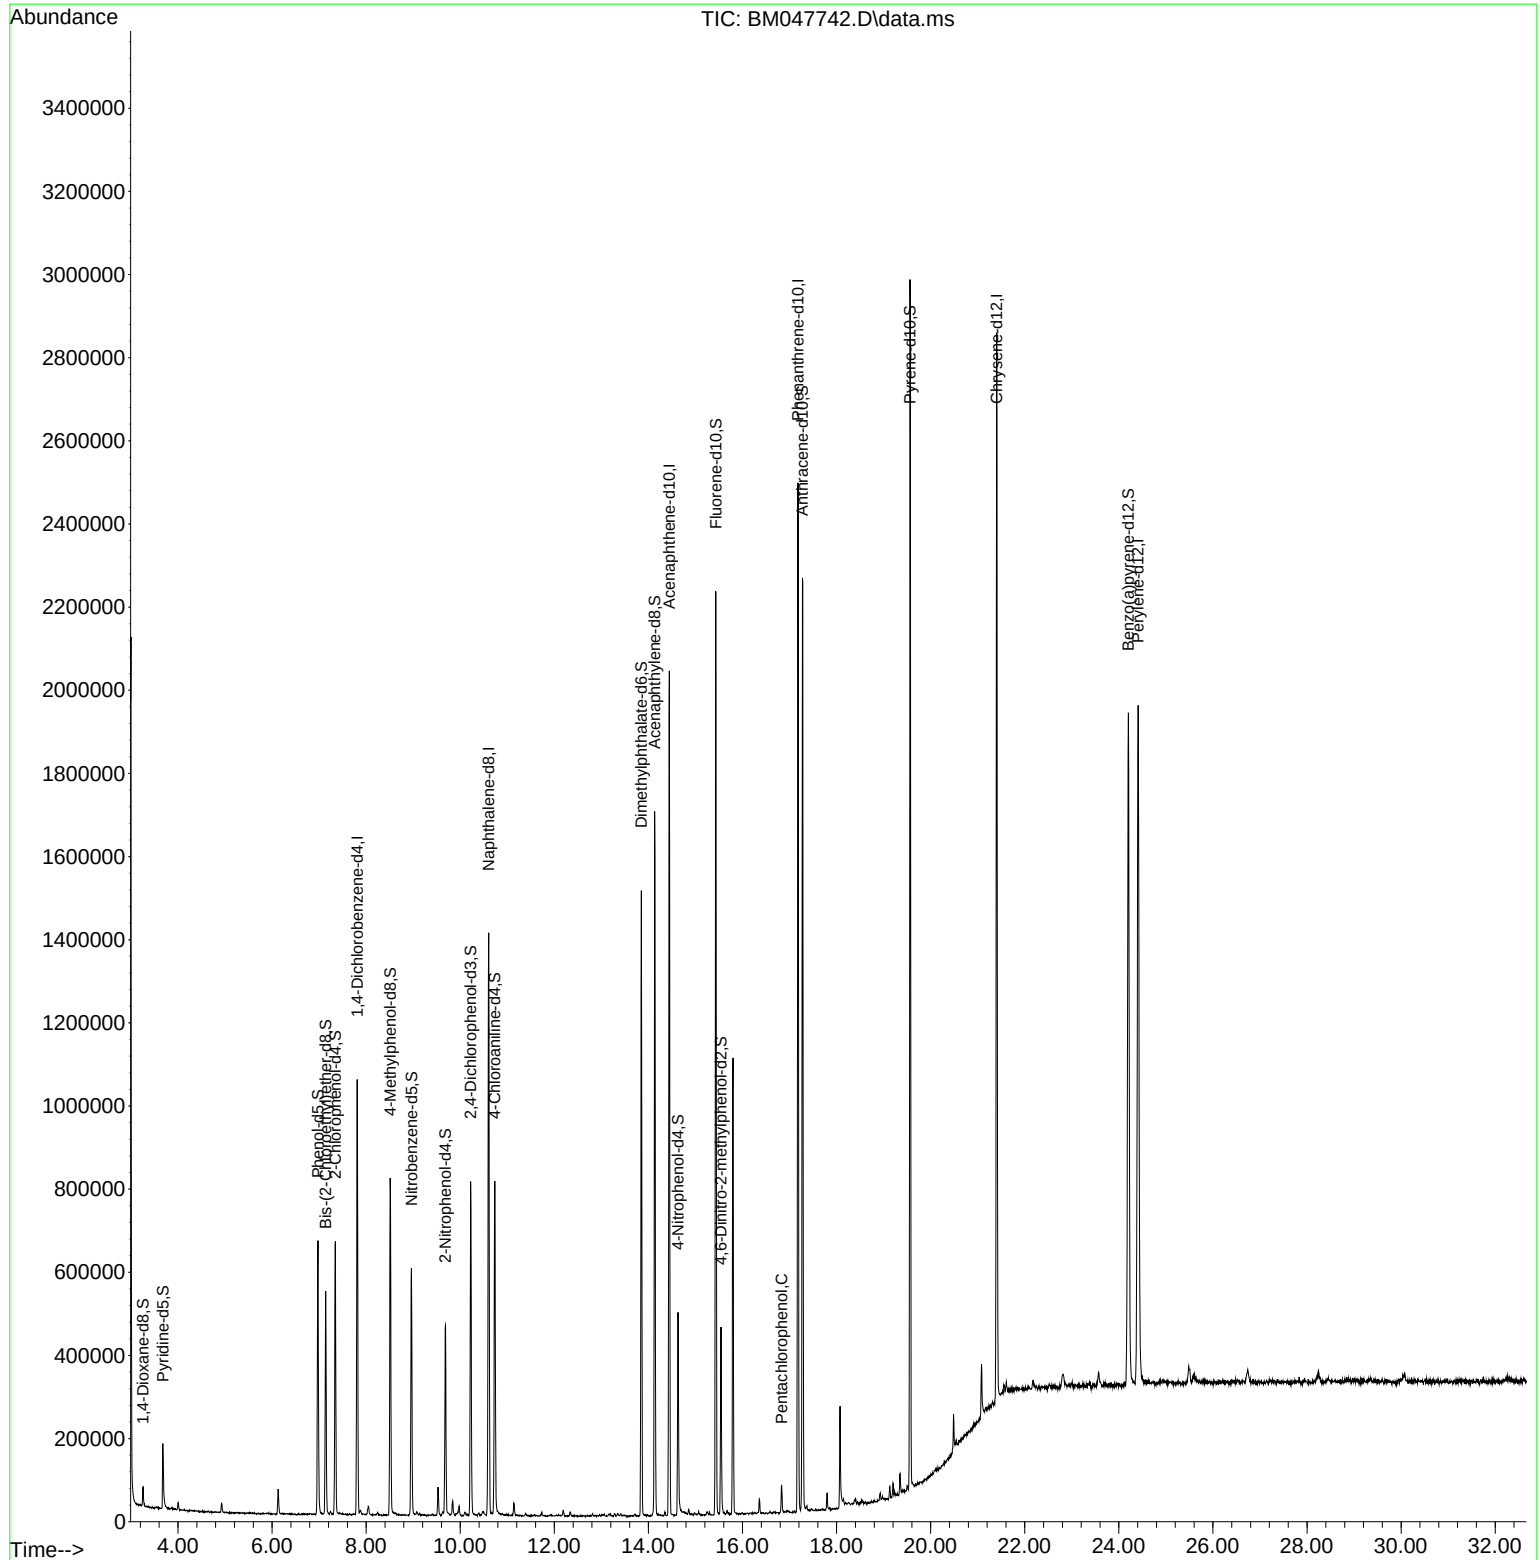

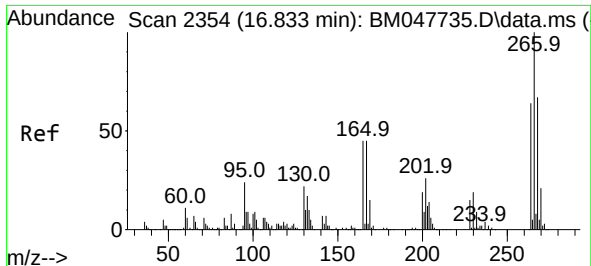

#71
 Pentachlorophenol
 Concen: 1.077 ng/ul
 RT: 16.833 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BM047742.D
 Acq: 01 Oct 2024 14:24

Instrument :
 BNA_M
 ClientSampleId :
 DDCF7

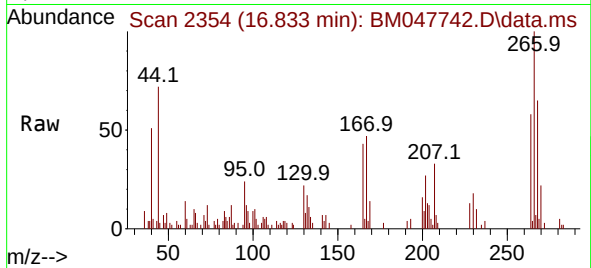

Tgt Ion:	266	Resp:	12071
Ion	Ratio	Lower	Upper
266	100		
264	57.9	50.2	75.2
268	70.3	50.9	76.3

