

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
 Data File : BM047744.D
 Acq On : 01 Oct 2024 15:43
 Operator : RC/JU
 Sample : P4018-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCA2

Quant Time: Oct 01 23:09:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 02:30:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	318437	20.000	ng/u1	0.00
20) Naphthalene-d8	10.604	136	1317450	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	800483	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	1531442	20.000	ng/u1	0.00
79) Chrysene-d12	21.403	240	1465894	20.000	ng/u1	0.00
88) Perylene-d12	24.409	264	1678658	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.257	96	27929	2.834	ng/uL	0.00
4) Pyridine-d5	3.675	84	371266	12.868	ng/u1	0.00
7) Phenol-d5	6.975	99	554478	18.414	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	335203	15.688	ng/u1	0.00
11) 2-Chlorophenol-d4	7.345	132	432786	19.755	ng/u1	0.00
15) 4-Methylphenol-d8	8.516	113	430364	19.223	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	204995	19.543	ng/u1	0.00
24) 2-Nitrophenol-d4	9.686	143	220426	21.928	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	413830	20.608	ng/u1	0.00
31) 4-Chloroaniline-d4	10.739	131	435396	14.025	ng/u1	0.00
46) Dimethylphthalate-d6	13.851	166	1187264	20.458	ng/u1	0.00
49) Acenaphthylene-d8	14.139	160	1417019	20.593	ng/u1	0.00
54) 4-Nitrophenol-d4	14.639	143	204841	17.728	ng/u1	0.00
60) Fluorene-d10	15.439	176	1021544	20.322	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.545	200	142452	15.895	ng/u1	0.00
73) Anthracene-d10	17.286	188	1499790	19.917	ng/u1	0.00
81) Pyrene-d10	19.568	212	1806330	21.712	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.203	264	1829490	21.005	ng/u1	0.00
Target Compounds						
					Qvalue	
23) Isophorone	9.533	82	373061	6.999	ng/u1#	89
30) Naphthalene	10.657	128	276033	3.643	ng/u1	98
36) 2-Methylnaphthalene	12.269	142	544702	11.313	ng/u1	98
37) 1-Methylnaphthalene	12.486	142	335119	6.841	ng/u1	99
41) 2,4,6-Trichlorophenol	12.874	196	17497	1.161	ng/u1#	96
58) 2,3,4,6-Tetrachlorophenol	15.074	232	2136766	164.419	ng/u1#	95
71) Pentachlorophenol	16.874	266	13824105	1183.434	ng/u1	99
72) Phenanthrene	17.227	178	181942	2.026	ng/u1#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047744.D
Acq On : 01 Oct 2024 15:43
Operator : RC/JU
Sample : P4018-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCA2

Quant Time: Oct 01 23:09:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

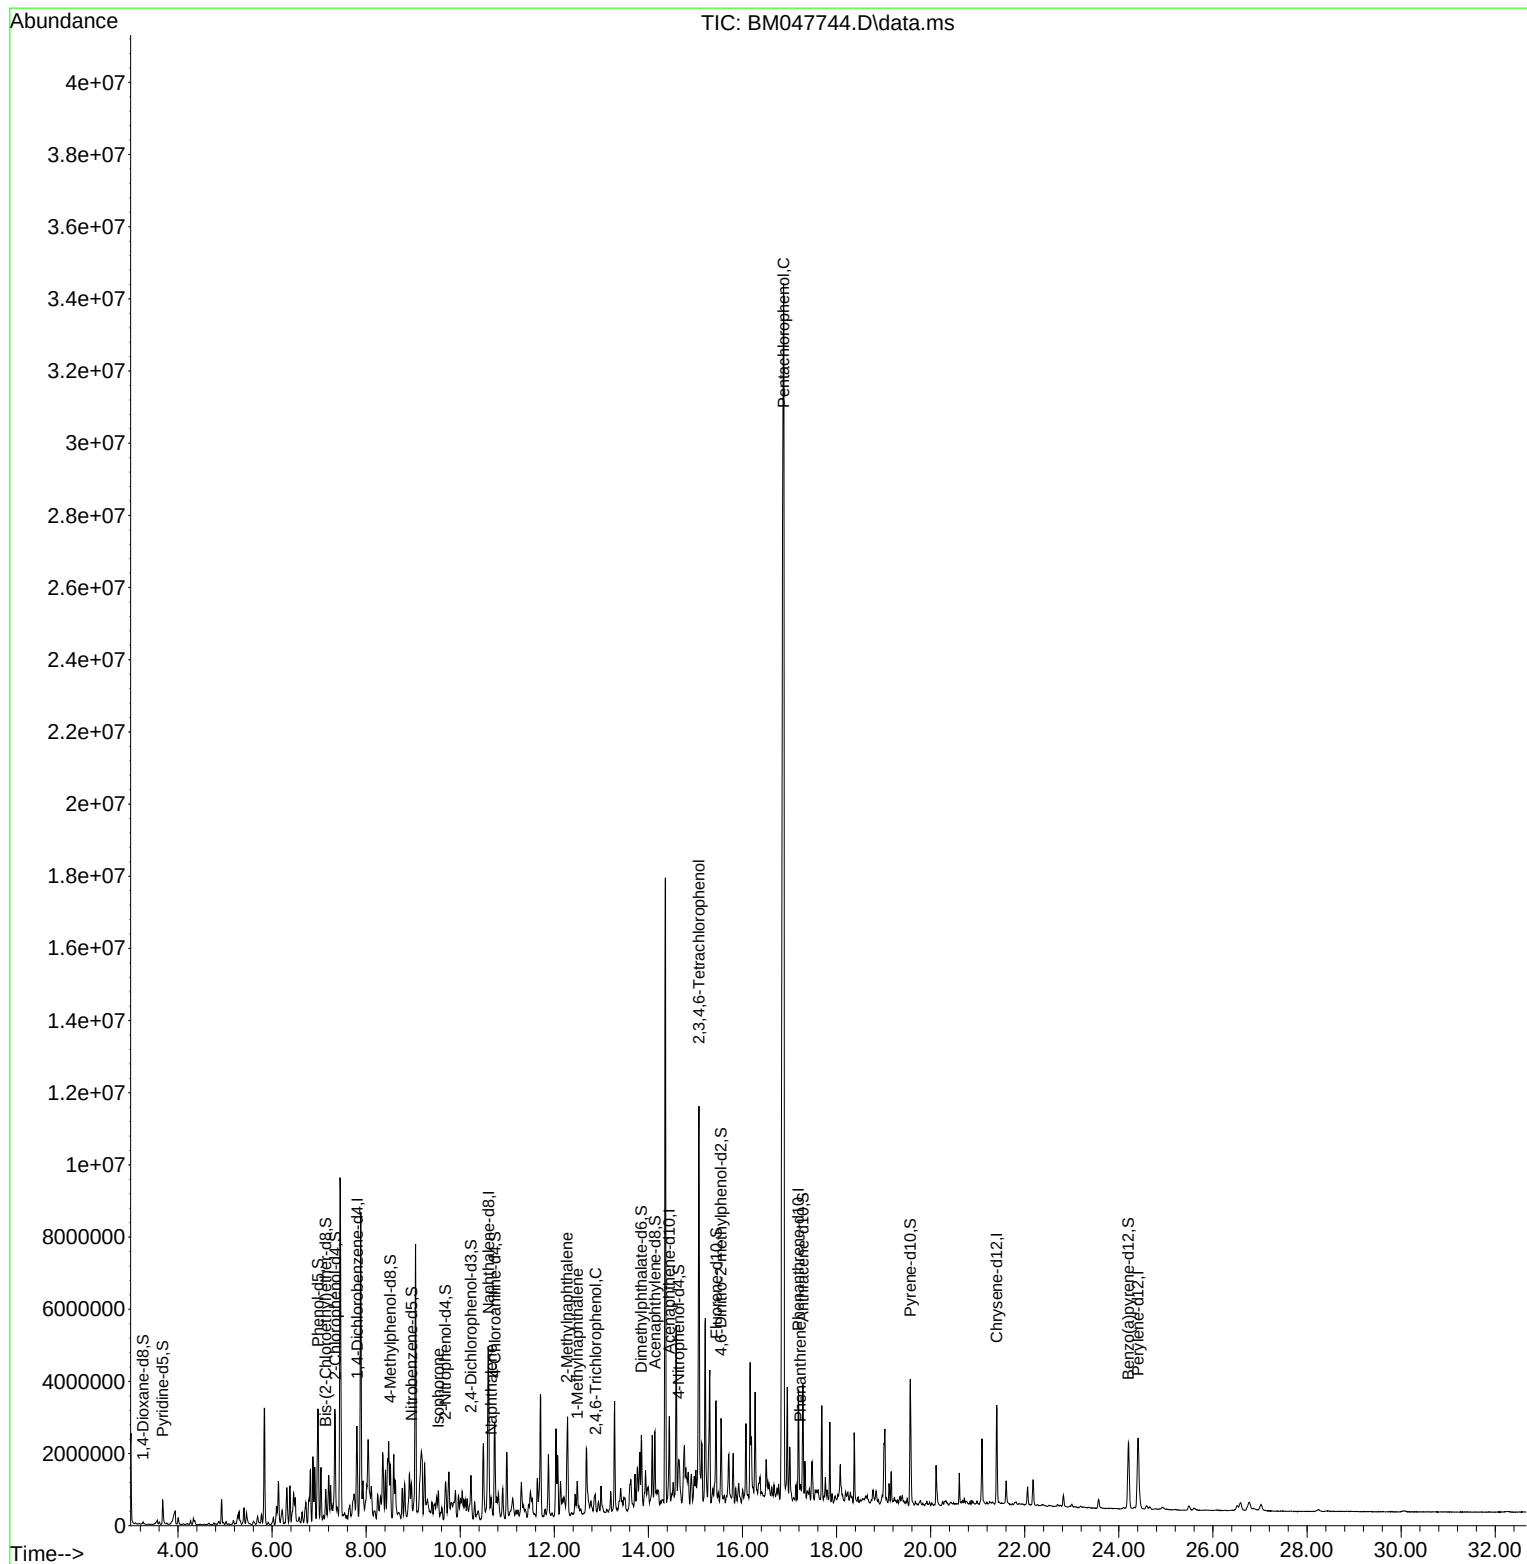

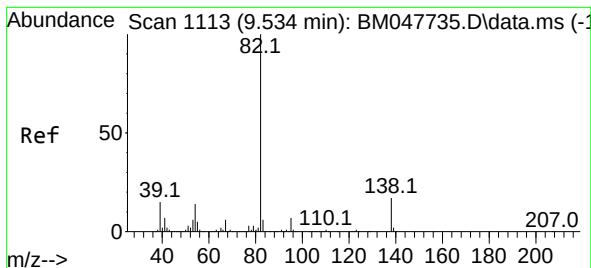

#23

Isophorone

Concen: 6.999 ng/ul

RT: 9.533 min Scan# 1113

Delta R.T. -0.006 min

Lab File: BM047744.D

Acq: 01 Oct 2024 15:43

Instrument :

BNA_M

ClientSampleId :

DDCA2





Tgt Ion: 82 Resp: 373061

Ion Ratio Lower Upper

82 100

95 14.6 4.9 7.3#

138 17.1 12.0 18.0

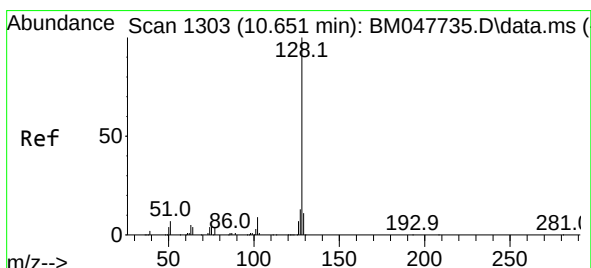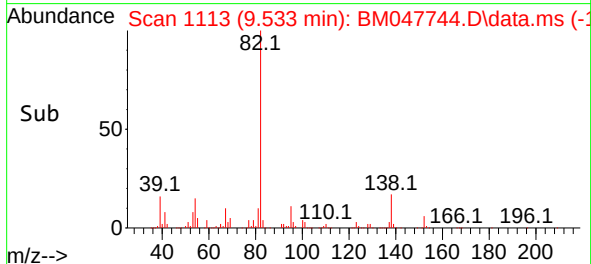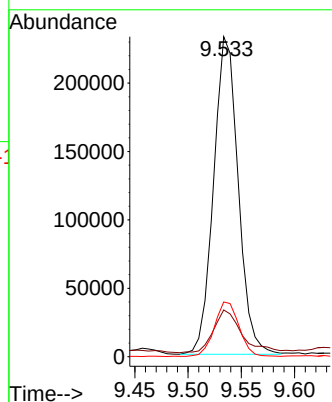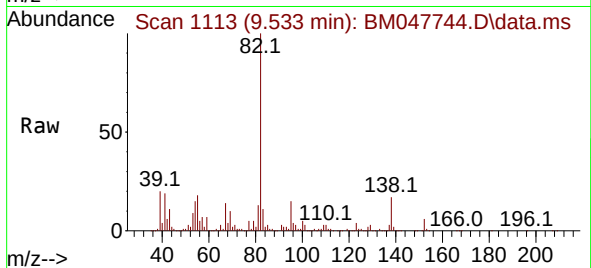

#30

Naphthalene

Concen: 3.643 ng/ul

RT: 10.657 min Scan# 1304

Delta R.T. -0.006 min

Lab File: BM047744.D

Acq: 01 Oct 2024 15:43




Tgt Ion: 128 Resp: 276033


Ion Ratio Lower Upper

128 100

129 12.0 8.6 12.8

127 13.2 10.4 15.6


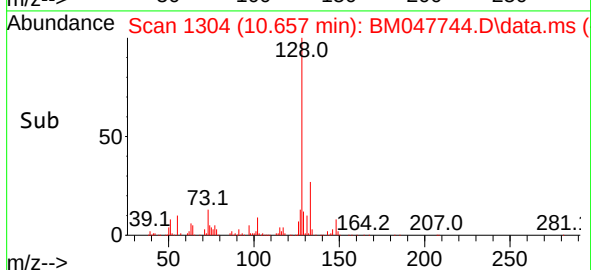
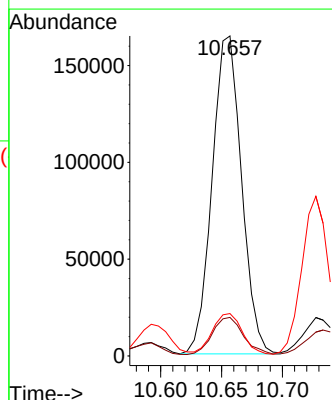
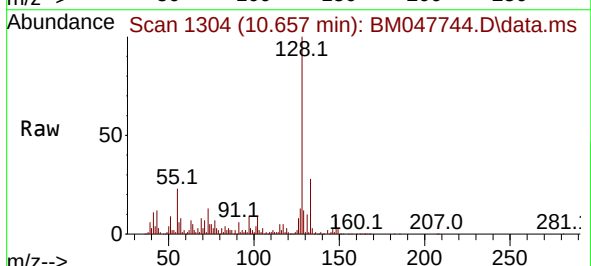


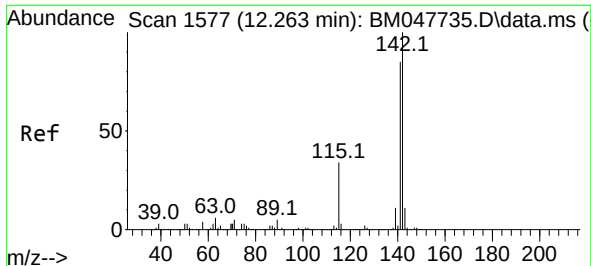

#36
2-Methylnaphthalene
Concen: 11.313 ng/ul
RT: 12.269 min Scan# 11
Delta R.T. -0.000 min
Lab File: BM047744.D
Acq: 01 Oct 2024 15:43




Instrument :
BNA_M
ClientSampleId :
DDCA2


Tgt Ion:142 Resp: 544702
Ion Ratio Lower Upper
142 100
141 88.9 72.5 108.7

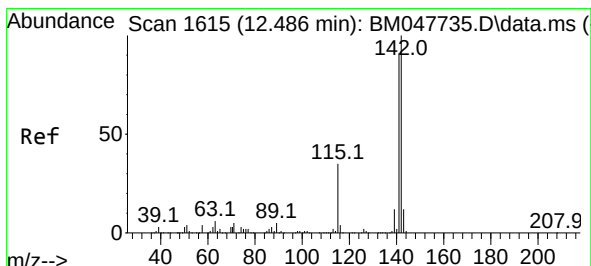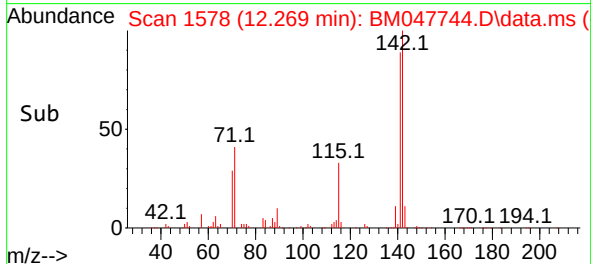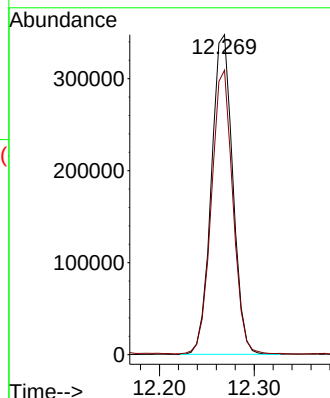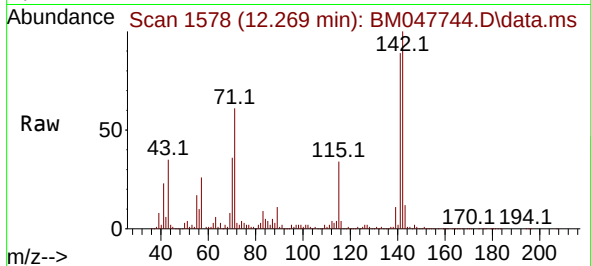

#37
1-Methylnaphthalene
Concen: 6.841 ng/ul
RT: 12.486 min Scan# 1615
Delta R.T. -0.006 min
Lab File: BM047744.D
Acq: 01 Oct 2024 15:43

Tgt Ion:142 Resp: 335119
Ion Ratio Lower Upper
142 100
141 92.5 73.4 110.2
116 3.9 3.0 4.6


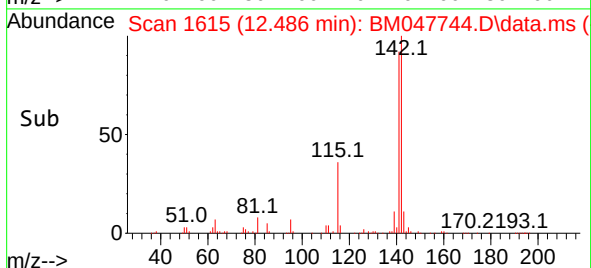
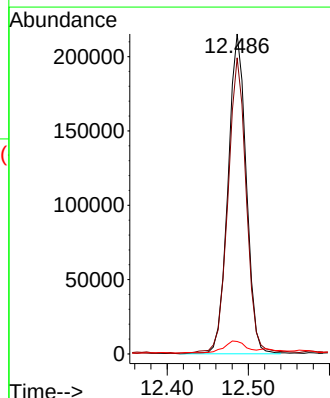
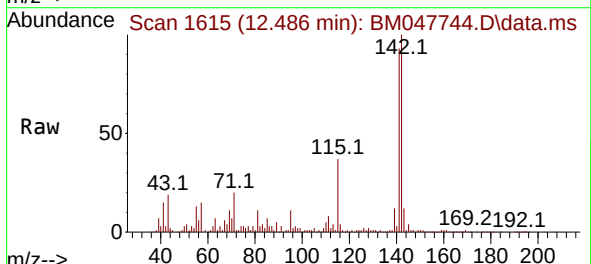


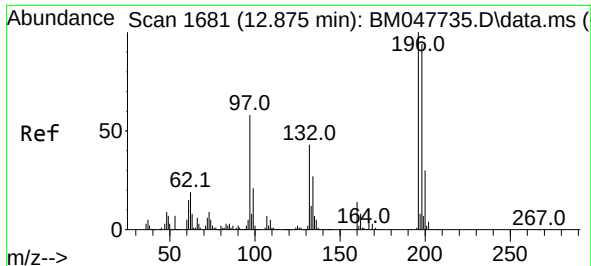

#41
2,4,6-Trichlorophenol
Concen: 1.161 ng/ul
RT: 12.874 min Scan# 1
Delta R.T. -0.006 min
Lab File: BM047744.D
Acq: 01 Oct 2024 15:43




Instrument :
BNA_M
ClientSampleId :
DDCA2


Tgt Ion:196 Resp: 17497
Ion Ratio Lower Upper
196 100
198 98.6 77.1 115.7
200 36.9 24.5 36.7#

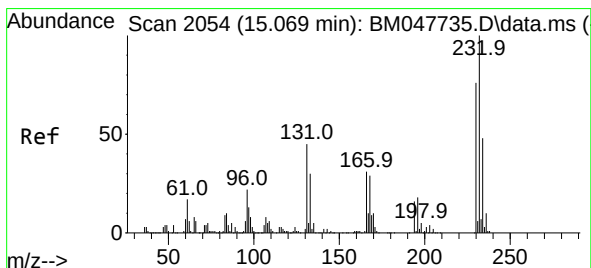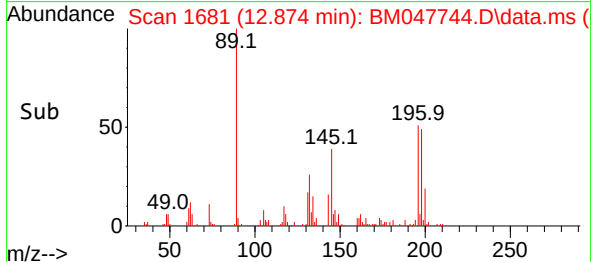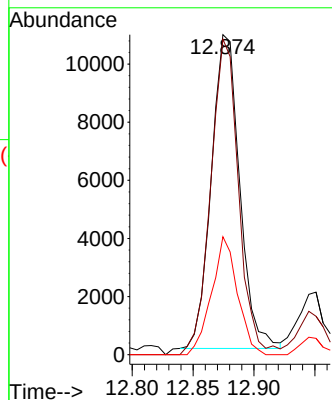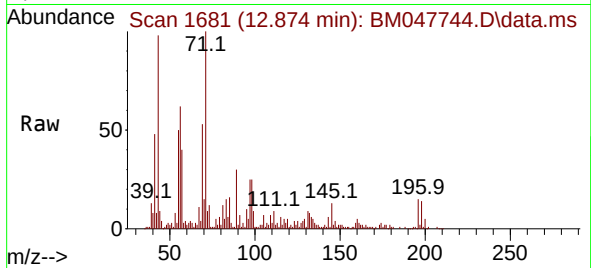

#58
2,3,4,6-Tetrachlorophenol
Concen: 164.419 ng/ul
RT: 15.074 min Scan# 2055
Delta R.T. 0.006 min
Lab File: BM047744.D
Acq: 01 Oct 2024 15:43

Tgt Ion:232 Resp: 2136766
Ion Ratio Lower Upper
232 100
131 45.8 40.2 60.4
130 2.5 2.6 4.0#
166 30.4 25.3 37.9


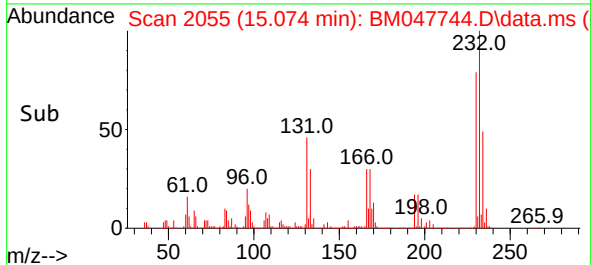
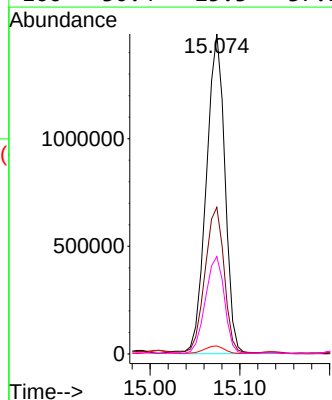
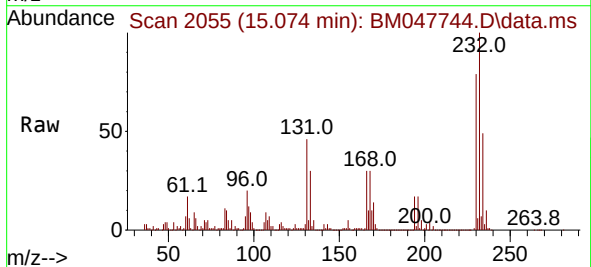


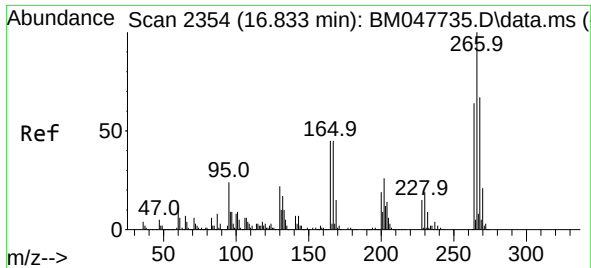

#71
 Pentachlorophenol
 Concen: 1183.434 ng/ul
 RT: 16.874 min Scan# 21
 Delta R.T. 0.035 min
 Lab File: BM047744.D
 Acq: 01 Oct 2024 15:43

Instrument :
 BNA_M
 ClientSampleId :
 DDCA2

Tgt Ion:266 Resp:13824105
 Ion Ratio Lower Upper
 266 100
 264 64.5 50.2 75.2
 268 63.9 50.9 76.3

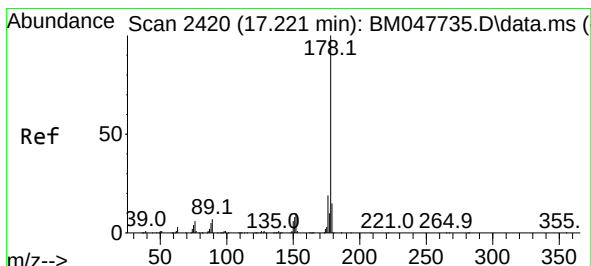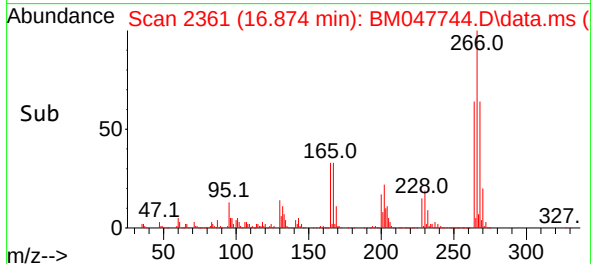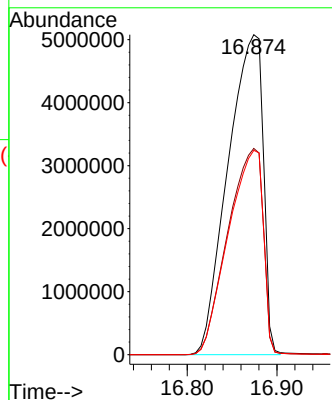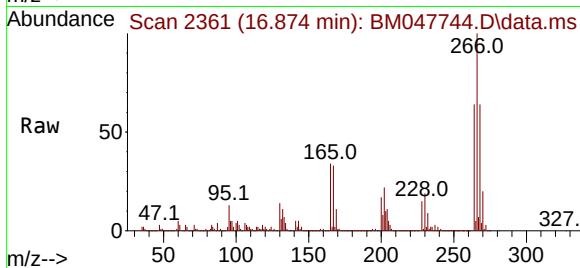

#72
 Phenanthrene
 Concen: 2.026 ng/ul
 RT: 17.227 min Scan# 2421
 Delta R.T. -0.000 min
 Lab File: BM047744.D
 Acq: 01 Oct 2024 15:43

Tgt Ion:178 Resp: 181942
 Ion Ratio Lower Upper
 178 100
 179 18.3 12.0 18.0#
 176 19.8 15.4 23.0

