

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
 Data File : BM047758.D
 Acq On : 02 Oct 2024 01:35
 Operator : RC/JU
 Sample : P4018-11DL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCB7DL

Quant Time: Oct 02 02:18:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 02:30:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	224357	20.000	ng/u1	0.00
20) Naphthalene-d8	10.604	136	919495	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.439	164	567093	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.180	188	1161706	20.000	ng/u1	0.00
79) Chrysene-d12	21.403	240	1034312	20.000	ng/u1	0.00
88) Perylene-d12	24.403	264	1201799	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	3496	0.504	ng/uL	0.00
4) Pyridine-d5	3.681	84	37677	1.853	ng/u1	0.00
7) Phenol-d5	6.975	99	47244	2.227	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	28673	1.905	ng/u1	0.00
11) 2-Chlorophenol-d4	7.346	132	34529	2.237	ng/u1	0.00
15) 4-Methylphenol-d8	8.510	113	35215	2.233	ng/u1	0.00
21) Nitrobenzene-d5	8.957	128	14656	2.002	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.687	143	12926	1.842	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	31650	2.258	ng/u1	0.00
31) 4-Chloroaniline-d4	10.734	131	48801	2.252	ng/u1	0.00
46) Dimethylphthalate-d6	13.851	166	121308	2.950	ng/u1	0.00
49) Acenaphthylene-d8	14.133	160	131076	2.689	ng/u1	0.00
54) 4-Nitrophenol-d4	14.639	143	6514	0.796	ng/u1	0.00
60) Fluorene-d10	15.433	176	102797	2.887	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.539	200	6764	0.995	ng/u1	-0.01
73) Anthracene-d10	17.274	188	157956	2.765	ng/u1	-0.01
81) Pyrene-d10	19.562	212	181350	3.089	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.197	264	168630	2.704	ng/u1	-0.01
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	15.069	232	14973	1.626	ng/u1	92
71) Pentachlorophenol	16.833	266	278263	31.403	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047758.D
Acq On : 02 Oct 2024 01:35
Operator : RC/JU
Sample : P4018-11DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCB7DL

Quant Time: Oct 02 02:18:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration




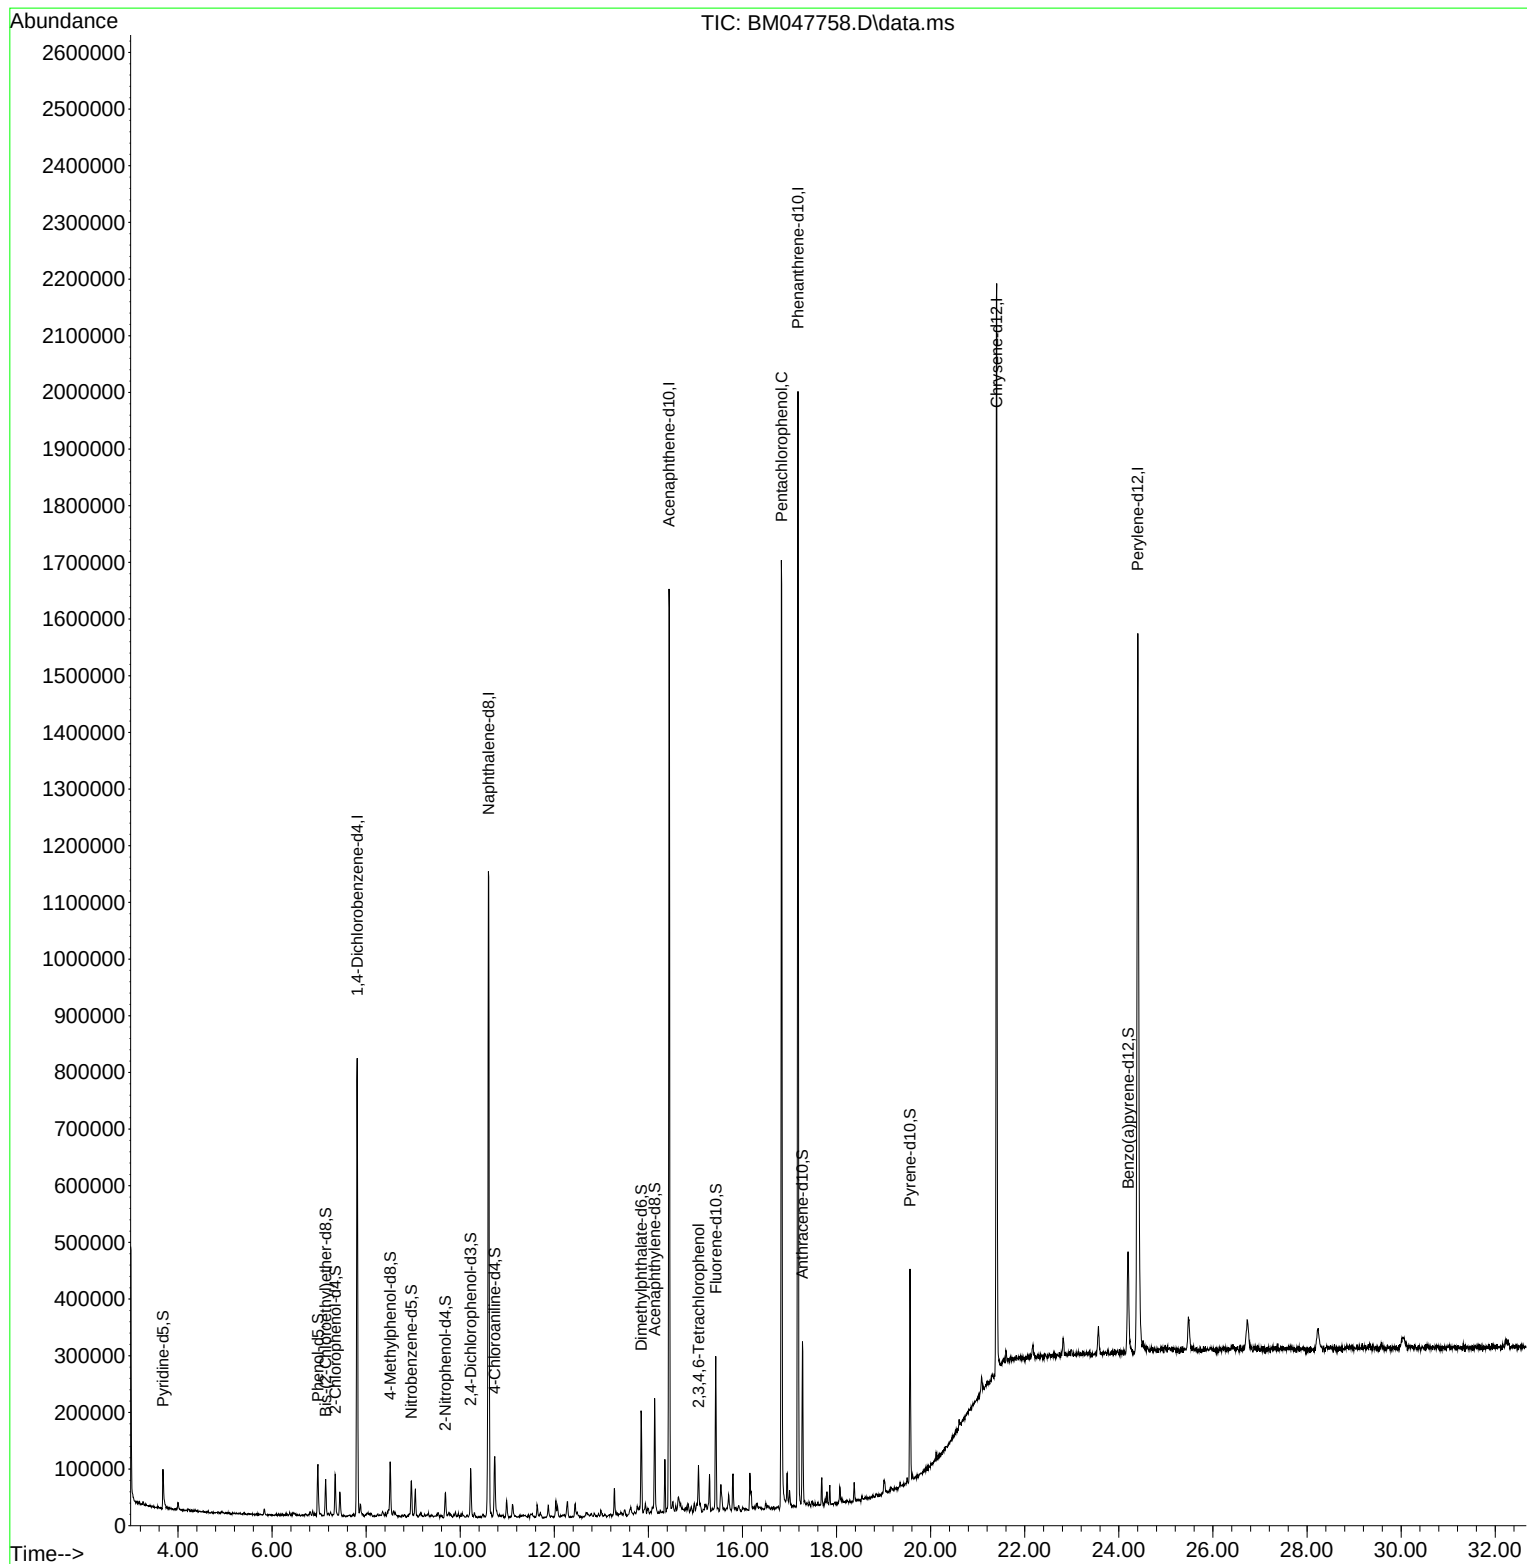


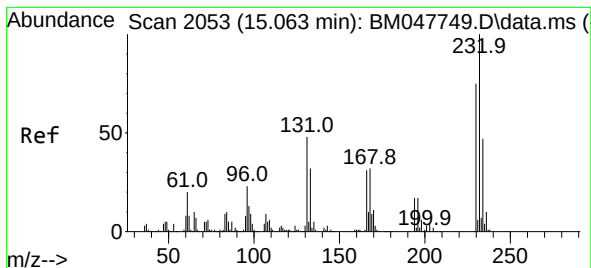

#58
2,3,4,6-Tetrachlorophenol
Concen: 1.626 ng/ul
RT: 15.069 min Scan# 2053
Delta R.T. -0.000 min
Lab File: BM047758.D
Acq: 02 Oct 2024 01:35

Instrument :
BNA_M
ClientSampleId :
DDCB7DL

Tgt Ion:	232	Resp:	14973
Ion	Ratio	Lower	Upper
232	100		
131	43.0	40.2	60.4
130	2.7	2.6	4.0
166	28.9	25.3	37.9

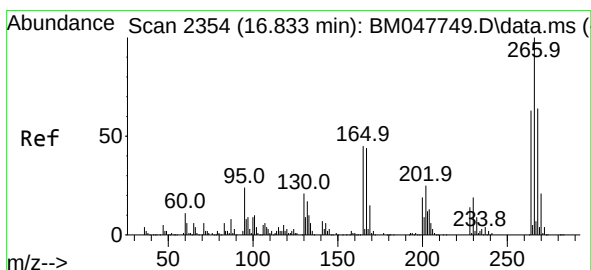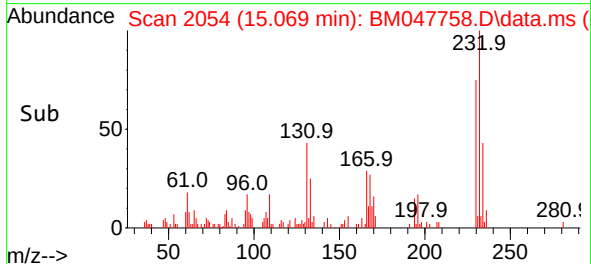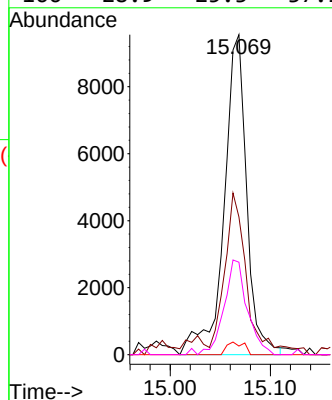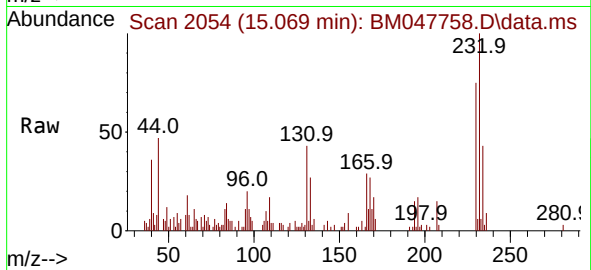

#71
Pentachlorophenol
Concen: 31.403 ng/ul
RT: 16.833 min Scan# 2354
Delta R.T. -0.006 min
Lab File: BM047758.D
Acq: 02 Oct 2024 01:35

Tgt Ion:	266	Resp:	278263
Ion	Ratio	Lower	Upper
266	100		
264	61.4	50.2	75.2
268	64.1	50.9	76.3

