

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
 Data File : BM047761.D
 Acq On : 02 Oct 2024 03:34
 Operator : RC/JU
 Sample : P4018-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCE2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/02/2024
 Supervised By :mohammad ahmed 10/04/2024

Quant Time: Oct 02 05:27:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 02:30:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	307094	20.000	ng/u1	0.00
20) Naphthalene-d8	10.604	136	1305898	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.439	164	812130	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.180	188	1620834	20.000	ng/u1	0.00
79) Chrysene-d12	21.403	240	1490173	20.000	ng/u1	0.00
88) Perylene-d12	24.403	264	1730474	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	22080	2.324	ng/uL	0.00
4) Pyridine-d5	3.675	84	148120	5.323	ng/u1	0.00
7) Phenol-d5	6.975	99	430141	14.813	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	273666	13.281	ng/u1	0.00
11) 2-Chlorophenol-d4	7.340	132	338631	16.028	ng/u1	0.00
15) 4-Methylphenol-d8	8.510	113	364760	16.895	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	174846	16.816	ng/u1	0.00
24) 2-Nitrophenol-d4	9.681	143	180258	18.091	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.222	165	351139	17.641	ng/u1	0.00
31) 4-Chloroaniline-d4	10.734	131	488541	15.876	ng/u1	0.00
46) Dimethylphthalate-d6	13.851	166	1179836	20.038	ng/u1	0.00
49) Acenaphthylene-d8	14.133	160	1345889	19.279	ng/u1	0.00
54) 4-Nitrophenol-d4	14.633	143	178823	15.254	ng/u1	0.00
60) Fluorene-d10	15.433	176	1040905	20.410	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.545	200	136848	14.428	ng/u1	0.00
73) Anthracene-d10	17.280	188	1608995	20.189	ng/u1	0.00
81) Pyrene-d10	19.562	212	1865452	22.057	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.197	264	1897303	21.132	ng/u1	-0.01
Target Compounds						
58) 2,3,4,6-Tetrachlorophenol	15.063	232	136473m	10.351	ng/u1	Qvalue
71) Pentachlorophenol	16.845	266	4955802	400.851	ng/u1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047761.D
Acq On : 02 Oct 2024 03:34
Operator : RC/JU
Sample : P4018-16
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DDCE2

Quant Time: Oct 02 05:27:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 10/02/2024
Supervised By :mohammad ahmed 10/04/2024

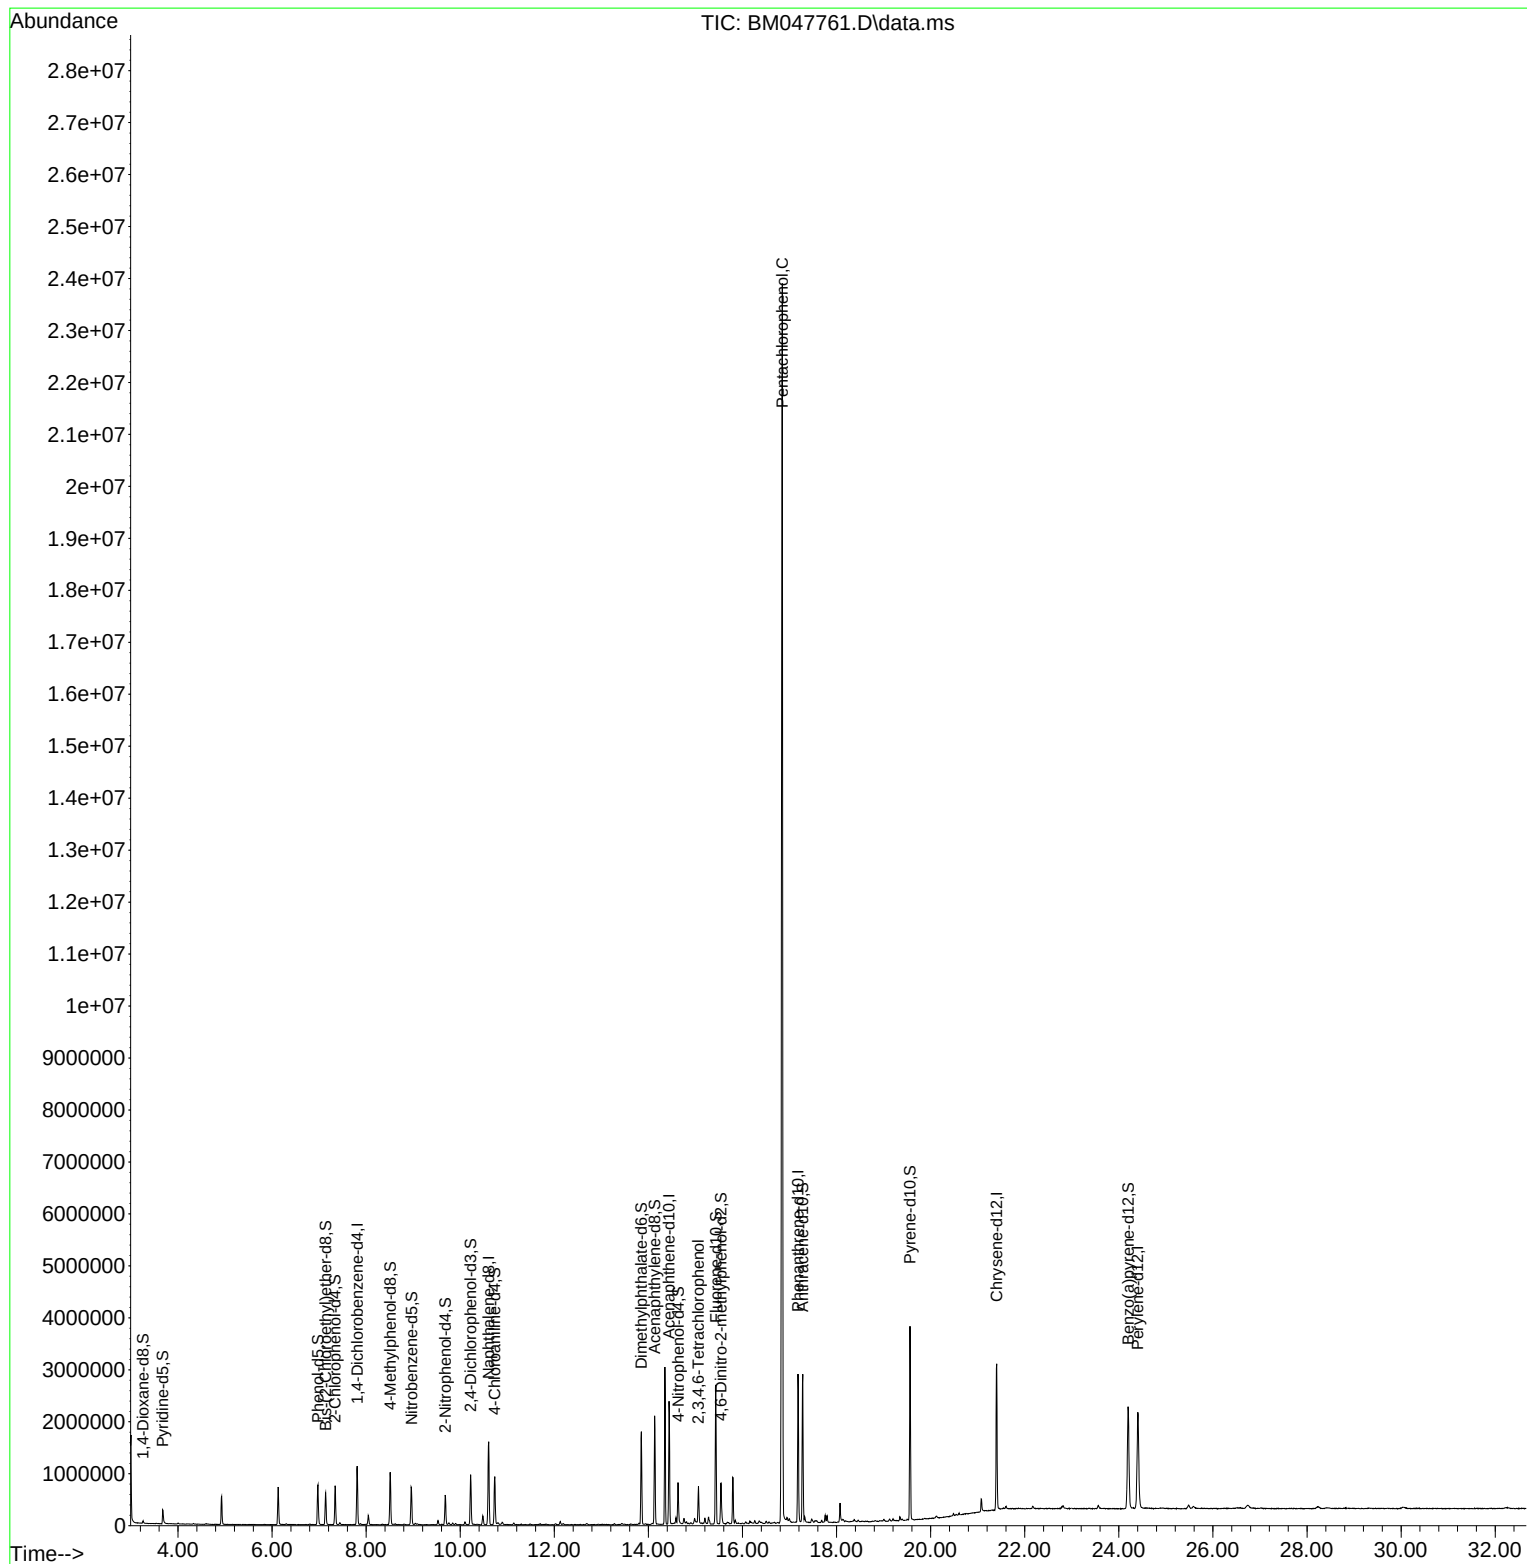

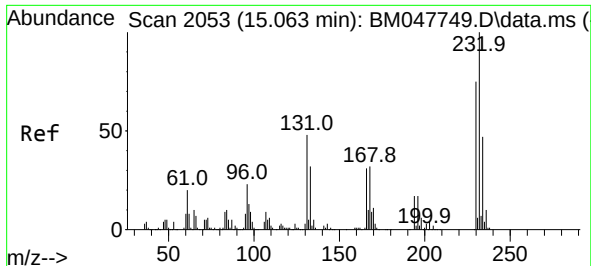

#58
2,3,4,6-Tetrachlorophenol
Concen: 10.351 ng/ul m
RT: 15.063 min Scan# 2053
Delta R.T. -0.006 min
Lab File: BM047761.D
Acq: 02 Oct 2024 03:34




Instrument :
BNA_M
ClientSampleId :
DDCE2

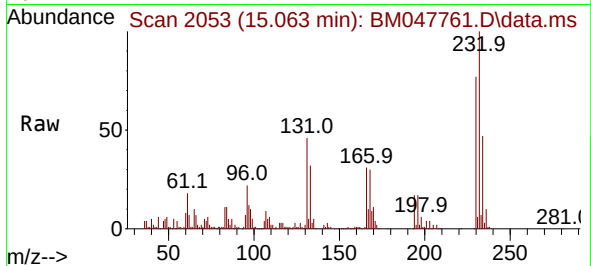

Tgt Ion:232 Resp: 136471
Ion Ratio Lower Upper
232 100
131 46.3 40.2 60.4
130 2.5 2.6 4.0
166 30.7 25.3 37.9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/02/2024
Supervised By :mohammad ahmed 10/04/2024

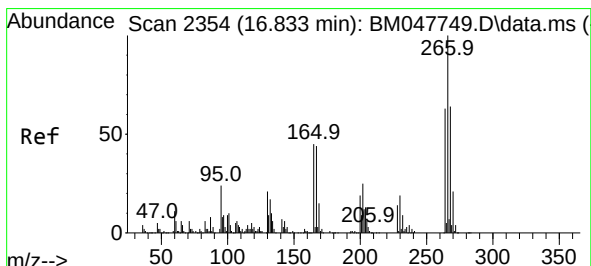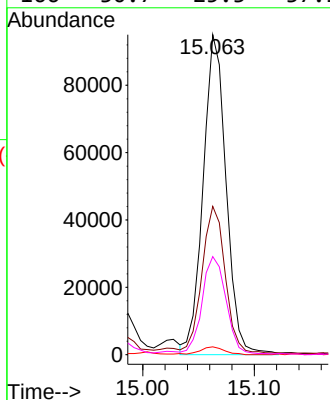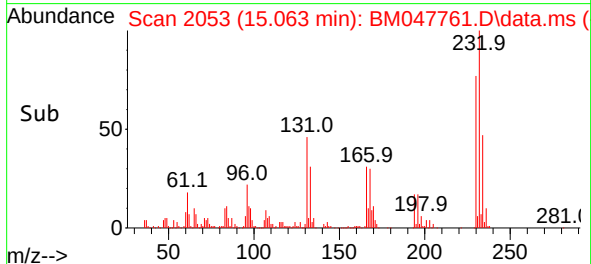

#71
Pentachlorophenol
Concen: 400.851 ng/ul
RT: 16.845 min Scan# 2356
Delta R.T. 0.006 min
Lab File: BM047761.D
Acq: 02 Oct 2024 03:34

Tgt Ion:266 Resp: 4955802
Ion Ratio Lower Upper
266 100
264 63.6 50.2 75.2
268 63.0 50.9 76.3

