

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
 Data File : BM047736.D
 Acq On : 01 Oct 2024 10:19
 Operator : RC/JU
 Sample : PB163390BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK390

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	7	9	12	rVB3	14316	14887	0.26%	0.024%
2	3.093	15	18	25	rVB3	18516	29440	0.51%	0.047%
3	3.258	42	46	56	rVB	79198	103564	1.80%	0.166%
4	3.669	112	116	132	rBV	902040	1392129	24.16%	2.228%
5	4.005	168	173	179	rVB	19452	27829	0.48%	0.045%
6	4.222	207	210	214	rBV3	14960	20730	0.36%	0.033%
7	4.640	276	281	285	rVB6	9485	15281	0.27%	0.024%
8	6.916	662	668	669	rBV3	4408	5967	0.10%	0.010%
9	6.975	669	678	687	rBV	1071947	1671007	29.00%	2.674%
10	7.140	699	706	718	rVB	875407	1331000	23.10%	2.130%
11	7.346	733	741	748	rBV	1033623	1670431	28.99%	2.674%
12	7.810	812	820	830	rBV	934311	1469501	25.50%	2.352%
13	8.516	932	940	954	rBV	1227759	2033189	35.29%	3.254%
14	8.963	1009	1016	1030	rBV	994293	1610881	27.96%	2.578%
15	9.687	1131	1139	1148	rBV	776117	1296030	22.49%	2.074%
16	10.222	1221	1230	1240	rBV	1240140	2081900	36.13%	3.332%
17	10.604	1287	1295	1308	rVB	1293799	2146853	37.26%	3.436%
18	10.734	1308	1317	1331	rBV	1135332	1984527	34.44%	3.176%
19	12.192	1561	1565	1573	rVB2	19510	31361	0.54%	0.050%
20	13.275	1745	1749	1753	rBV4	5100	6941	0.12%	0.011%
21	13.851	1840	1847	1853	rBV	2160367	2901512	50.36%	4.644%
22	14.133	1888	1895	1905	rBV	2393214	3620465	62.84%	5.795%
23	14.445	1941	1948	1955	rBV	1915338	2809044	48.75%	4.496%
24	14.633	1974	1980	1997	rBV	948059	1518122	26.35%	2.430%
25	14.845	2015	2016	2026	rVB7	8087	14718	0.26%	0.024%
26	15.263	2083	2087	2090	rVB5	5679	7861	0.14%	0.013%
27	15.433	2109	2116	2123	rBV	3074227	4422394	76.75%	7.078%
28	15.545	2128	2135	2146	rVV	854679	1167312	20.26%	1.868%
29	15.674	2152	2157	2165	rVB4	12937	26495	0.46%	0.042%
30	16.216	2242	2249	2254	rBV7	11088	15137	0.26%	0.024%
31	16.369	2274	2275	2282	rVB6	3757	5813	0.10%	0.009%
32	16.498	2292	2297	2301	rVB6	5412	8104	0.14%	0.013%
33	16.833	2349	2354	2358	rBV6	15386	26039	0.45%	0.042%
34	17.063	2390	2393	2396	rVB4	5720	6797	0.12%	0.011%
35	17.180	2406	2413	2423	rBV	2309259	3243545	56.29%	5.191%
36	17.280	2423	2430	2442	rVV	3151704	4550045	78.97%	7.282%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047736.D
Acq On : 01 Oct 2024 10:19
Operator : RC/JU
Sample : PB163390BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK390

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	17.845	2524	2526	2530	rVB5	7098	8947	0.16%	0.014%
38	18.068	2562	2564	2567	rBV4	12555	14482	0.25%	0.023%
39	18.151	2574	2578	2579	rBV4	6572	6604	0.11%	0.011%
40	18.404	2616	2621	2629	rBV5	25353	47446	0.82%	0.076%
41	18.551	2644	2646	2651	rVB6	12065	13467	0.23%	0.022%
42	18.963	2713	2716	2721	rBV4	21505	34142	0.59%	0.055%
43	19.133	2741	2745	2752	rBV4	37242	51673	0.90%	0.083%
44	19.198	2752	2756	2761	rBV	41988	66160	1.15%	0.106%
45	19.562	2812	2818	2826	rBV	4012423	5544331	96.23%	8.874%
46	21.404	3125	3131	3142	rBV	2413893	3517110	61.04%	5.629%
47	24.203	3598	3607	3619	rBV2	2304860	5761800	100.00%	9.222%
48	24.409	3634	3642	3658	rVB	1494331	4126897	71.63%	6.605%




Sum of corrected areas: 62479910

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047736.D
Acq On : 01 Oct 2024 10:19
Operator : RC/JU
Sample : PB163390BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK390

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

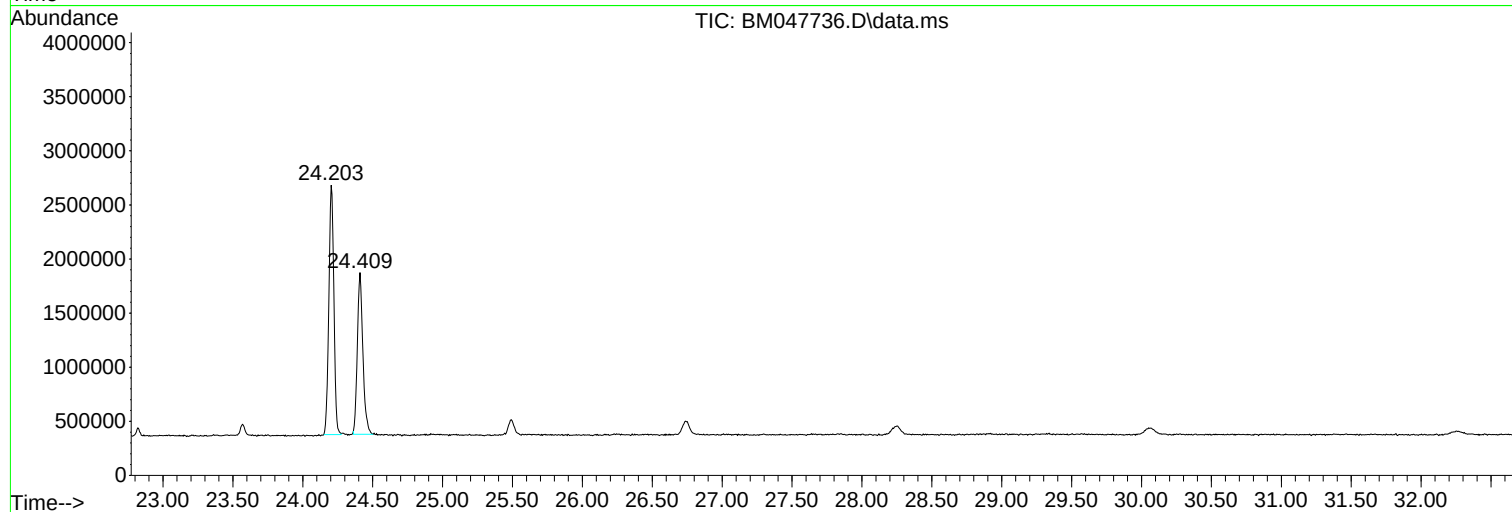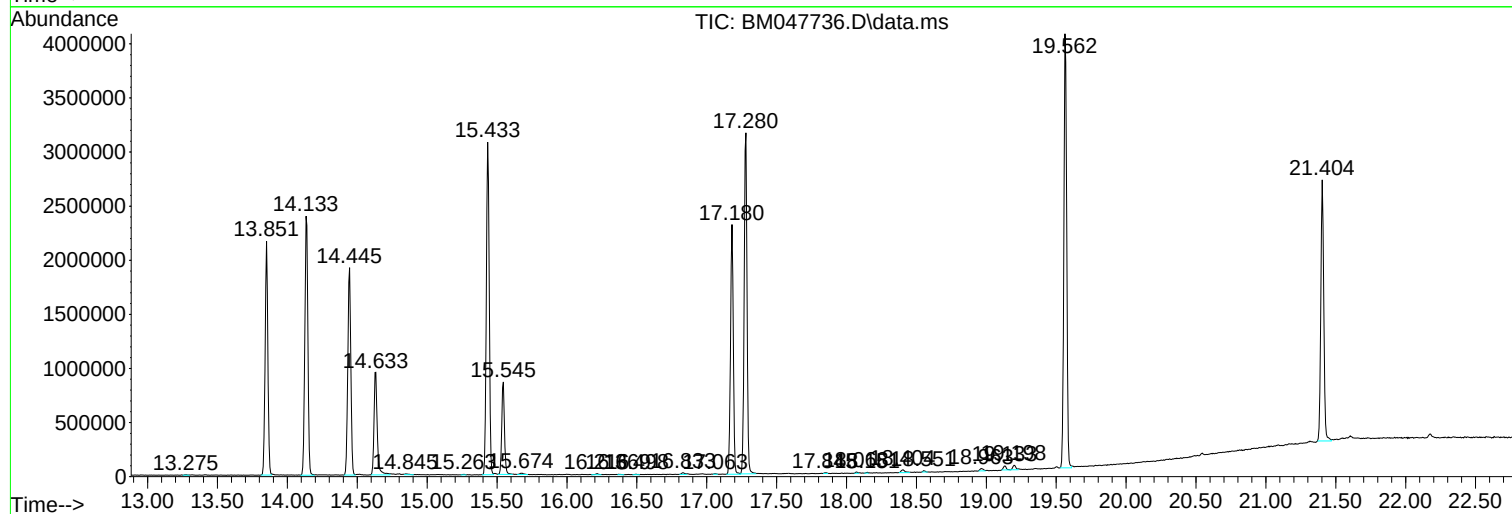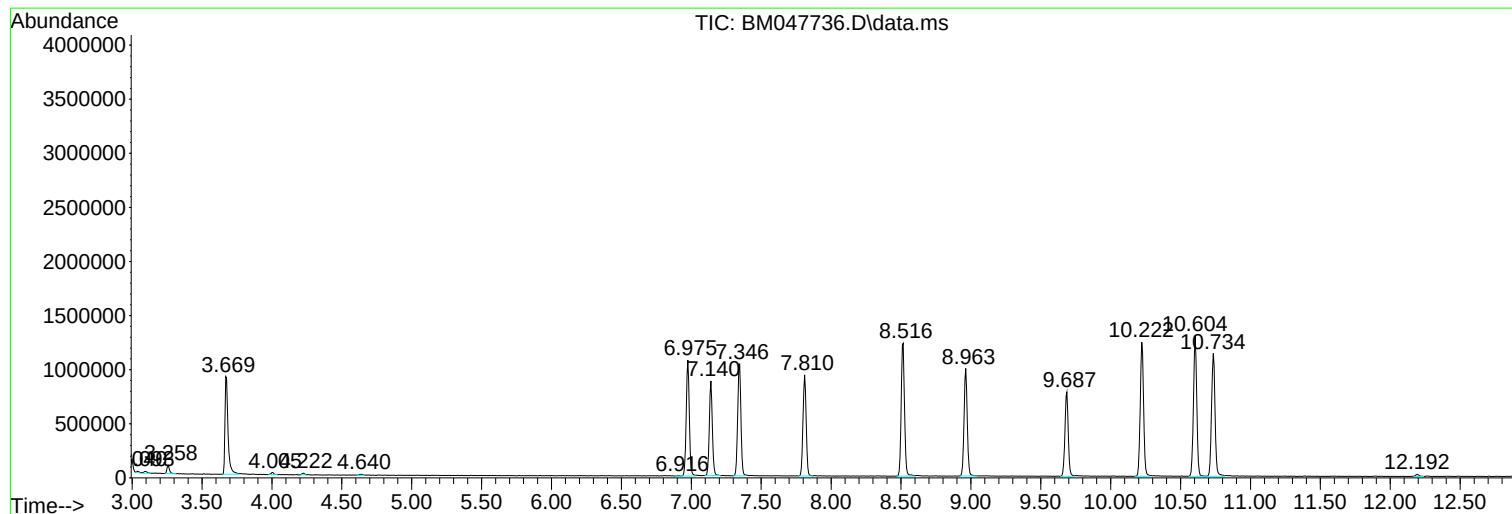

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047736.D
Acq On : 01 Oct 2024 10:19
Operator : RC/JU
Sample : PB163390BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK390

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047736.D
Acq On : 01 Oct 2024 10:19
Operator : RC/JU
Sample : PB163390BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK390

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc