

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
 Data File : BM047750.D
 Acq On : 01 Oct 2024 20:19
 Operator : RC/JU
 Sample : PB163513BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK513

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047750.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	42	46	59	rVB	66635	92787	2.24%	0.181%
2	3.669	112	116	138	rBV	832691	1273116	30.77%	2.490%
3	4.005	169	173	179	rVB2	20980	30477	0.74%	0.060%
4	4.222	208	210	214	rVB5	5253	5237	0.13%	0.010%
5	4.916	325	328	331	rBV5	3262	4289	0.10%	0.008%
6	5.793	474	477	481	rBV5	3618	5371	0.13%	0.011%
7	6.975	671	678	693	rVB	845599	1329647	32.14%	2.601%
8	7.140	699	706	716	rVB	693185	1084080	26.20%	2.120%
9	7.340	733	740	754	rBV	868437	1396277	33.75%	2.731%
10	7.810	812	820	829	rBV	964823	1529464	36.97%	2.991%
11	8.510	932	939	949	rBV	987187	1600202	38.68%	3.130%
12	8.963	1007	1016	1031	rBV	776063	1296017	31.32%	2.535%
13	9.681	1132	1138	1151	rVV	583136	983299	23.77%	1.923%
14	10.222	1223	1230	1243	rBV	980415	1617054	39.08%	3.163%
15	10.604	1287	1295	1304	rBV	1274472	2159736	52.20%	4.224%
16	10.734	1309	1317	1331	rBV	977715	1690275	40.85%	3.306%
17	10.904	1344	1346	1352	rVB7	2628	4498	0.11%	0.009%
18	12.192	1558	1565	1573	rBV2	16024	25636	0.62%	0.050%
19	13.545	1789	1795	1800	rBV7	2515	6579	0.16%	0.013%
20	13.851	1839	1847	1855	rBV	1614172	2145328	51.85%	4.196%
21	14.133	1888	1895	1906	rBV	1882195	2735197	66.11%	5.350%
22	14.445	1941	1948	1955	rBV	1872247	2782968	67.26%	5.443%
23	14.516	1958	1960	1965	rVB5	3215	4499	0.11%	0.009%
24	14.627	1973	1979	1992	rBV	640556	1022779	24.72%	2.000%
25	14.857	2014	2018	2023	rVB8	3538	4475	0.11%	0.009%
26	15.433	2109	2116	2128	rBV	2348307	3250804	78.57%	6.358%
27	15.545	2128	2135	2145	rBV	527860	764779	18.48%	1.496%
28	15.669	2152	2156	2161	rVB4	10226	16746	0.40%	0.033%
29	16.833	2350	2354	2356	rBV4	5777	8442	0.20%	0.017%
30	17.180	2406	2413	2423	rBV	2274024	3211826	77.63%	6.282%
31	17.274	2423	2429	2439	rVV	2376904	3436600	83.06%	6.722%
32	17.363	2442	2444	2449	rVB6	4656	6010	0.15%	0.012%
33	17.563	2475	2478	2481	rVB5	4481	5893	0.14%	0.012%
34	19.133	2741	2745	2749	rBV3	30025	40898	0.99%	0.080%
35	19.198	2753	2756	2761	rVB	25593	34209	0.83%	0.067%
36	19.562	2812	2818	2826	rBV	2849218	3927979	94.94%	7.683%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047750.D
Acq On : 01 Oct 2024 20:19
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK513

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	21.403	3125	3131	3144	rBV	2396572	3488309	84.31%	6.823%
38	24.203	3599	3607	3621	rVB2	1663972	4137331	100.00%	8.092%
39	24.409	3634	3642	3657	rVB	1537367	3968720	95.92%	7.762%




Sum of corrected areas: 51127833

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047750.D
Acq On : 01 Oct 2024 20:19
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

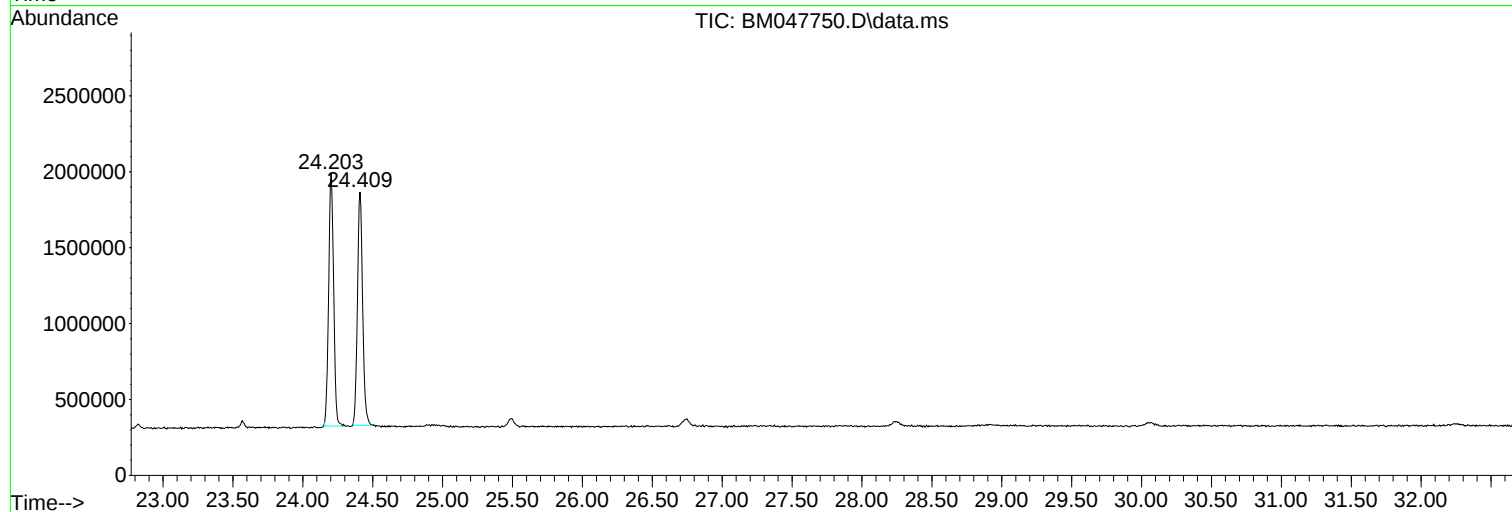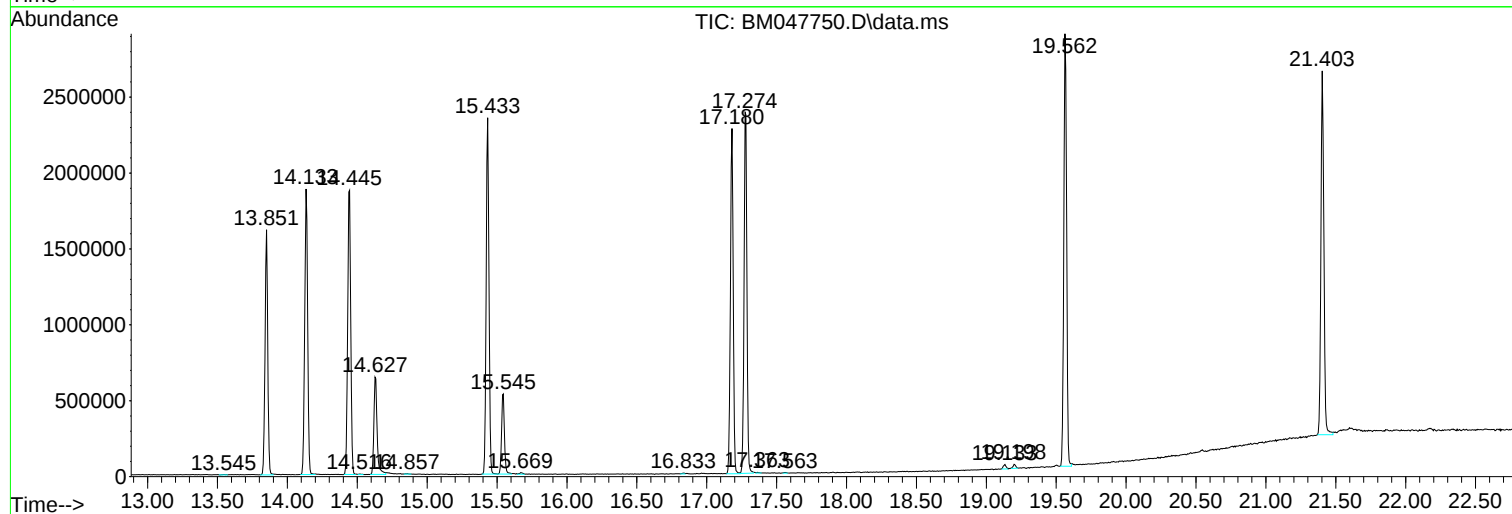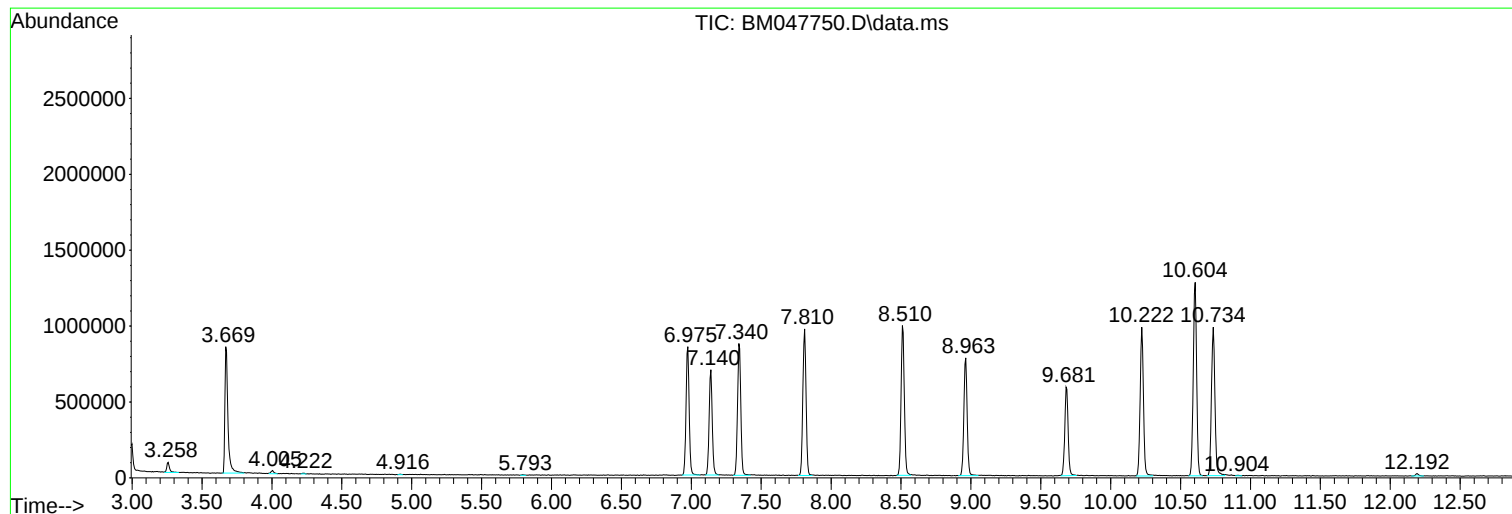

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047750.D
Acq On : 01 Oct 2024 20:19
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047750.D
Acq On : 01 Oct 2024 20:19
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc