

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
 Data File : BM047758.D
 Acq On : 02 Oct 2024 01:35
 Operator : RC/JU
 Sample : P4018-11DL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCB7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047758.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.681	115	118	129	rBV	69615	115384	3.45%	0.496%
2	3.999	169	172	182	rVB2	13981	22824	0.68%	0.098%
3	4.222	207	210	217	rVB9	4637	9142	0.27%	0.039%
4	5.834	480	484	490	rVB5	10325	16146	0.48%	0.069%
5	6.375	571	576	581	rVB5	6711	10186	0.30%	0.044%
6	6.804	646	649	655	rVV6	7418	13998	0.42%	0.060%
7	6.863	655	659	663	rVB5	8301	11316	0.34%	0.049%
8	6.975	673	678	685	rBV	90303	153126	4.58%	0.658%
9	7.140	700	706	712	rBV	64460	104781	3.14%	0.450%
10	7.246	719	724	728	rVV7	6534	11683	0.35%	0.050%
11	7.340	735	740	750	rVV	73592	130632	3.91%	0.561%
12	7.440	752	757	765	rVB2	43027	71206	2.13%	0.306%
13	7.810	811	820	827	rBV	808486	1317208	39.42%	5.657%
14	7.875	827	831	838	rVB2	18747	34571	1.03%	0.148%
15	8.351	907	912	919	rVB6	7744	16231	0.49%	0.070%
16	8.481	930	934	935	rVV3	8797	12369	0.37%	0.053%
17	8.510	935	939	948	rVB	94305	146293	4.38%	0.628%
18	8.581	948	951	954	rBV4	7717	11547	0.35%	0.050%
19	8.810	985	990	998	rVB9	4983	11075	0.33%	0.048%
20	8.922	1001	1009	1010	rBV7	5062	9493	0.28%	0.041%
21	8.963	1010	1016	1021	rVV	60874	101836	3.05%	0.437%
22	9.045	1024	1030	1039	rVB2	49856	80421	2.41%	0.345%
23	9.534	1109	1113	1118	rVB5	9497	18037	0.54%	0.077%
24	9.687	1131	1139	1145	rBV3	44540	86726	2.60%	0.372%
25	9.898	1172	1175	1179	rVV4	9327	13299	0.40%	0.057%
26	10.222	1221	1230	1240	rBV	85774	150684	4.51%	0.647%
27	10.298	1240	1243	1251	rVB6	7831	12500	0.37%	0.054%
28	10.481	1270	1274	1278	rBV5	6117	11213	0.34%	0.048%
29	10.598	1282	1294	1302	rVV	1139581	1984041	59.37%	8.521%
30	10.734	1309	1317	1330	rBV3	106496	216683	6.48%	0.931%
31	10.986	1355	1360	1368	rVB4	31148	56316	1.69%	0.242%
32	11.110	1374	1381	1389	rVV3	22041	44678	1.34%	0.192%
33	11.498	1443	1447	1450	rBV5	6963	13978	0.42%	0.060%
34	11.633	1465	1470	1475	rBV4	22560	36287	1.09%	0.156%
35	11.704	1479	1482	1489	rVB6	9765	18875	0.56%	0.081%
36	11.869	1503	1510	1519	rBV5	21561	40895	1.22%	0.176%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
 Data File : BM047758.D
 Acq On : 02 Oct 2024 01:35
 Operator : RC/JU
 Sample : P4018-11DL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCB7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

37	12.033	1531	1538	1541	rBV4	29663	49709	1.49%	0.213%
38	12.069	1541	1544	1550	rVB5	19091	27604	0.83%	0.119%
39	12.280	1572	1580	1586	rVB3	27930	57657	1.73%	0.248%
40	12.445	1601	1608	1612	rBV5	24230	45888	1.37%	0.197%

41	12.486	1612	1615	1619	rVB2	6618	9484	0.28%	0.041%
42	12.675	1641	1647	1648	rVV6	8081	10986	0.33%	0.047%
43	12.704	1651	1652	1659	rVV5	6675	10878	0.33%	0.047%
44	12.845	1673	1676	1681	rBV6	5891	9346	0.28%	0.040%
45	12.939	1687	1692	1696	rBV7	5699	9099	0.27%	0.039%

46	12.986	1696	1700	1705	rBV4	11108	17715	0.53%	0.076%
47	13.198	1732	1736	1740	rVB6	5303	10198	0.31%	0.044%
48	13.275	1744	1749	1757	rVV	47468	70708	2.12%	0.304%
49	13.492	1780	1786	1793	rVB8	11059	26874	0.80%	0.115%
50	13.627	1795	1809	1813	rBV8	16505	48646	1.46%	0.209%

51	13.704	1818	1822	1827	rBV8	5164	9611	0.29%	0.041%
52	13.763	1827	1832	1835	rBV3	13776	23086	0.69%	0.099%
53	13.810	1838	1840	1841	rVV2	10955	10254	0.31%	0.044%
54	13.845	1841	1846	1852	rVV	181080	270830	8.10%	1.163%
55	13.933	1858	1861	1866	rVB4	17857	25757	0.77%	0.111%

56	13.992	1869	1871	1876	rVB5	9778	14211	0.43%	0.061%
57	14.080	1883	1886	1887	rBV3	9642	9882	0.30%	0.042%
58	14.133	1890	1895	1906	rVB	203000	317145	9.49%	1.362%
59	14.351	1928	1932	1936	rBV	94440	118383	3.54%	0.508%
60	14.439	1941	1947	1954	rVV	1625594	2405602	71.99%	10.332%

61	14.522	1957	1961	1968	rVB6	17486	28961	0.87%	0.124%
62	14.580	1968	1971	1974	rBV3	9909	12001	0.36%	0.052%
63	14.639	1975	1981	1987	rBV9	23182	58262	1.74%	0.250%
64	14.686	1987	1989	1993	rVB5	9454	9499	0.28%	0.041%
65	14.839	2013	2015	2021	rVB6	15530	22758	0.68%	0.098%

66	14.910	2022	2027	2032	rVB5	11088	20806	0.62%	0.089%
67	14.974	2034	2038	2042	rBV5	15384	24593	0.74%	0.106%
68	15.027	2042	2047	2048	rBV5	12032	15892	0.48%	0.068%
69	15.063	2049	2053	2058	rVV	71019	94494	2.83%	0.406%
70	15.204	2074	2077	2079	rBV3	10140	13703	0.41%	0.059%

71	15.298	2085	2093	2097	rVB	65168	96488	2.89%	0.414%
72	15.433	2110	2116	2121	rVB	269246	381903	11.43%	1.640%
73	15.539	2129	2134	2142	rBV7	46749	101516	3.04%	0.436%
74	15.704	2157	2162	2172	rVB4	29482	59223	1.77%	0.254%
75	15.798	2172	2178	2182	rBV	65703	98940	2.96%	0.425%

76	15.863	2185	2189	2192	rVB5	6448	10614	0.32%	0.046%
----	--------	------	------	------	------	------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
 Data File : BM047758.D
 Acq On : 02 Oct 2024 01:35
 Operator : RC/JU
 Sample : P4018-11DL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCB7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

77	15.921	2192	2199	2207	rVB5	11308	29192	0.87%	0.125%
78	15.998	2208	2212	2214	rBV5	7573	9600	0.29%	0.041%
79	16.157	2234	2239	2242	rBV	66458	96309	2.88%	0.414%
80	16.292	2258	2262	2264	rBV4	9609	13705	0.41%	0.059%
81	16.316	2264	2266	2270	rVB3	8941	9114	0.27%	0.039%
82	16.498	2293	2297	2300	rBV6	9919	13303	0.40%	0.057%
83	16.827	2346	2353	2367	rBV	1675731	2468456	73.87%	10.602%
84	16.951	2370	2374	2379	rVV2	58731	89783	2.69%	0.386%
85	16.998	2379	2382	2387	rVB3	26313	37416	1.12%	0.161%
86	17.180	2407	2413	2423	rBV	1968375	2821966	84.45%	12.120%
87	17.274	2423	2429	2435	rBV	286778	419640	12.56%	1.802%
88	17.415	2452	2453	2459	rVB6	9367	11681	0.35%	0.050%
89	17.474	2459	2463	2464	rBV4	9853	12667	0.38%	0.054%
90	17.686	2494	2499	2504	rVB	50318	64063	1.92%	0.275%
91	17.757	2508	2511	2514	rVV4	12005	16156	0.48%	0.069%
92	17.792	2514	2517	2524	rVV5	23405	33923	1.02%	0.146%
93	17.857	2524	2528	2532	rVB2	34902	41792	1.25%	0.179%
94	18.068	2556	2564	2570	rBV9	31129	60976	1.82%	0.262%
95	18.374	2612	2616	2621	rBV	33928	46307	1.39%	0.199%
96	19.009	2720	2724	2725	rBV2	23637	30542	0.91%	0.131%
97	19.562	2813	2818	2824	rBV	375980	507267	15.18%	2.179%
98	21.403	3125	3131	3142	rBV	1921499	2939947	87.98%	12.627%
99	24.197	3601	3606	3616	rVB	171916	393265	11.77%	1.689%
100	24.403	3633	3641	3656	rVB	1259865	3341608	100.00%	14.352%




Sum of corrected areas: 23283564

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047758.D
Acq On : 02 Oct 2024 01:35
Operator : RC/JU
Sample : P4018-11DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCB7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

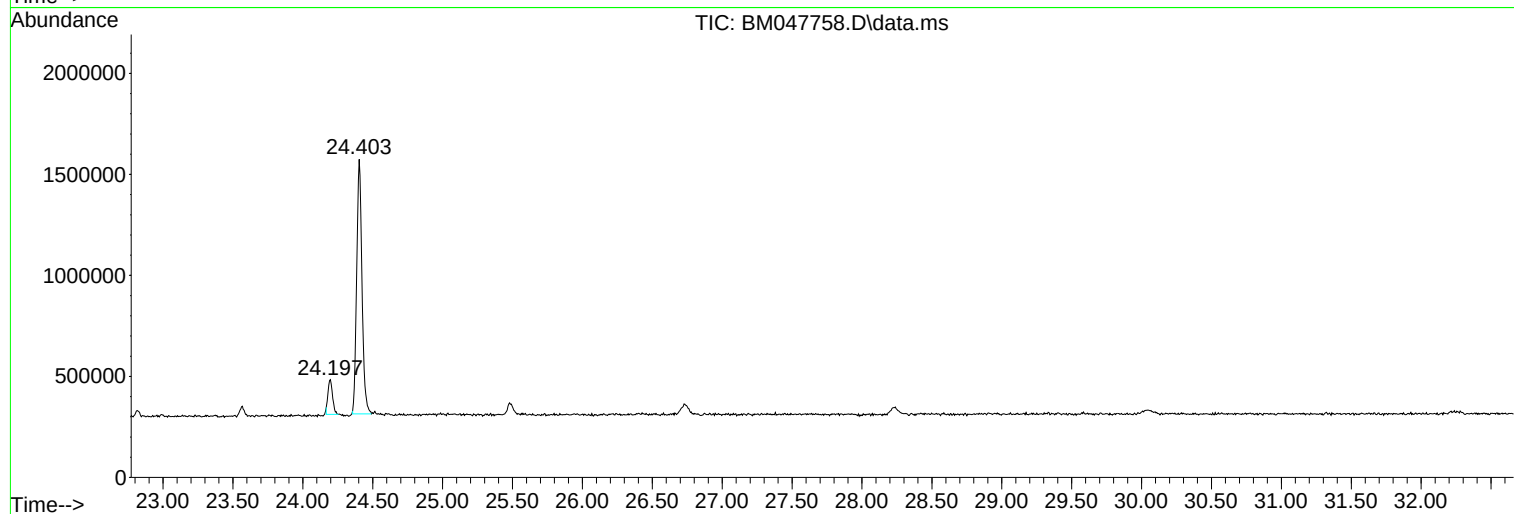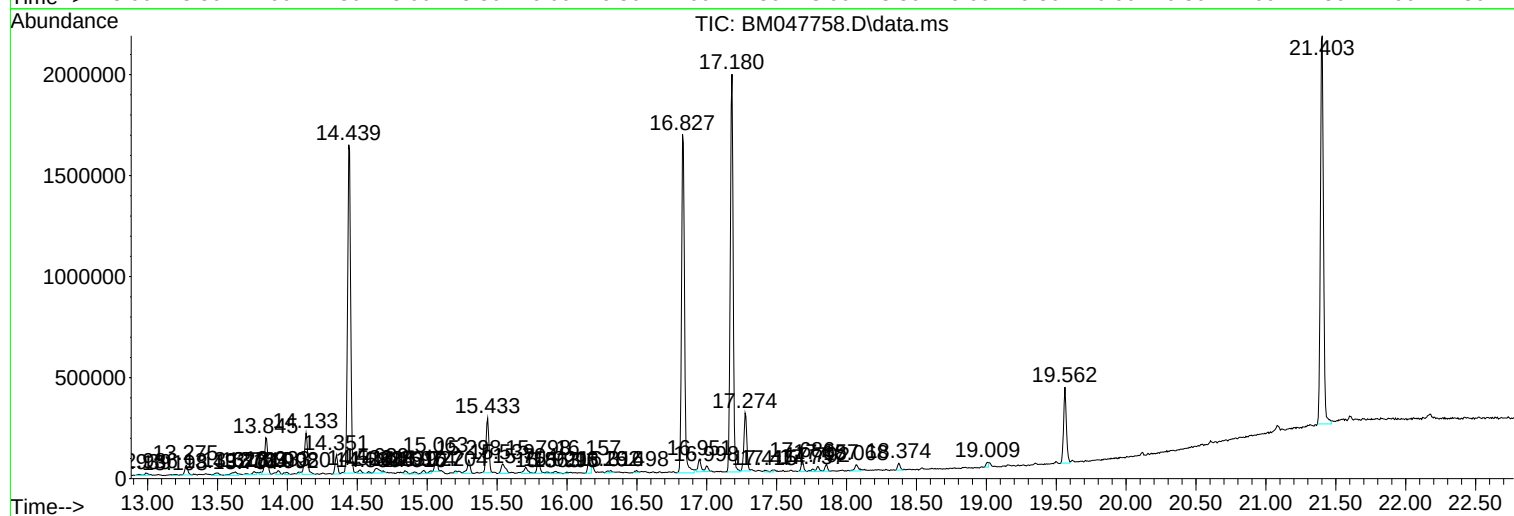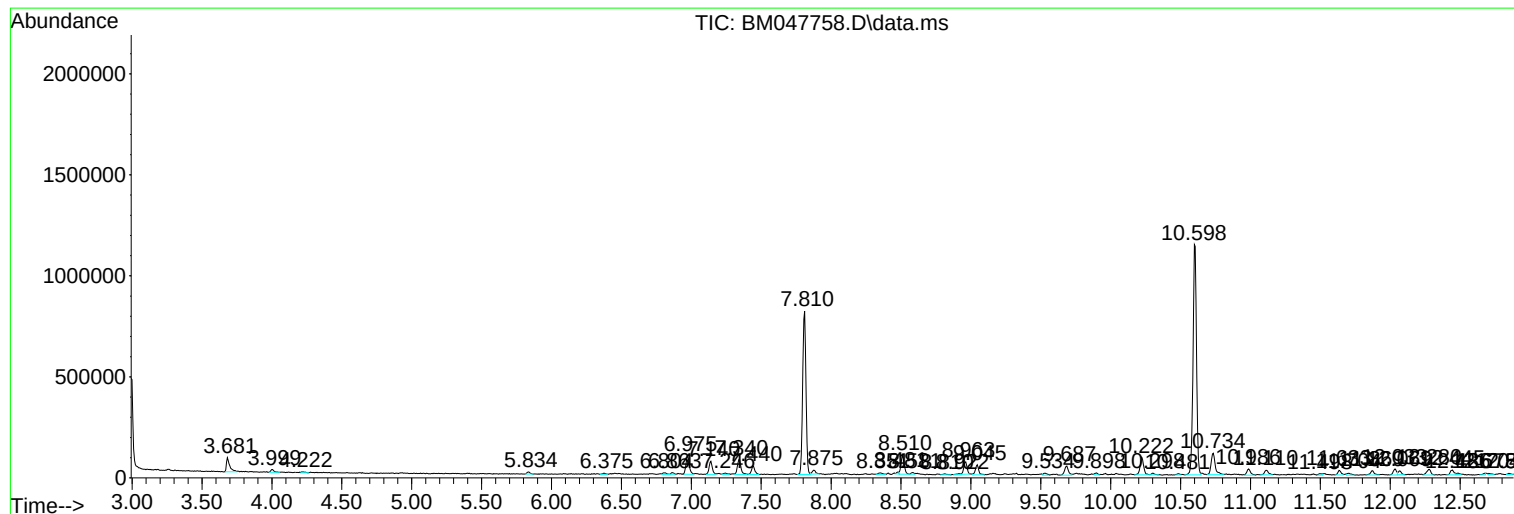

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047758.D
Acq On : 02 Oct 2024 01:35
Operator : RC/JU
Sample : P4018-11DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCB7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047758.D
Acq On : 02 Oct 2024 01:35
Operator : RC/JU
Sample : P4018-11DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCB7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc