

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
 Data File : BM047764.D
 Acq On : 02 Oct 2024 06:12
 Operator : RC/JU
 Sample : PB163513BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK513

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047764.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	42	46	52	rVB	69791	92254	2.20%	0.183%
2	3.669	112	116	133	rBV	894234	1340978	31.95%	2.653%
3	3.999	169	172	177	rVB3	17080	22672	0.54%	0.045%
4	4.222	206	210	214	rVB7	10056	13301	0.32%	0.026%
5	4.634	278	280	284	rVB4	5596	7014	0.17%	0.014%
6	6.975	670	678	690	rBV	886899	1432451	34.13%	2.834%
7	7.140	699	706	715	rBV	717202	1146932	27.33%	2.269%
8	7.340	733	740	749	rBV	945439	1467566	34.97%	2.904%
9	7.810	813	820	830	rBV	856579	1371784	32.69%	2.714%
10	8.192	882	885	890	rBV5	3389	5608	0.13%	0.011%
11	8.510	932	939	958	rBV	1080825	1716840	40.91%	3.397%
12	8.957	1007	1015	1026	rBV	814234	1367214	32.58%	2.705%
13	9.139	1042	1046	1049	rVB5	3945	5957	0.14%	0.012%
14	9.681	1125	1138	1146	rBV	636165	1038314	24.74%	2.055%
15	10.222	1223	1230	1244	rBV	1015251	1690821	40.29%	3.346%
16	10.598	1287	1294	1305	rBV	1149374	1952756	46.53%	3.864%
17	10.733	1309	1317	1333	rBV	1019209	1773905	42.27%	3.510%
18	11.475	1440	1443	1445	rBV2	3692	4512	0.11%	0.009%
19	12.192	1558	1565	1570	rBV4	16946	26696	0.64%	0.053%
20	13.851	1840	1847	1856	rBV	1591179	2241092	53.40%	4.434%
21	14.133	1888	1895	1903	rBV	1931301	2845403	67.80%	5.630%
22	14.439	1939	1947	1959	rBV	1720986	2491110	59.36%	4.929%
23	14.627	1973	1979	1998	rBV	709583	1102907	26.28%	2.182%
24	14.857	2015	2018	2022	rVB5	3431	5046	0.12%	0.010%
25	15.433	2109	2116	2125	rBV	2427373	3385563	80.67%	6.699%
26	15.539	2128	2134	2147	rBV	583876	819964	19.54%	1.622%
27	15.674	2152	2157	2161	rVB4	10373	16545	0.39%	0.033%
28	16.974	2372	2378	2384	rBV7	5358	11343	0.27%	0.022%
29	17.180	2406	2413	2421	rBV	1954654	2816113	67.10%	5.572%
30	17.274	2423	2429	2443	rVV	2496720	3525150	83.99%	6.975%
31	18.815	2689	2691	2693	rBV3	5675	6144	0.15%	0.012%
32	18.956	2713	2715	2717	rBV3	6769	6172	0.15%	0.012%
33	19.127	2741	2744	2750	rVB3	24617	30240	0.72%	0.060%
34	19.198	2753	2756	2760	rVB	24760	33731	0.80%	0.067%
35	19.562	2812	2818	2826	rBV	3091800	4057679	96.68%	8.029%
36	21.403	3125	3131	3141	rBV	2067197	3051438	72.71%	6.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047764.D
Acq On : 02 Oct 2024 06:12
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK513

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	24.203	3598	3607	3621	rVB2	1730122	4196921	100.00%	8.304%
38	24.403	3633	3641	3655	rVB	1346128	3418093	81.44%	6.763%




Sum of corrected areas: 50538229

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047764.D
Acq On : 02 Oct 2024 06:12
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

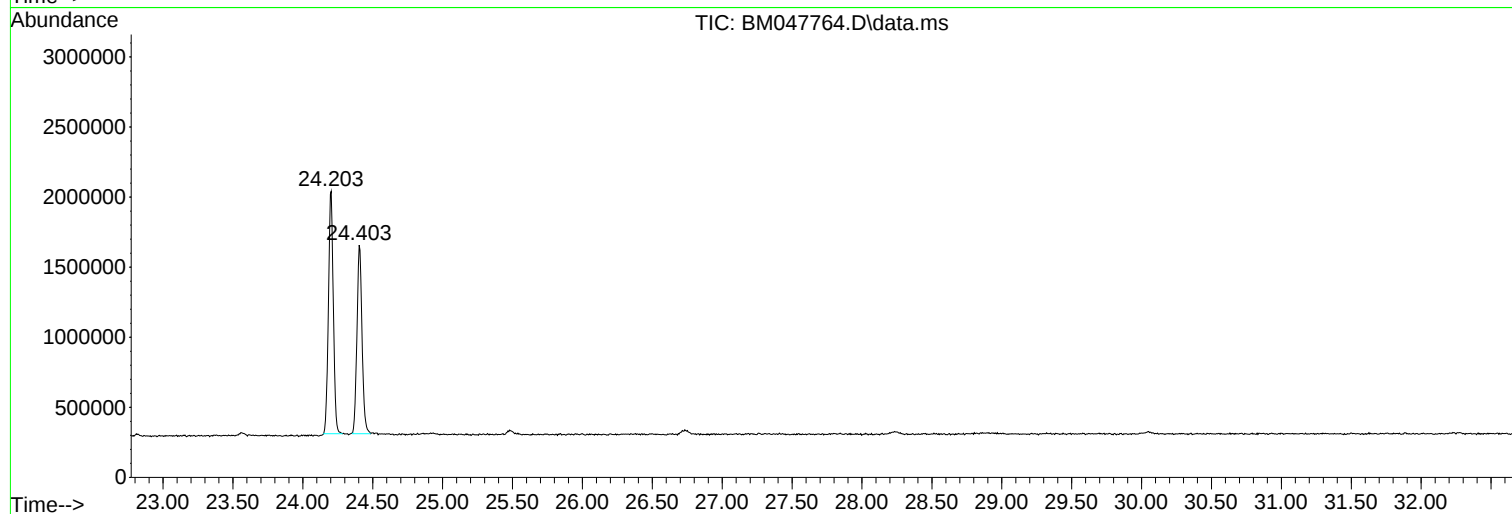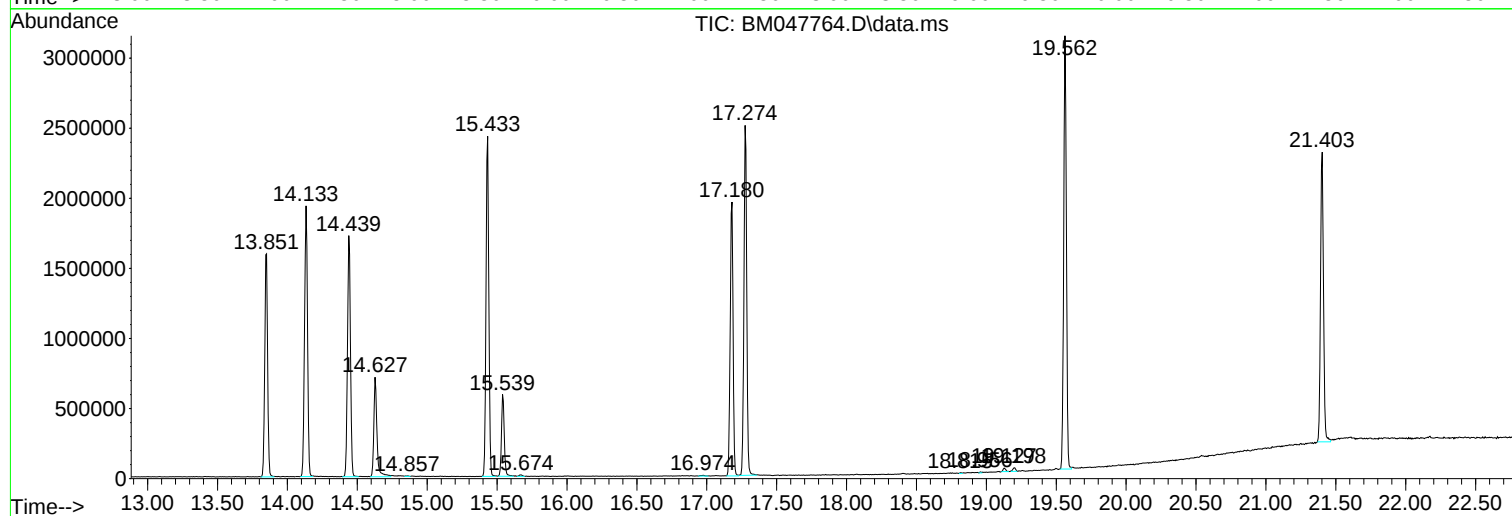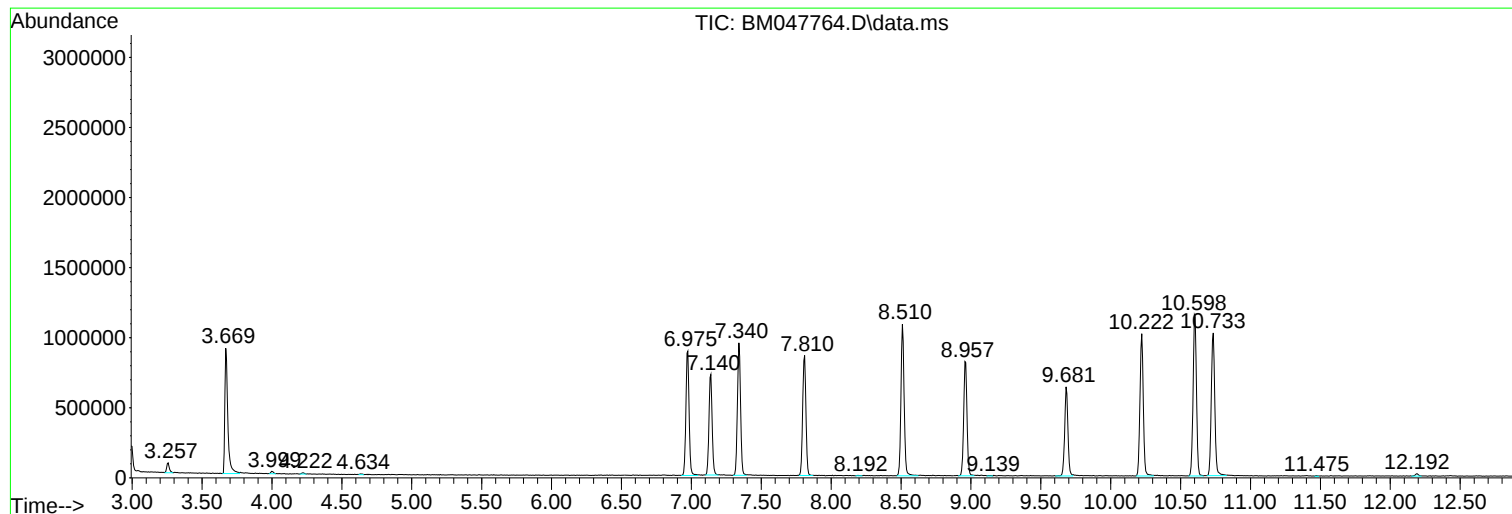

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047764.D
Acq On : 02 Oct 2024 06:12
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100124\
Data File : BM047764.D
Acq On : 02 Oct 2024 06:12
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------