

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100215\
 Data File : BM002834.D
 Acq On : 02 Oct 2015 17:42
 Operator : UM/IZ
 Sample : PB85900BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK00

Quant Time: Oct 03 00:44:34 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHOD\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 00:37:55 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.69	152	53466	20.00	ng/ul	0.00
18) Naphthalene-d8	11.54	136	229545	20.00	ng/ul	0.00
36) Acenaphthene-d10	15.28	164	117841	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.99	188	244456	20.00	ng/ul	0.00
78) Chrysene-d12	22.08	240	263197	20.00	ng/ul	0.00
86) Perylene-d12	24.67	264	262532	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.76	96	9623	8.36	ng/uL	0.00
5) Phenol-d5	7.80	99	165712	40.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.97	67	93484	41.02	ng/ul	0.00
9) 2-Chlorophenol-d4	8.20	132	154345	40.93	ng/ul	0.00
13) 4-Methylphenol-d8	9.39	113	138396	41.43	ng/ul	0.00
19) Nitrobenzene-d5	9.88	128	72150	41.22	ng/ul	0.00
22) 2-Nitrophenol-d4	10.61	143	75185	41.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	11.15	165	121744	37.71	ng/ul	0.00
29) 4-Chloroaniline-d4	11.67	131	197134	50.72	ng/ul	0.00
44) Dimethylphthalate-d6	14.66	166	372362	42.00	ng/ul	0.00
47) Acenaphthylene-d8	14.99	160	486481	41.12	ng/ul	0.00
52) 4-Nitrophenol-d4	15.46	143	57031	36.23	ng/ul	0.00
58) Fluorene-d10	16.26	176	320658	40.15	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	16.38	200	36688	30.77	ng/ul	0.00
71) Anthracene-d10	18.09	188	476271	40.82	ng/ul	0.00
79) Pyrene-d10	20.32	212	492516	40.09	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.50	264	550772	41.01	ng/ul	0.00

Target Compounds


					Ovalue	
15) N-Nitroso-di-n-propylamine	9.39	70	2486	1.05	ng/ul#	1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100215\
Data File : BM002834.D
Acq On : 02 Oct 2015 17:42
Operator : UM/IZ
Sample : PB85900BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK00

Quant Time: Oct 03 00:44:34 2015
Quant Method : Z:\HPCHEM1\BNA M\METHOD\SOM02.2-EPA-BM092915.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 03 00:37:55 2015
Response via : Initial Calibration

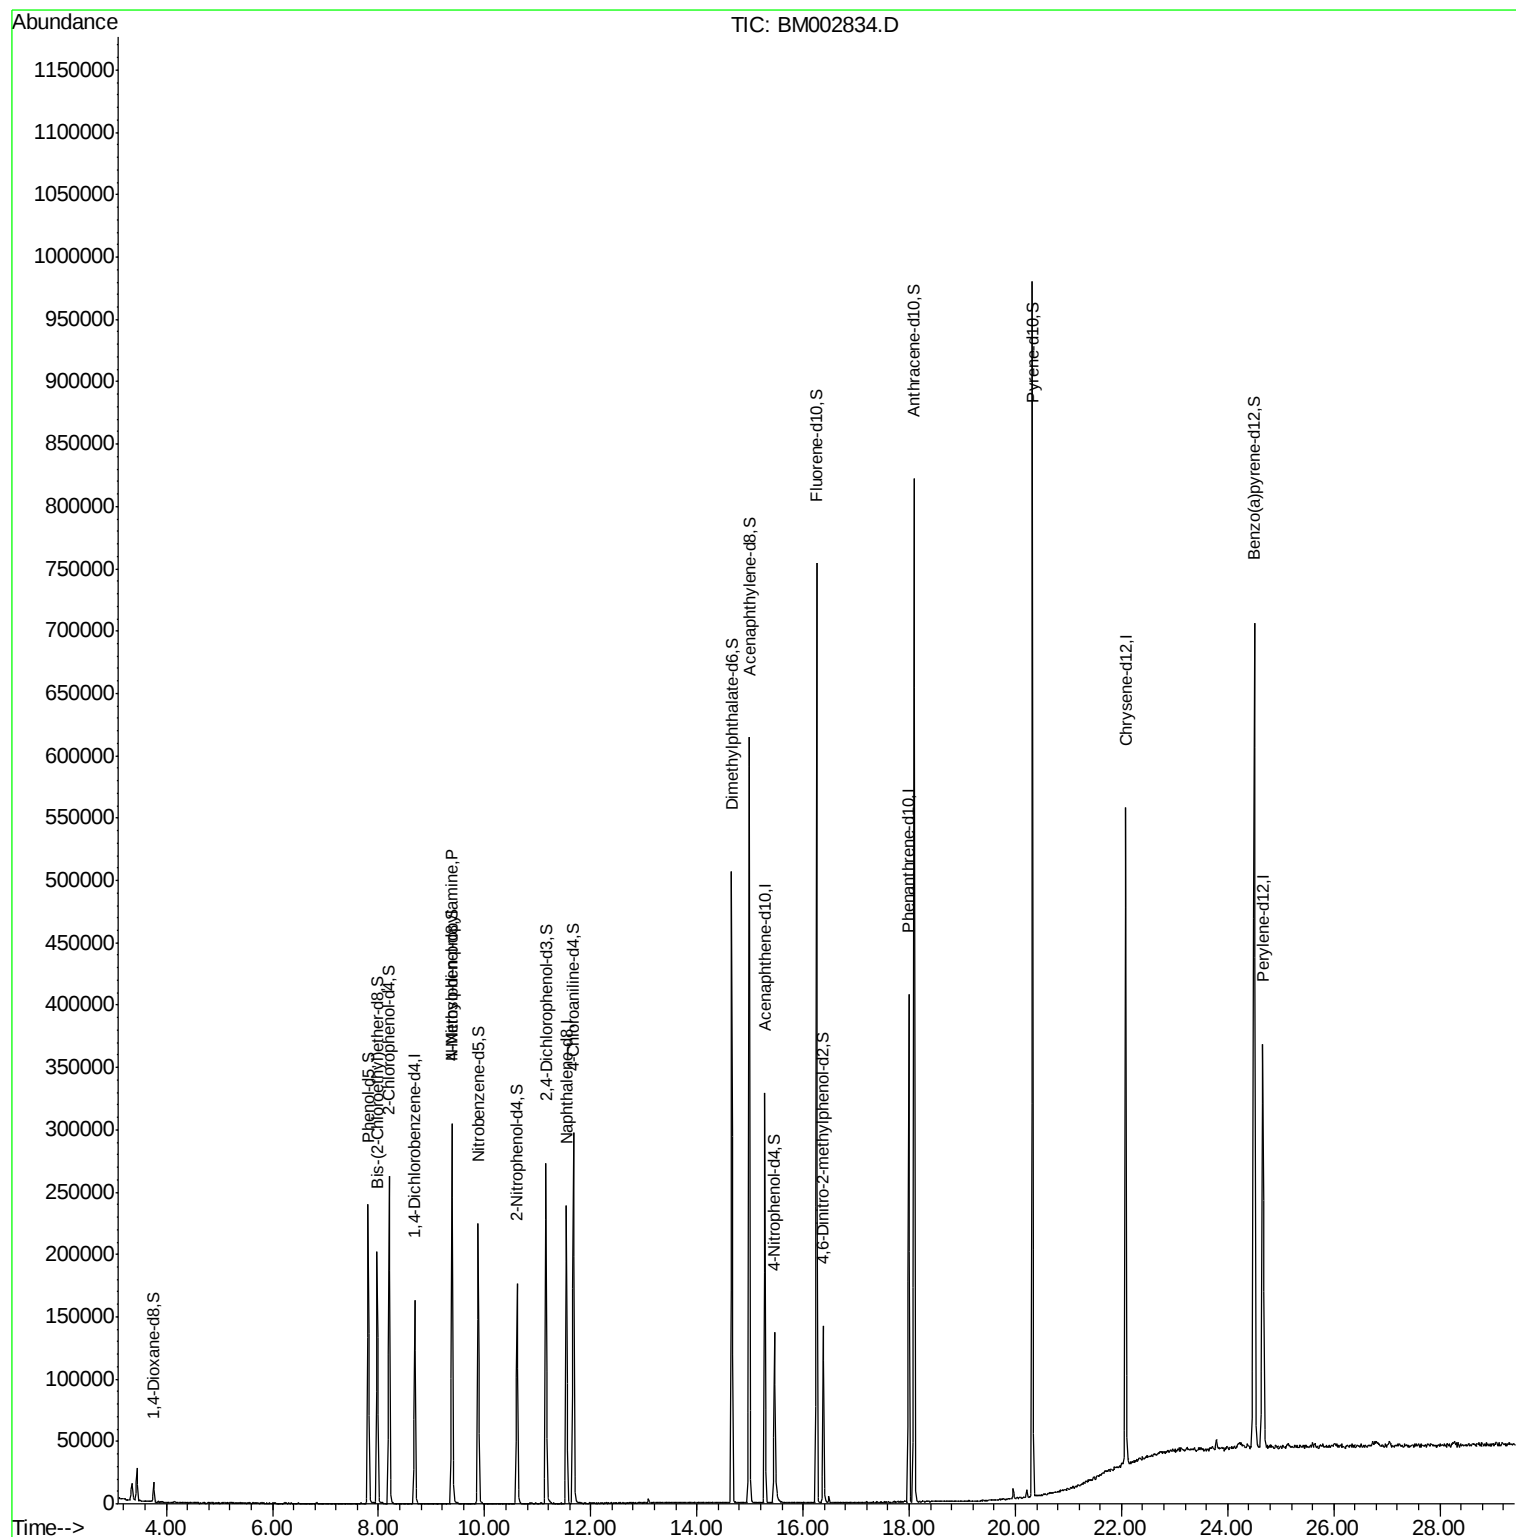

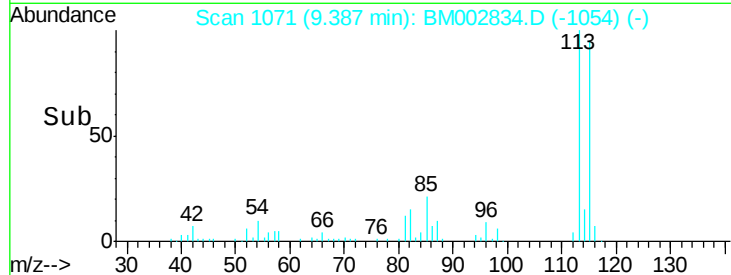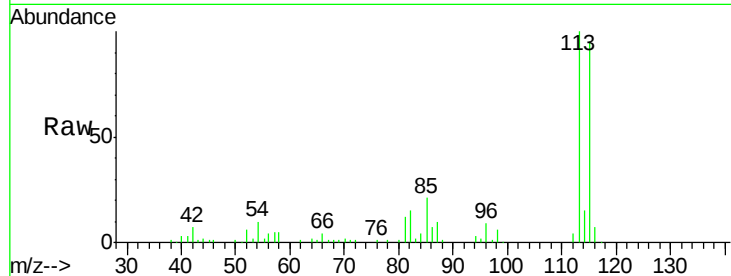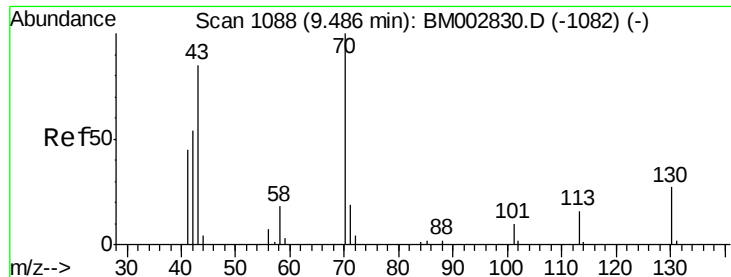

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.05 ng/ul
 RT: 9.39 min Scan# 1071
 Delta R.T. -0.10 min
 Lab File: BM002834.D
 Acq: 02 Oct 2015 17:42

Instrument :
 BNA_M
 ClientSampleId :
 SBLK00

Tot Ion:	70	Resp:	2486
Ion	Ratio	Lower	Upper
70	100		
42	372.0	45.2	67.8#
101	0.0	9.1	13.7#
130	0.0	22.2	33.2#

