


Data Path : Z:\HPCHEM1\BNA M\Data\BM100215\
Data File : BM002835.D
Acq On : 02 Oct 2015 18:18
Operator : UM/IZ
Sample : G3852-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C03G1

Quant Time: Oct 03 01:20:43 2015
Quant Method : Z:\HPCHEM1\BNA M\METHOD\SOM02.2-EPA-BM092915.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 03 00:37:55 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDADODA
10/5/2015 1:23:17 PM

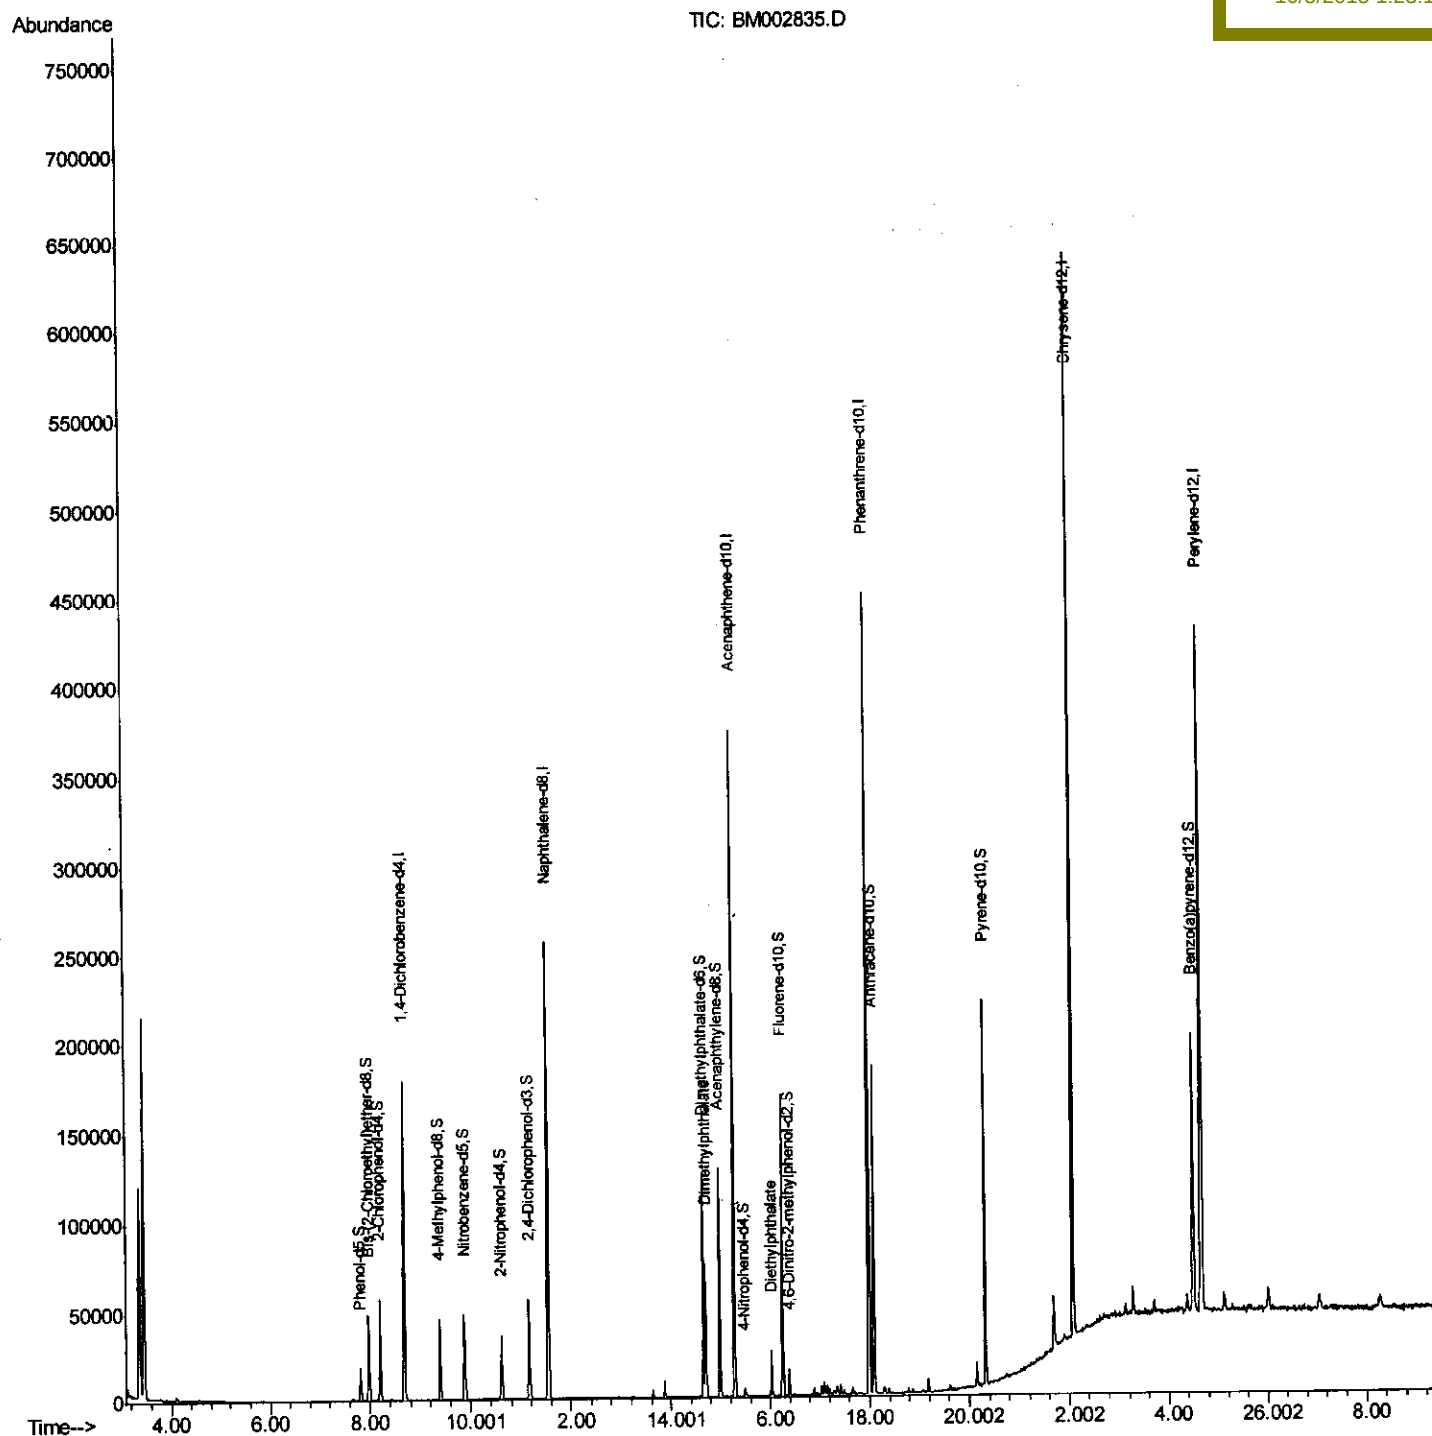

Quantitation Report (Qedit)



Data Path : Z:\HPCHEM1\BNA M\Data\BM100215\
 Data File : BM002835.D
 Acq On : 02 Oct 2015 18:18
 Operator : UM/IZ
 Sample : G3852-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C03G1

Quant Time: Oct 03 01:13:06 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHOD\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 00:37:55 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDADODA
 10/5/2015 1:23:17 PM

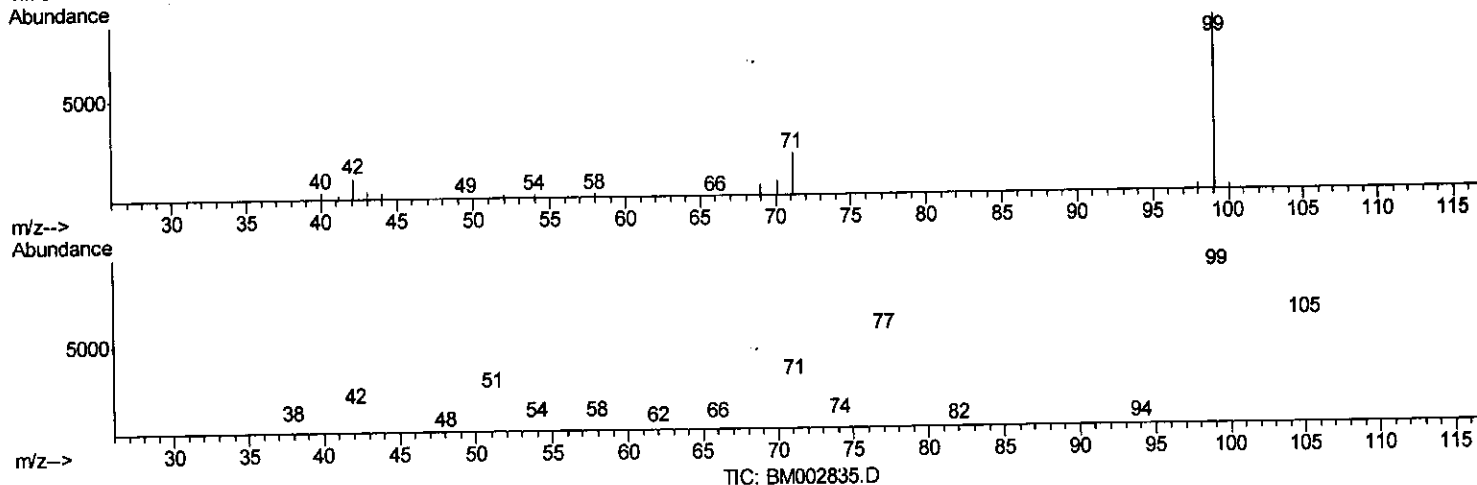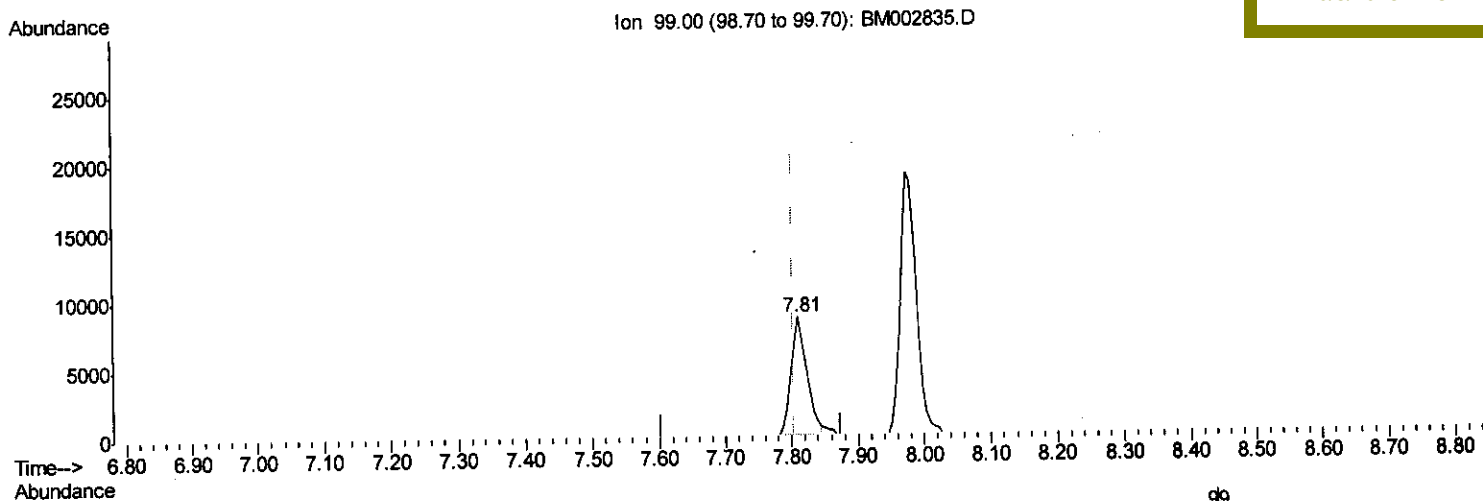

(5) Phenol-d5 (S)

7.810min (+0.006) 3.24ng/ul

response 14313

Ion	Exp%	Act%
99.00	100	100
71.00	27.60	26.42
42.00	15.50	14.88
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM100215\
 Data File : BM002835.D
 Acq On : 02 Oct 2015 18:18
 Operator : UM/IZ
 Sample : G3852-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C03G1

Quant Time: Oct 03 01:13:06 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHOD\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 00:37:55 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDADODA
 10/5/2015 1:23:17 PM

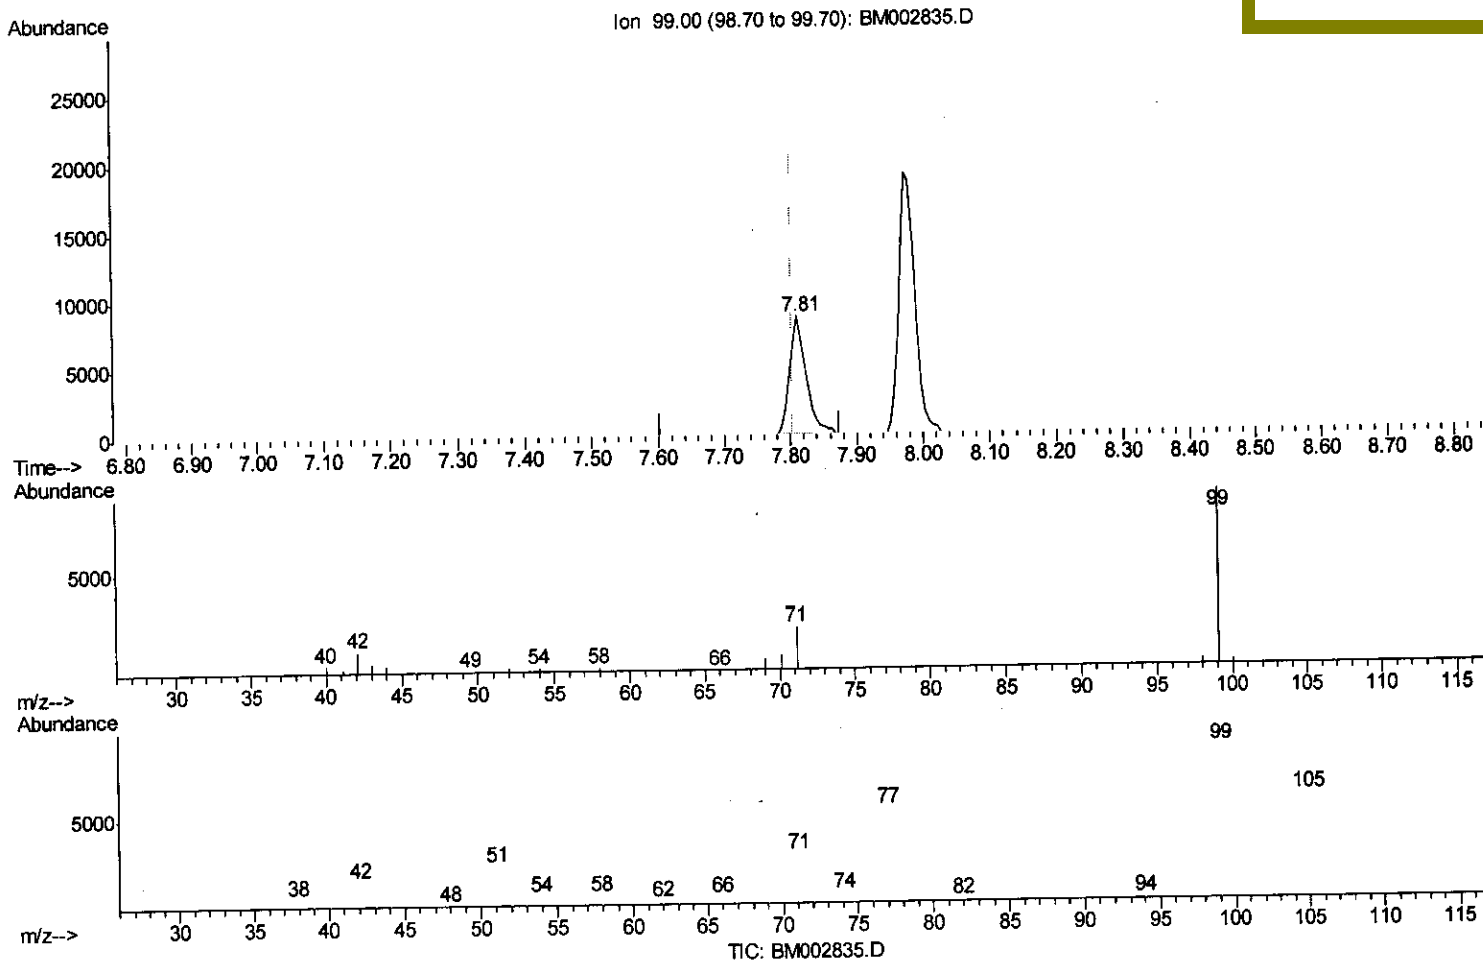

(5) Phenol-d5 (S)

7.810min (+0.006) 3.33ng/ul m

response 14716

U. M
 10/6/15

Ion	Exp%	Act%
99.00	100	100
71.00	27.60	26.42
42.00	15.50	14.88
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM100215\
 Data File : BM002835.D
 Acq On : 02 Oct 2015 18:18
 Operator : UM/IZ
 Sample : G3852-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 C03G1

Quant Time: Oct 03 01:13:06 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHOD\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 00:37:55 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDADODA
 10/5/2015 1:23:17 PM

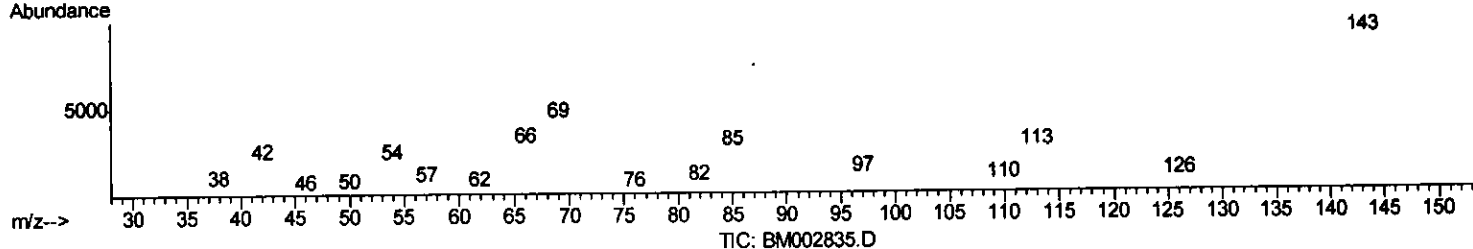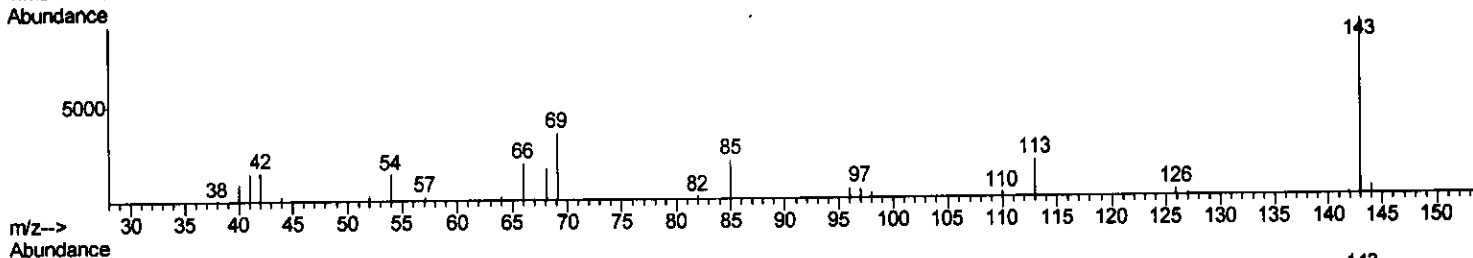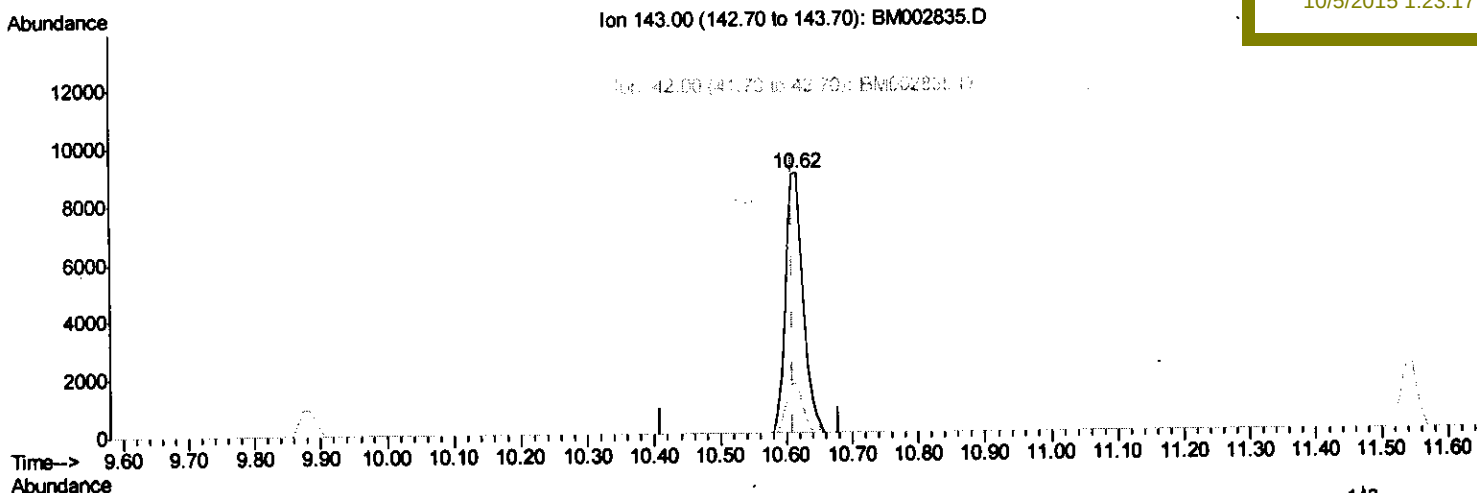

(22) 2-Nitrophenol-d4 (S)

10.616min (+0.006) 8.36ng/ul

response 16636

Ion	Exp%	Act%
143.00	100	100
69.00	38.50	40.11
41.00	16.80	18.62
42.00	17.20	19.18

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM100215\
Data File : BM002835.D
Acq On : 02 Oct 2015 18:18
Operator : UM/IZ
Sample : G3852-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C03G1

Quant Time: Oct 03 01:13:06 2015
Quant Method : Z:\HPCHEM1\BNA M\METHOD\SOM02.2-EPA-BM092915.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 03 00:37:55 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDADODA
10/5/2015 1:23:17 PM

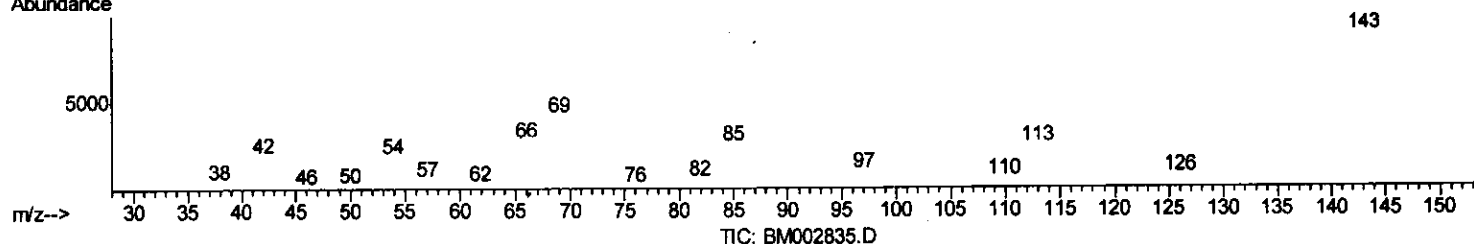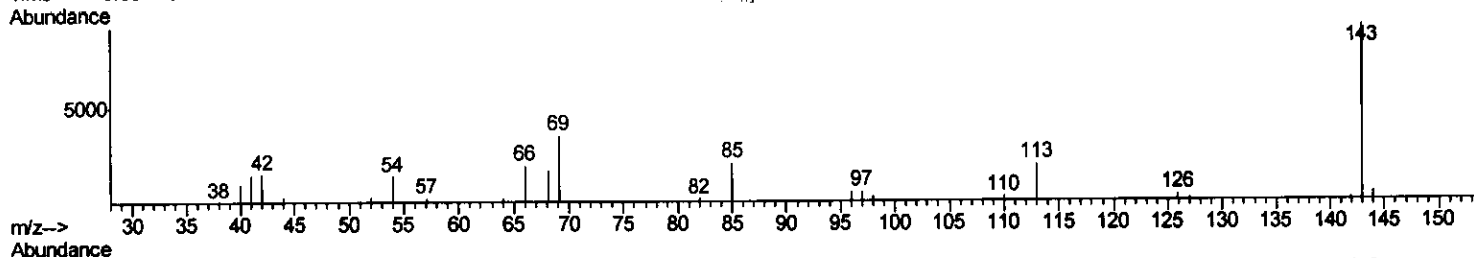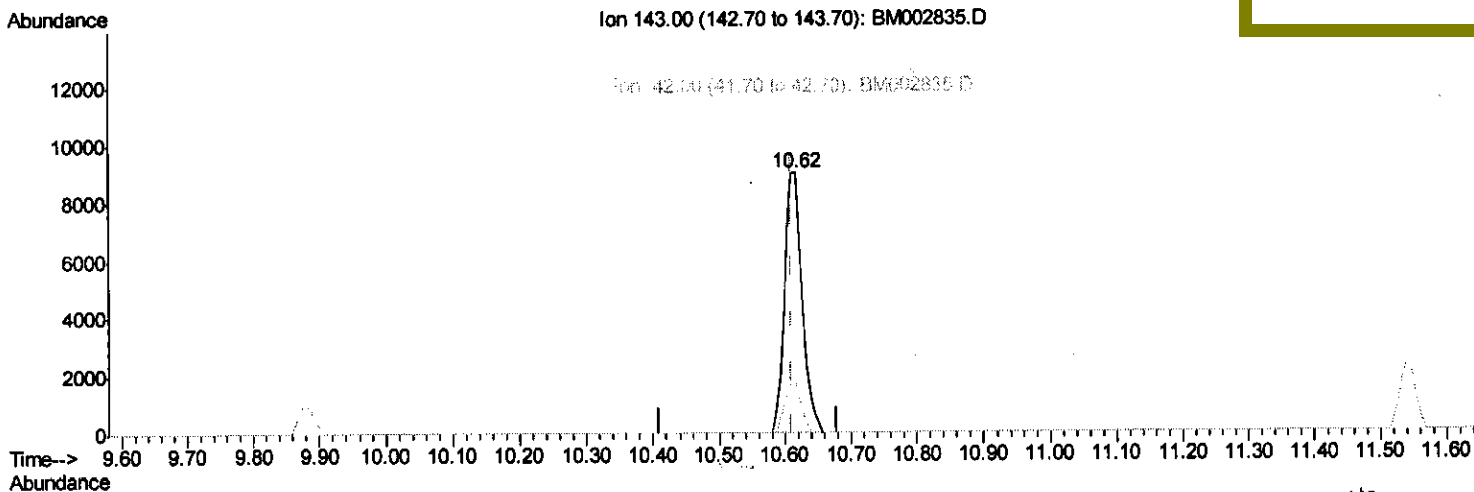

(22) 2-Nitrophenol-d4 (S)

10.616min (+0.006) 8.36ng/ul m

U.M
10/6/15

response 16637

Ion	Exp%	Act%
143.00	100	100
69.00	38.50	40.11
41.00	16.80	18.62
42.00	17.20	19.18

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM100215\
 Data File : BM002835.D
 Acq On : 02 Oct 2015 18:18
 Operator : UM/IZ
 Sample : G3852-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C03G1

Quant Time: Oct 03 01:13:06 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHOD\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 00:37:55 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDADODA
 10/5/2015 1:23:17 PM

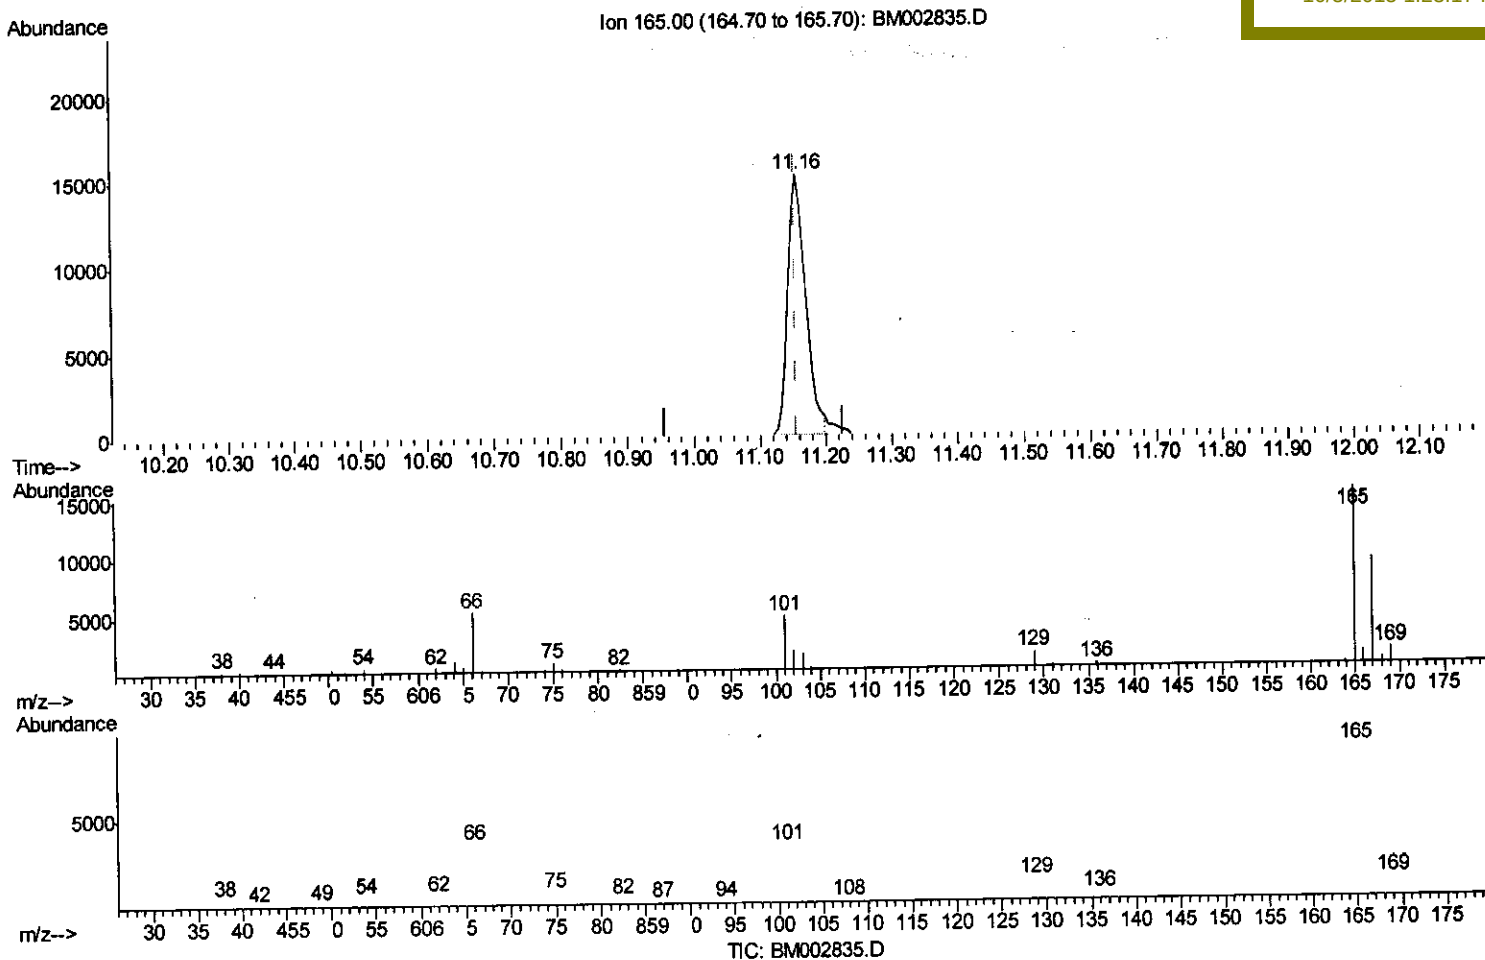

(26) 2,4-Dichlorophenol-d3 (S)

11.157min (+0.000) 8.21ng/ul

response 28856

Ion	Exp%	Act%
165.00	100	100
167.00	61.90	61.25
101.00	32.10	32.15
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM100215\
Data File : BM002835.D
Acq On : 02 Oct 2015 18:18
Operator : UM/IZ
Sample : G3852-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Oct 03 01:13:06 2015
Quant Method : Z:\HPCHEM1\BNA M\METHOD\SOM02.2-EPA-BM092915.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 03 00:37:55 2015
Response via : Initial Calibration

Instrument :
BNA M
ClientSampleId :
C03G1

Manual Integrations
APPROVED

MMDADODA
10/5/2015 1:23:17 PM

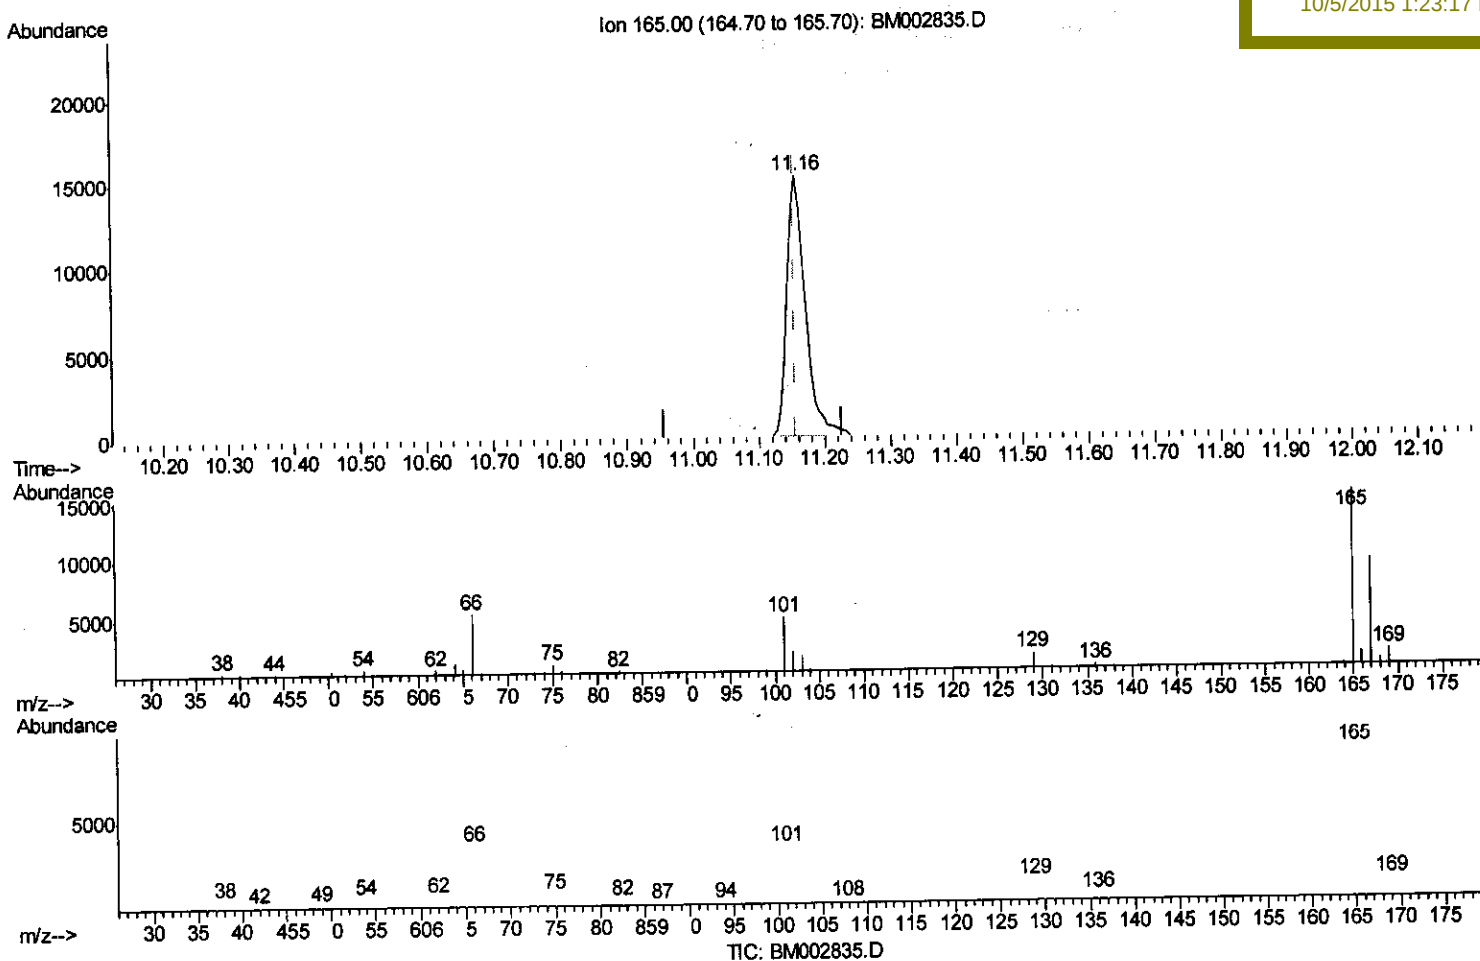

(26) 2,4-Dichlorophenol-d3 (S)

11.157min (+0.000) 8.50ng/ul m

response 29855

Ion	Exp%	Act%
165.00	100	100
167.00	61.90	61.25
101.00	32.10	32.15
0.00	0.00	0.00

U.M
10/6/15

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM100215\
 Data File : BM002835.D
 Acq On : 02 Oct 2015 18:18
 Operator : UM/IZ
 Sample : G3852-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C03G1

Quant Time: Oct 03 01:13:06 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHOD\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 00:37:55 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDADODA
 10/5/2015 1:23:17 PM

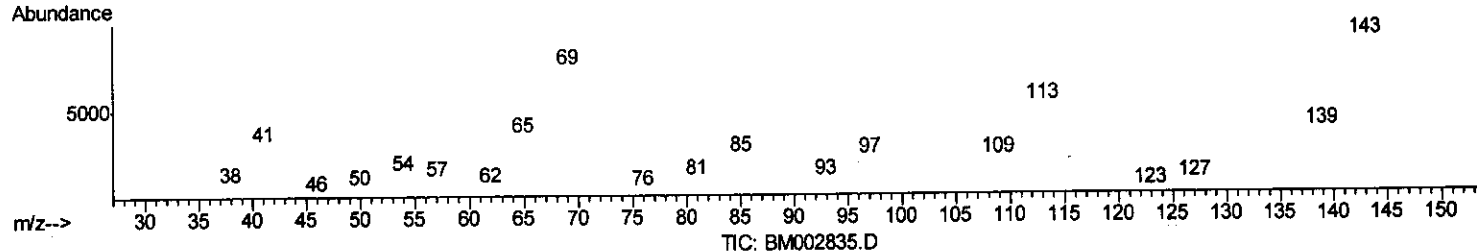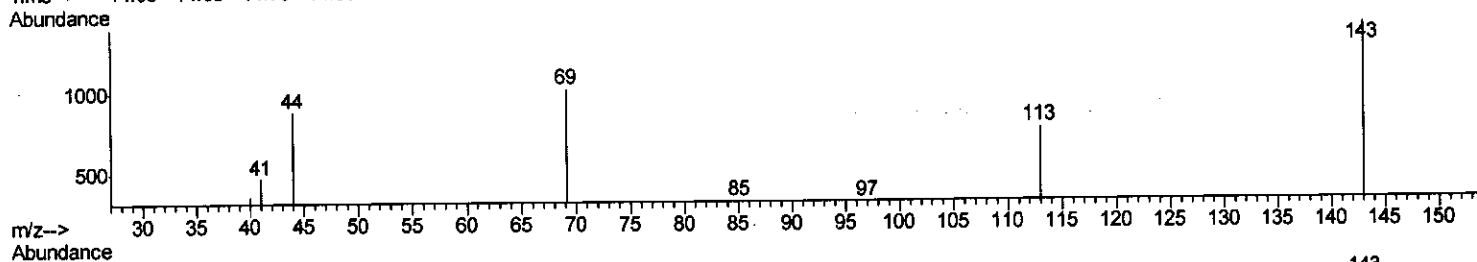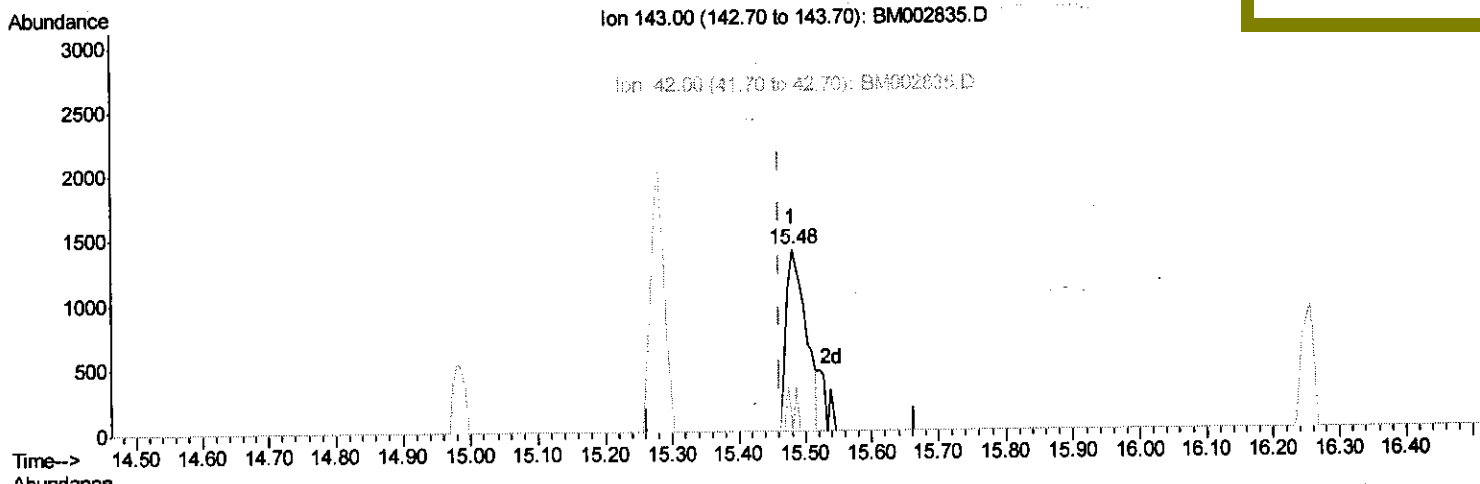

(52) 4-Nitrophenol-d4 (S)

15.480min (+0.018) 1.67ng/ul

response 2891

Ion	Exp%	Act%
143.00	100	100
113.00	54.70	54.39
41.00	31.90	33.40
42.00	21.90	0.00#

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM100215\
 Data File : BM002835.D
 Acq On : 02 Oct 2015 18:18
 Operator : UM/IZ
 Sample : G3852-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C03G1

Quant Time: Oct 03 01:13:06 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHOD\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 00:37:55 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDADODA
 10/5/2015 1:23:17 PM

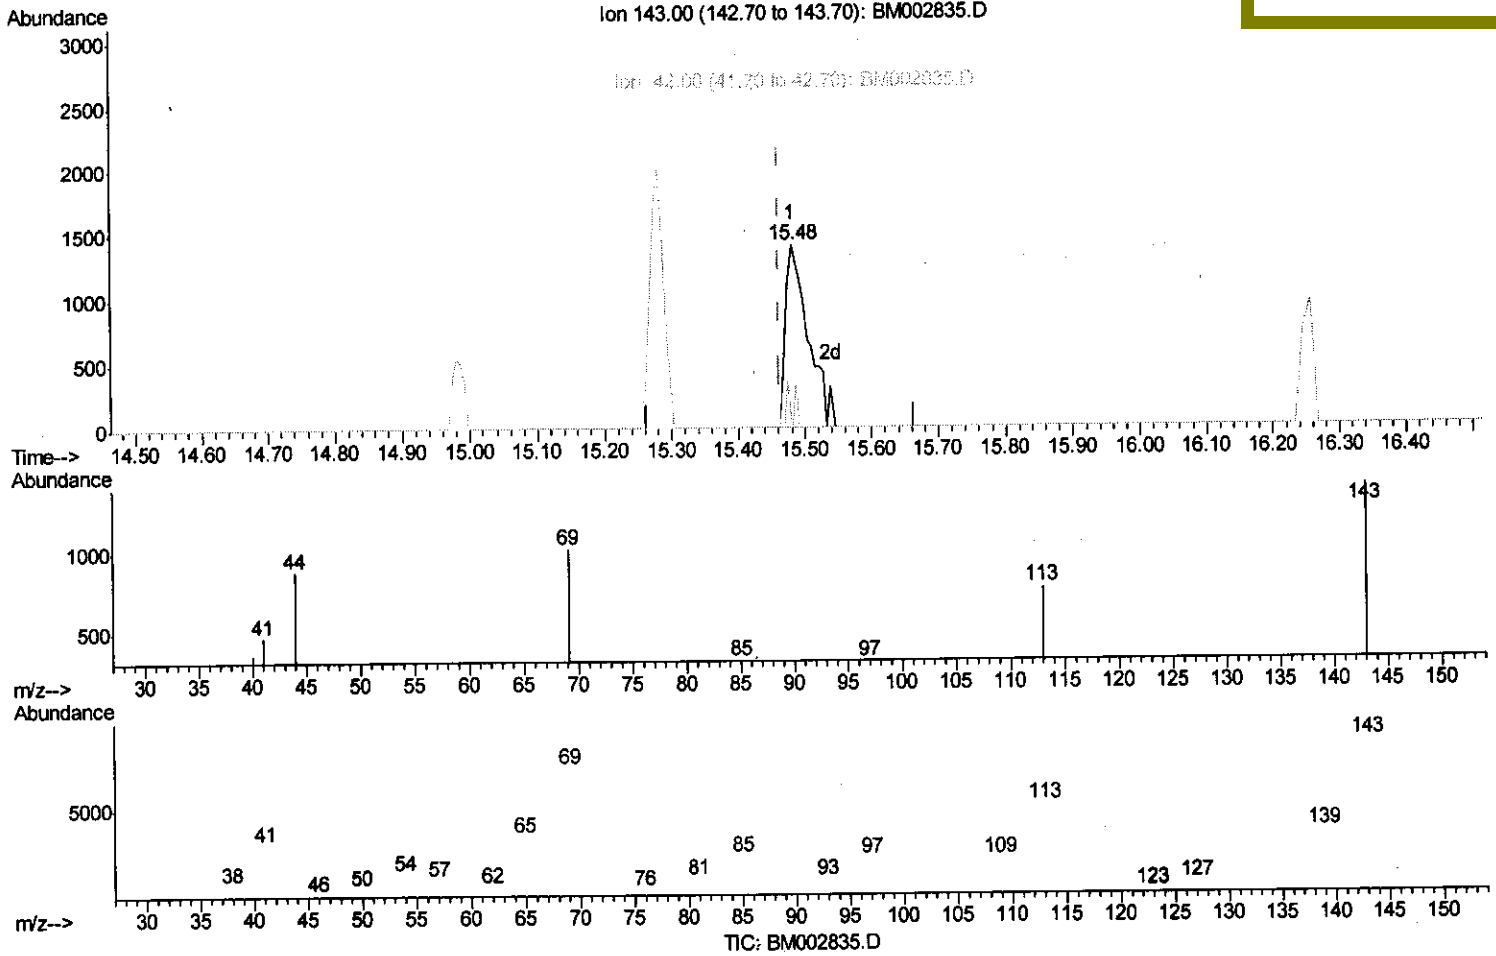

(52) 4-Nitrophenol-d4 (S)

15.480min (+0.018) 1.85ng/ul m

response 3209

Ion Exp% Act%

143.00 100 100

113.00 54.70 54.39

41.00 31.90 33.40

42.00 21.90 0.00#

U. M
 10/6/15

Data Path : Z:\HPCHEM1\BNA M\Data\BM100215\
 Data File : BM002835.D
 Acq On : 02 Oct 2015 18:18
 Operator : UM/IZ
 Sample : G3852-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 C03G1

Quant Time: Oct 03 01:20:43 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHOD\SOM02.2-EPA-BM092915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 00:37:55 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDADODA
 10/5/2015 1:23:17 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.68	152	58380	20.00	ng/ul	0.00
18) Naphthalene-d8	11.54	136	249748	20.00	ng/ul	0.00
36) Acenaphthene-d10	15.28	164	129569	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.99	188	274891	20.00	ng/ul	0.00
78) Chrysene-d12	22.08	240	297830	20.00	ng/ul	0.00
86) Perylene-d12	24.67	264	295639	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.76	96	784	0.62	ng/uL	0.00
5) Phenol-d5	7.81	99	14716m	3.33	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.97	67	23671	9.51	ng/ul	0.00
9) 2-Chlorophenol-d4	8.20	132	35670	8.66	ng/ul	0.00
13) 4-Methylphenol-d8	9.39	113	23197	6.36	ng/ul	0.00
19) Nitrobenzene-d5	9.88	128	16105	8.46	ng/ul	0.00
22) 2-Nitrophenol-d4	10.62	143	16637m	8.36	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	11.16	165	29855m	8.50	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	0.00
44) Dimethylphthalate-d6	14.66	166	92225	9.46	ng/ul	0.00
47) Acenaphthylene-d8	14.99	160	105393	8.10	ng/ul	0.00
52) 4-Nitrophenol-d4	15.48	143	3209m	1.85	ng/ul	0.02
58) Fluorene-d10	16.25	176	73634	8.39	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	16.39	200	5331	3.98	ng/ul	0.00
71) Anthracene-d10	18.09	188	110460	8.42	ng/ul	0.00
79) Pyrene-d10	20.32	212	116484	8.38	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.50	264	125164	8.28	ng/ul	0.00

U.M
 10/6/15

Target Compounds						Ovalue
45) Dimethylphthalate	14.70	163	56225	5.67	ng/ul	99
57) Diethylphthalate	16.03	149	17325	1.74	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed