


Data Path : Z:\HPCHEM1\BNA M\Data\BM100215\
Data File : BM002829.D
Acq On : 02 Oct 2015 12:42
Operator : UM/IZ
Sample : DFTPP20
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP20

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092915.M
Title : SVOA CALIBRATION
Last Update : Fri Oct 02 05:57:21 2015

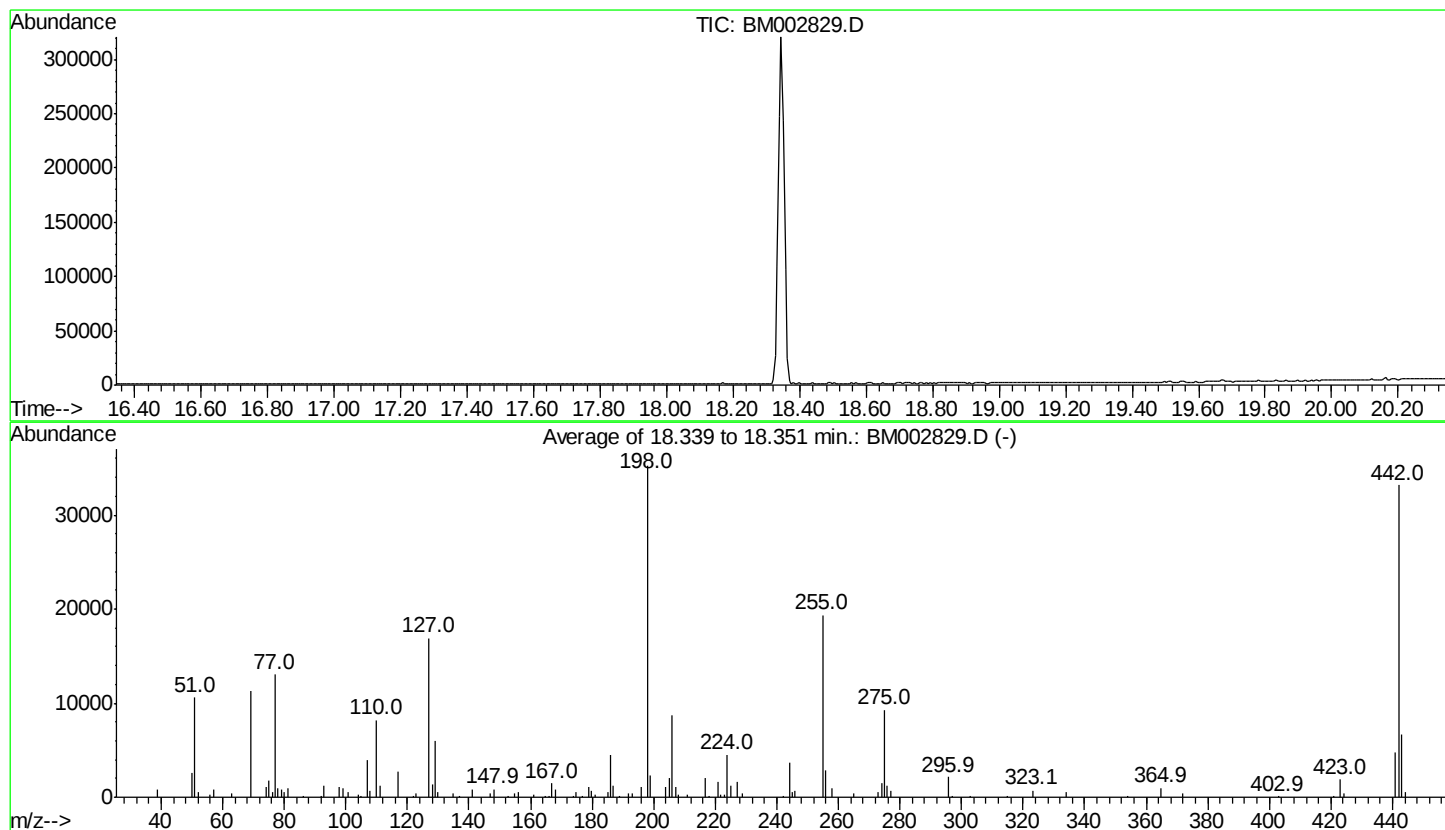

AutoFind: Scans 2593, 2594, 2595; Background Corrected with Scan 2588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	10567	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.2	11345	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	16888	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35253	PASS
199	198	5	9	6.7	2348	PASS
275	198	10	60	26.3	9276	PASS
365	198	1	100	2.9	1007	PASS
441	443	0.01	100	72.0	4766	PASS
442	198	50	100	94.1	33181	PASS
443	442	15	24	19.9	6617	PASS

Scan 2588 (18.310 min): BM002829.D
DFTPP20

m/z	Abundance
44.00	1090.0
207.00	428.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

m/z	Abundance
39.00	819.0
44.00	1061.0
50.00	2776.0
51.00	11125.0
52.00	607.0
55.90	360.0
57.00	877.0
63.00	457.0
69.00	11959.0
74.00	1126.0
75.00	1886.0
76.10	641.0
77.00	13727.0
78.00	1007.0
79.00	912.0
79.90	578.0
81.00	1006.0
91.90	332.0
92.90	1251.0
98.00	1009.0
99.00	1018.0
101.00	462.0
103.90	377.0
107.00	4090.0
108.00	556.0
110.00	8396.0
111.00	1373.0
117.00	2781.0
123.00	435.0
127.00	16608.0
128.00	1448.0
129.00	5938.0
130.00	464.0
135.00	467.0
141.00	774.0
146.90	392.0
147.90	743.0
152.90	327.0
155.00	427.0
156.00	634.0
161.00	372.0
167.00	1316.0
168.00	725.0
175.00	528.0
178.90	1026.0
180.00	643.0
185.00	504.0
186.00	4257.0
187.00	1172.0
191.90	351.0
193.00	387.0
196.00	997.0
198.00	32584.0
199.00	2241.0
204.00	936.0
205.00	1882.0
206.00	7791.0
207.00	1441.0
207.90	301.0
216.90	1694.0
221.00	1530.0
221.70	323.0
223.00	420.0
224.00	3921.0
225.00	1180.0
227.00	1596.0
228.90	358.0
244.00	3247.0
245.00	468.0
246.00	674.0
255.00	16776.0
256.00	2519.0
258.00	872.0
265.00	331.0
272.90	505.0
274.00	1400.0
275.00	8263.0
276.00	1031.0
277.00	520.0
295.90	1909.0
323.00	648.0
334.00	417.0
364.90	774.0
372.00	306.0
423.00	1295.0
424.00	340.0
441.00	3642.0
442.00	24480.0
443.00	5041.0
444.00	400.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

m/z	Abundance
39.00	1042.0
44.00	1076.0
50.10	3016.0
51.00	12360.0
52.00	531.0
55.90	379.0
57.00	955.0
63.00	589.0
69.00	13242.0
74.00	1208.0
75.00	2048.0
76.00	597.0
77.00	15079.0
78.00	977.0
79.00	944.0
80.00	673.0
81.00	1176.0
86.00	313.0
93.00	1541.0
98.00	1268.0
99.00	995.0
100.90	604.0
104.00	399.0
105.00	401.0
107.00	4529.0
108.00	873.0
110.00	9364.0
111.00	1400.0
117.00	3276.0
122.00	365.0
123.00	480.0
127.00	19832.0
128.00	1461.0
129.00	6977.0
129.90	629.0
134.90	511.0
137.00	322.0
140.90	930.0
146.90	497.0
148.00	1016.0
155.00	516.0
156.00	739.0
161.00	434.0
164.90	388.0
166.00	340.0
167.00	1731.0
168.00	932.0
174.00	420.0
174.90	724.0
176.90	422.0
178.90	1331.0
179.90	906.0
181.00	482.0
185.00	713.0
186.00	5171.0
187.00	1617.0
189.00	300.0
192.00	463.0
192.90	591.0
196.00	1301.0
198.00	41808.0
198.90	2743.0
204.00	1232.0
205.00	2428.0
206.00	10463.0
207.10	1750.0
208.00	375.0
210.80	349.0
217.00	2492.0
218.00	345.0
221.00	1935.0
221.70	418.0
222.90	530.0
224.00	5469.0
225.00	1374.0
227.00	1872.0
229.00	425.0
242.00	337.0
244.00	4489.0
245.00	516.0
246.00	758.0
255.00	23136.0
256.00	3459.0
257.90	1084.0
264.90	483.0
272.90	717.0
274.00	1746.0
275.00	10470.0
276.00	1418.0
276.90	880.0
296.00	2608.0
296.90	347.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

303.00	327.0
315.00	306.0
323.10	700.0
334.00	622.0
354.10	355.0
365.00	1071.0
372.00	485.0
423.00	2182.0
424.10	418.0
441.00	5612.0
442.00	38248.0
443.00	7726.0
444.00	746.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

m/z	Abundance
39.00	644.0
44.00	997.0
50.00	1860.0
51.10	8216.0
52.00	395.0
57.00	638.0
62.90	341.0
69.00	8835.0
74.00	895.0
75.00	1419.0
76.00	518.0
77.10	10354.0
78.00	690.0
79.00	568.0
80.00	532.0
81.00	760.0
93.00	1053.0
98.00	1031.0
99.00	741.0
100.90	435.0
107.00	3245.0
108.00	589.0
110.00	6789.0
111.00	1072.0
117.00	1989.0
122.90	407.0
127.00	14224.0
128.00	1019.0
129.00	4996.0
129.90	368.0
134.90	454.0
141.00	736.0
147.00	401.0
147.90	711.0
155.00	411.0
156.00	466.0
167.00	1268.0
167.90	665.0
175.00	475.0
178.90	1006.0
180.00	616.0
180.90	379.0
184.90	458.0
186.00	4065.0
187.00	1078.0
192.00	340.0
193.00	353.0
195.90	996.0
198.00	31368.0
198.90	2060.0
204.00	924.0
205.00	1696.0
206.00	7801.0
207.00	1324.0
207.90	318.0
210.90	308.0
217.00	1891.0
221.00	1585.0
224.00	4196.0
225.00	1118.0
227.00	1594.0
229.00	441.0
244.00	3469.0
245.00	467.0
245.90	644.0
255.00	18184.0
256.00	2653.0
258.00	915.0
264.90	399.0
272.90	520.0
274.00	1545.0
275.00	9097.0
275.90	1054.0
276.90	581.0
296.00	1934.0
323.00	893.0
334.00	471.0
365.00	1177.0
372.00	445.0
402.90	364.0
421.00	305.0
423.00	2122.0
424.00	386.0
441.00	5044.0
442.00	36816.0
443.00	7084.0
444.00	583.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20