


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100220\
Data File : BM027580.D
Acq On : 02 Oct 2020 14:27
Operator : JU/CG
Sample : L4188-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG0Q9

Manual Integrations
APPROVED

mohammad
10/5/2020 10:28:40 AM

Quant Time: Oct 02 15:01:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 13:04:03 2020
Response via : Initial Calibration

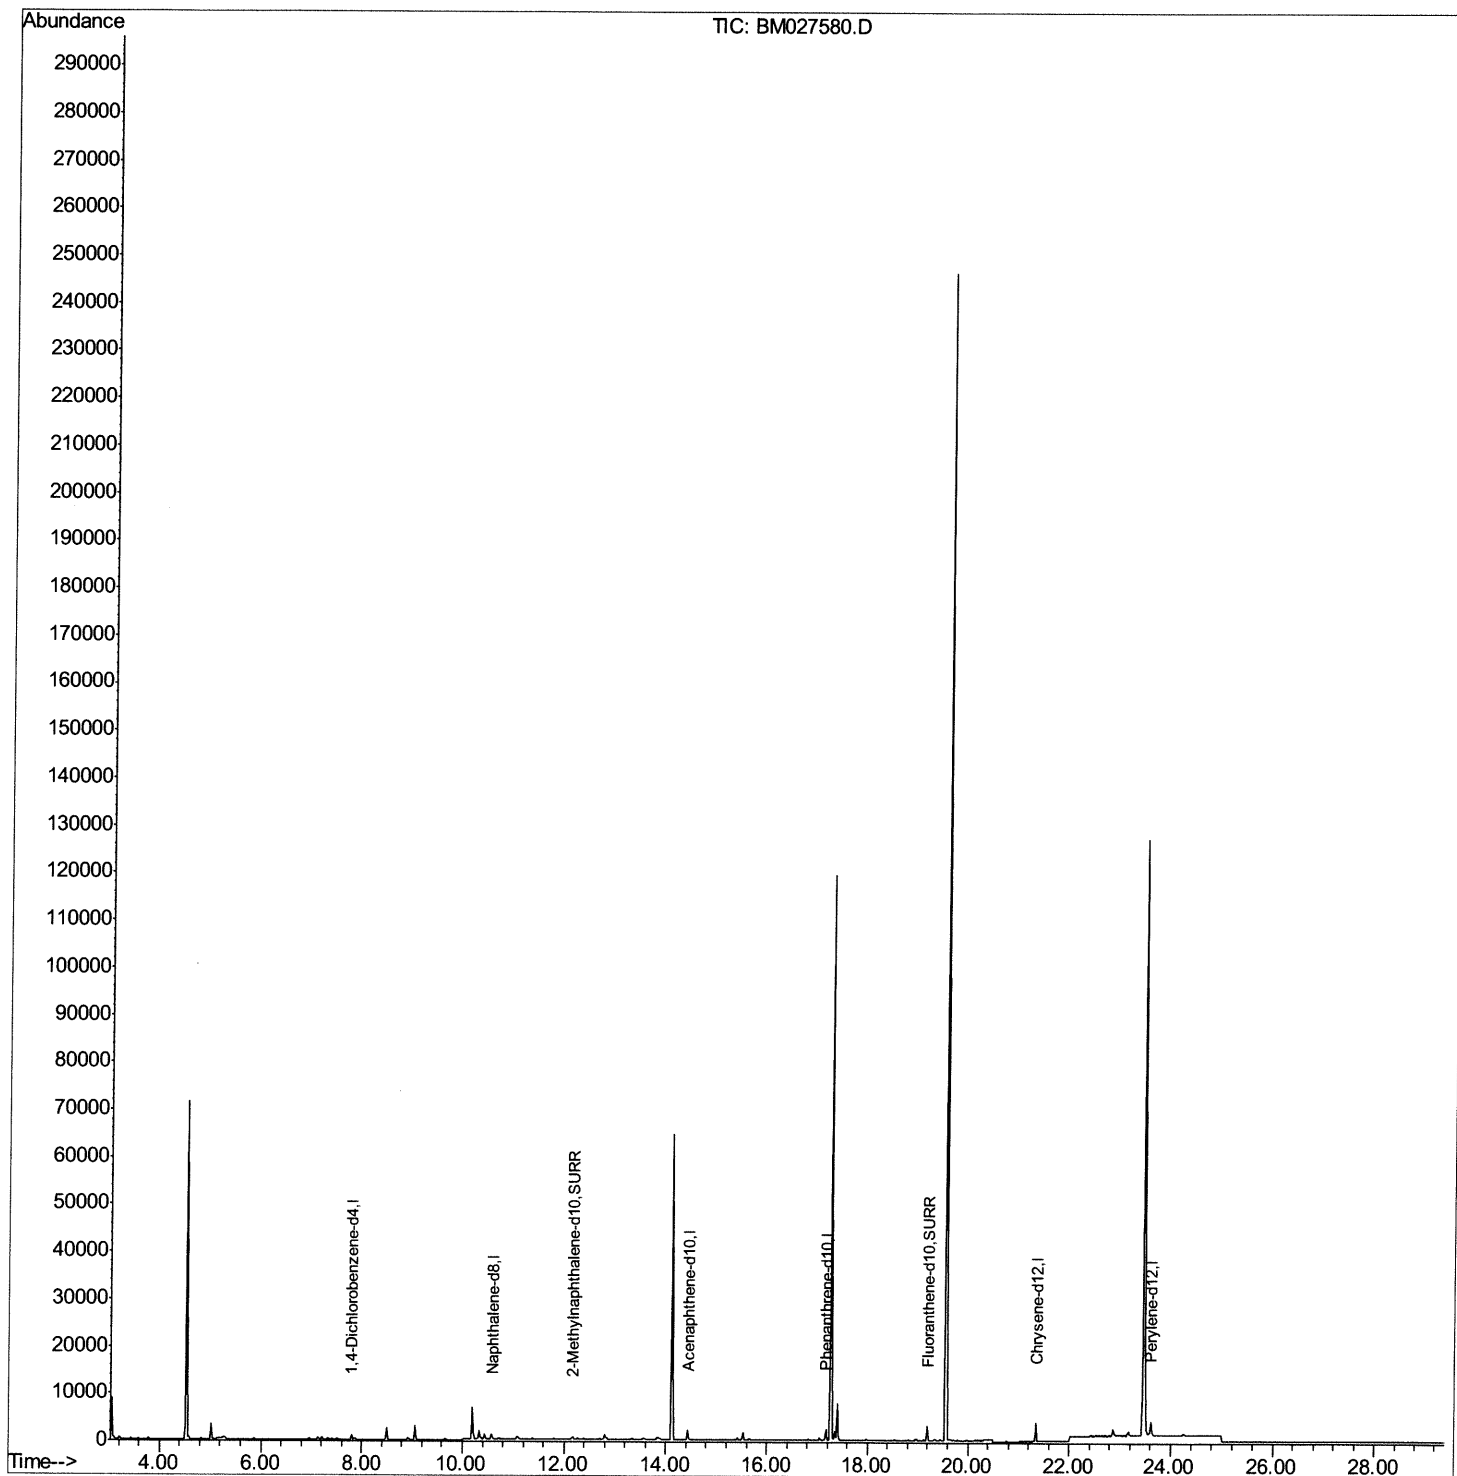

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100220\
Data File : BM027580.D
Acq On : 02 Oct 2020 14:27
Operator : JU/CG
Sample : L4188-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG0Q9

Manual Integrations
APPROVED

mohammad
10/5/2020 10:28:40 AM

Quant Time: Oct 02 15:00:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 13:04:03 2020
Response via : Initial Calibration

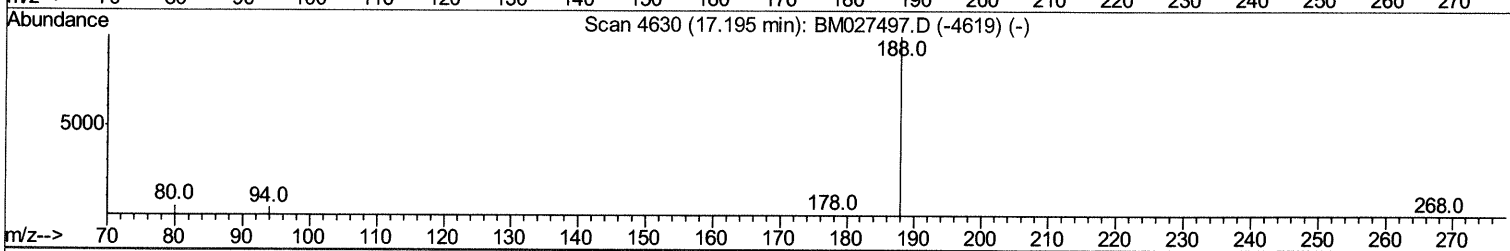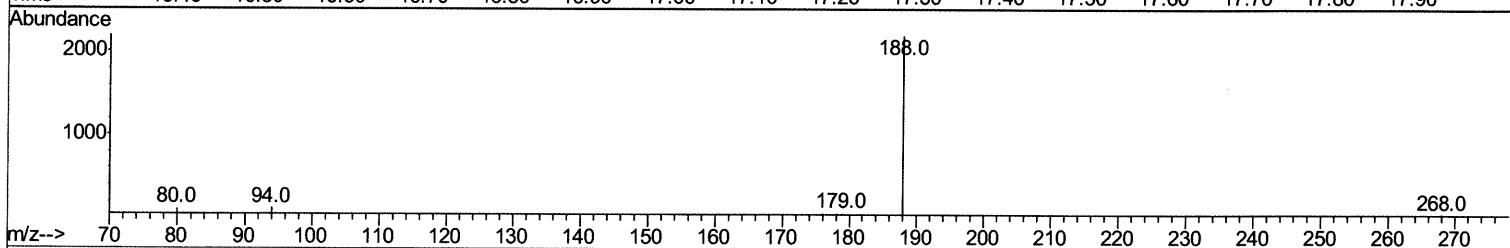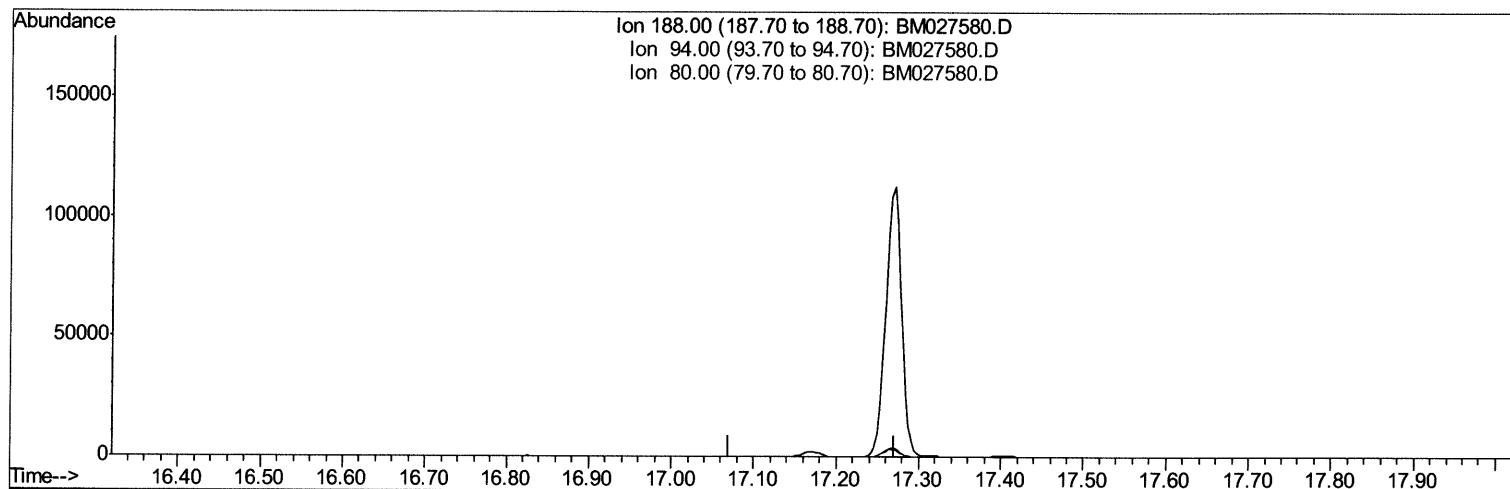

TIC: BM027580.D

(10) Phenanthrene-d10 (I)

17.171min (-17.171) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	5.20	0.00#
80.00	6.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100220\
 Data File : BM027580.D
 Acq On : 02 Oct 2020 14:27
 Operator : JU/CG
 Sample : L4188-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG0Q9

Manual Integrations
 APPROVED

mohammad
 10/5/2020 10:28:40 AM

Quant Time: Oct 02 15:00:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 02 13:04:03 2020
 Response via : Initial Calibration

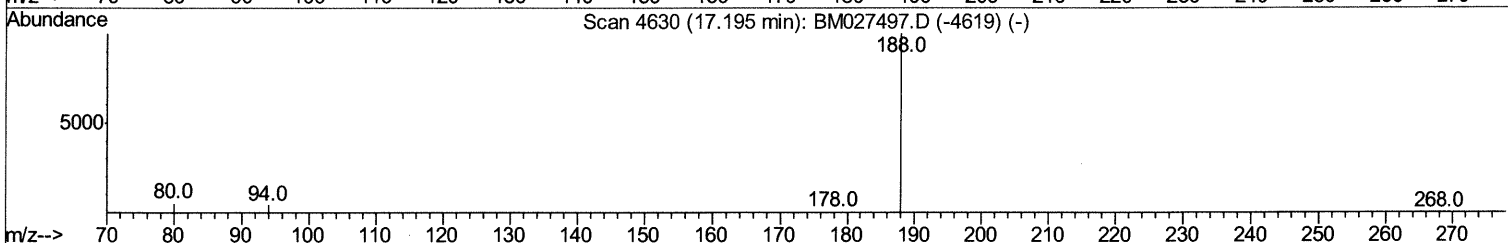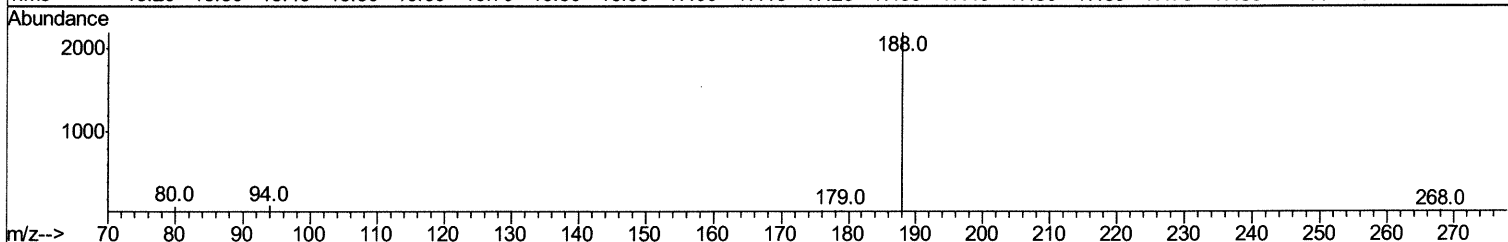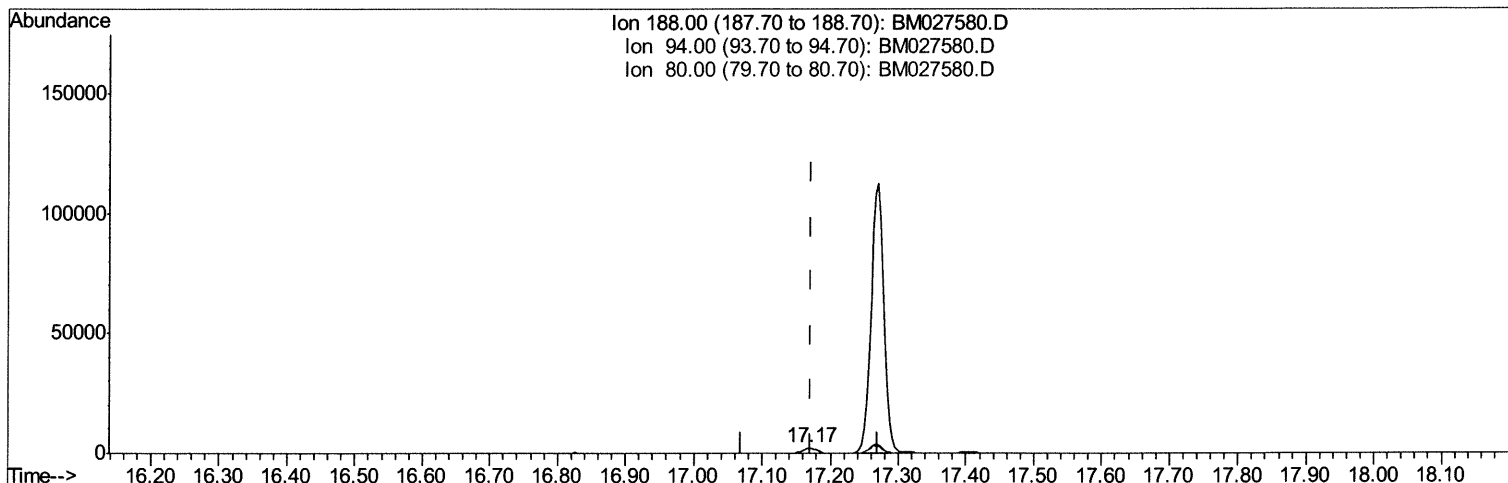

TIC: BM027580.D

(10) Phenanthrene-d10 (I)

17.169min (-0.002) 0.40ng/ul m

~~10/06/20~~ JU

response 3157

Ion	Exp%	Act%
188.00	100	100
94.00	5.20	5.23
80.00	6.20	5.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100220\
Data File : BM027580.D
Acq On : 02 Oct 2020 14:27
Operator : JU/CG
Sample : L4188-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG0Q9

Manual Integrations
APPROVED

mohammad
10/5/2020 10:28:40 AM

Quant Time: Oct 02 15:01:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 13:04:03 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	522	0.40	ng/ul	0.00
2) Naphthalene-d8	10.59	136	1413	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.43	164	1115	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.17	188	3157m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.35	240	3688	0.40	ng/ul	0.00
20) Perylene-d12	23.61	264	3807	0.40	ng/ul	0.00

10/06/2020

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.17	152	639	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.20	212	3504	0.41	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed