


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100220\
Data File : BM027583.D
Acq On : 02 Oct 2020 16:21
Operator : JU/CG
Sample : L4166-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
10/5/2020 10:28:47 AM

Quant Time: Oct 02 16:56:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 13:04:03 2020
Response via : Initial Calibration

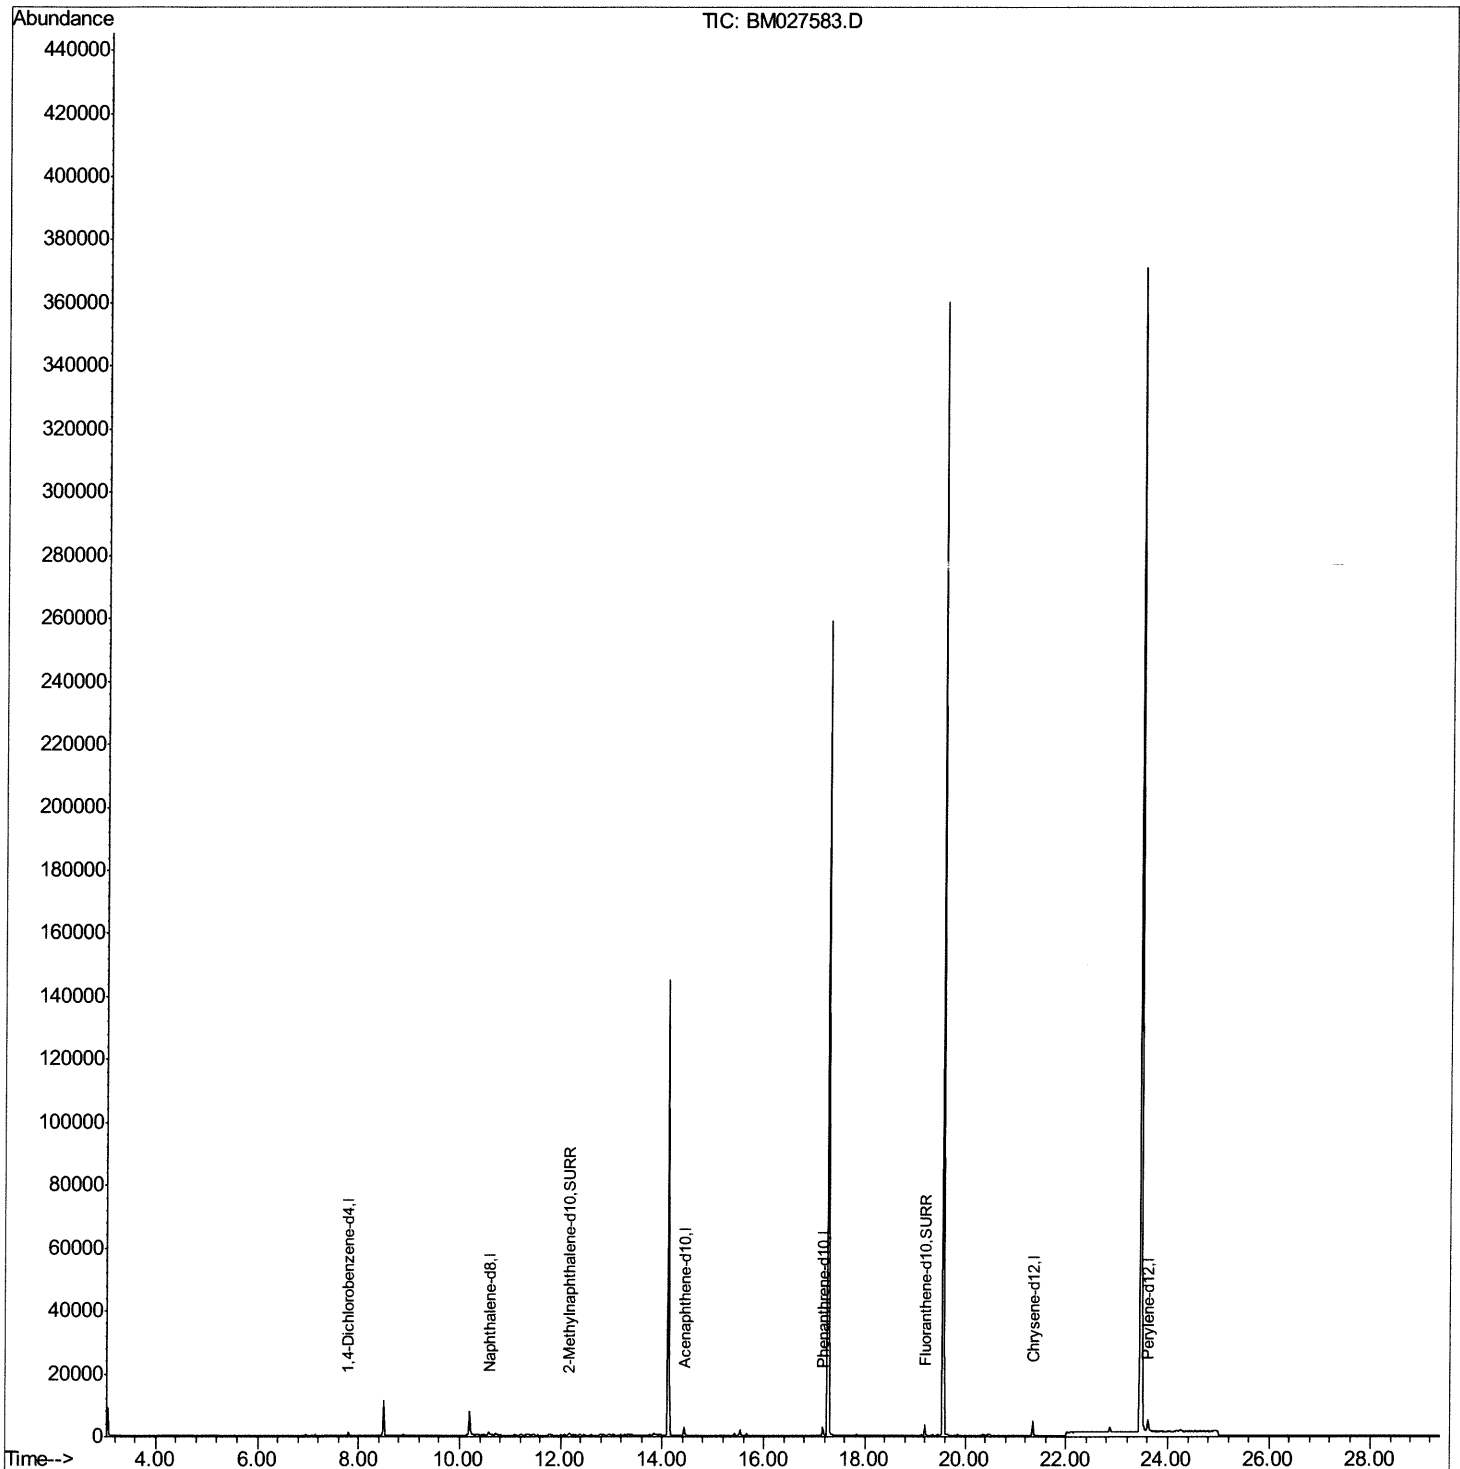

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100220\
 Data File : BM027583.D
 Acq On : 02 Oct 2020 16:21
 Operator : JU/CG
 Sample : L4166-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF1

Manual Integrations
 APPROVED

mohammad
 10/5/2020 10:28:47 AM

Quant Time: Oct 02 16:55:41 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 02 13:04:03 2020
 Response via : Initial Calibration

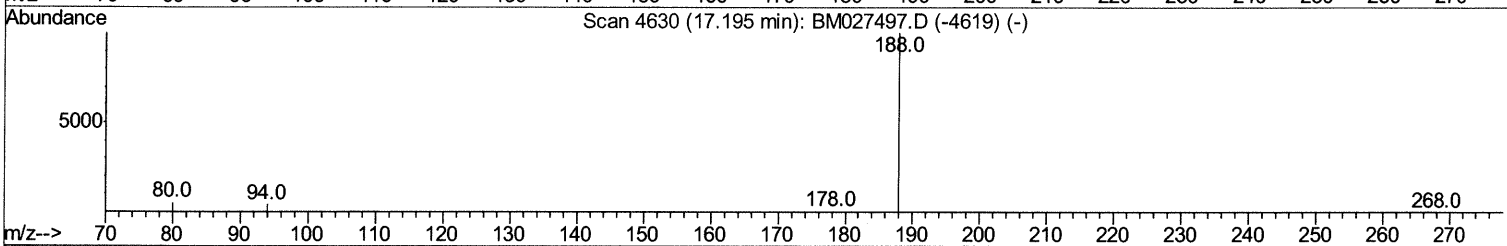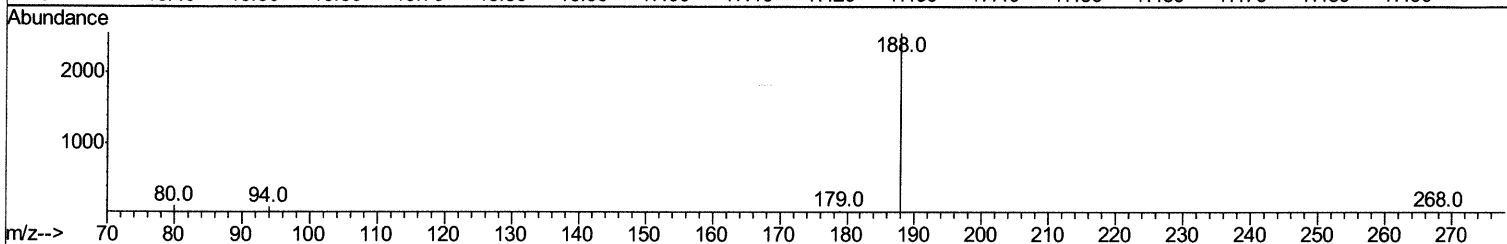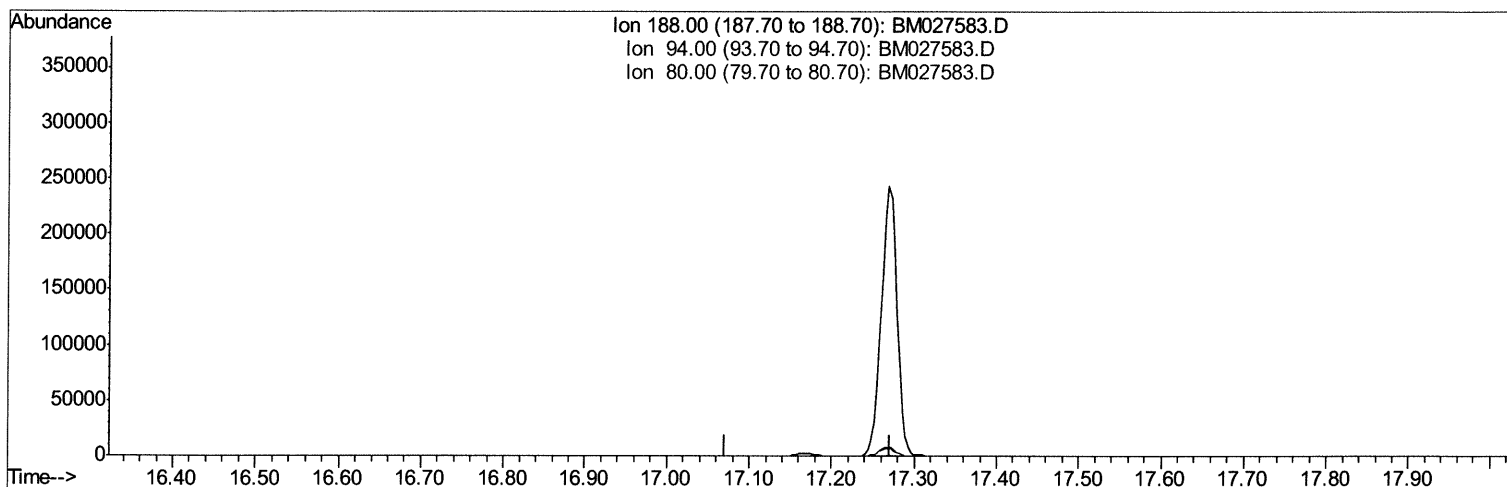

TIC: BM027583.D

(10) Phenanthrene-d10 (I)
 17.171min (-17.171) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	5.20	0.00#
80.00	6.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100220\
Data File : BM027583.D
Acq On : 02 Oct 2020 16:21
Operator : JU/CG
Sample : L4166-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
10/5/2020 10:28:47 AM

Quant Time: Oct 02 16:55:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 13:04:03 2020
Response via : Initial Calibration

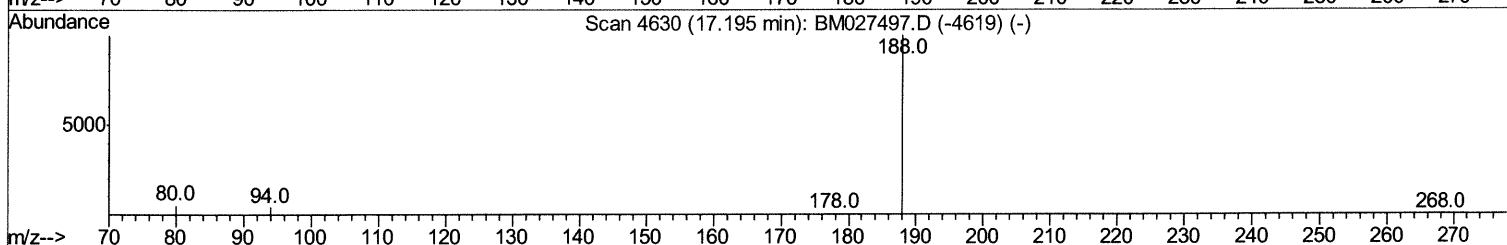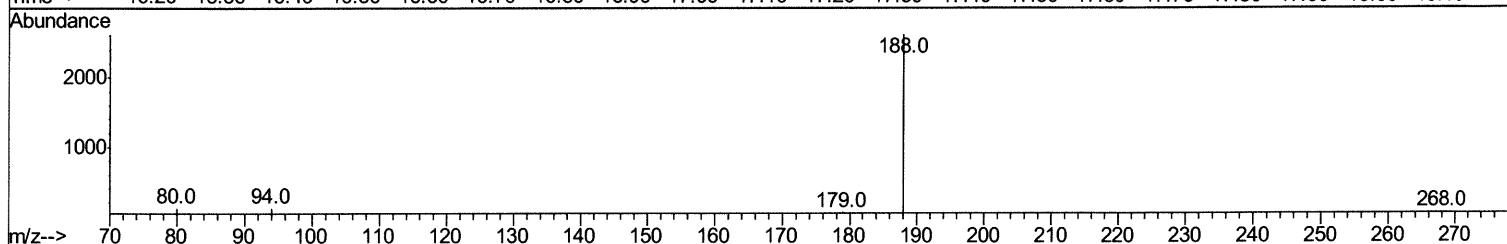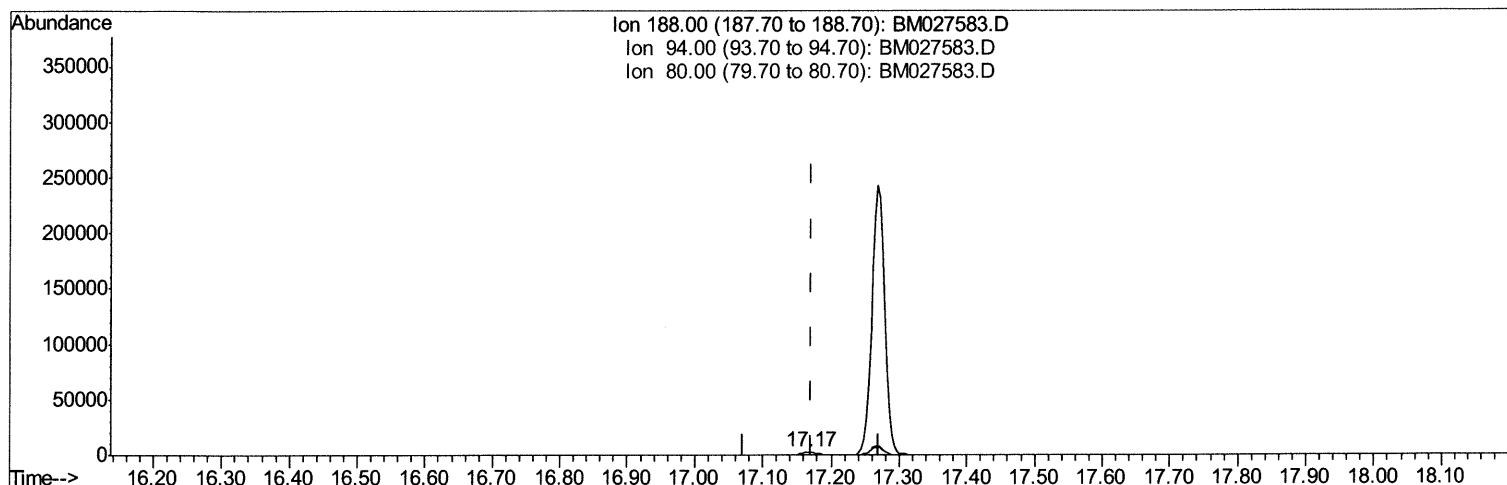

TIC: BM027583.D

(10) Phenanthrene-d10 (I)

17.168min (-0.003) 0.40ng/ul m 10/06/20 JU

response 3718

Ion	Exp%	Act%
188.00	100	100
94.00	5.20	4.69
80.00	6.20	4.53#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM100220\
Data File : BM027583.D
Acq On : 02 Oct 2020 16:21
Operator : JU/CG
Sample : L4166-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
10/5/2020 10:28:47 AM

Quant Time: Oct 02 16:56:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 02 13:04:03 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	534	0.40	ng/ul	0.00
2) Naphthalene-d8	10.58	136	1530	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.43	164	1410	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.17	188	3718m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.35	240	4390	0.40	ng/ul	0.00
20) Perylene-d12	23.61	264	4976	0.40	ng/ul	0.00

10/06/20 JG

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.17	152	888	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.19	212	4155	0.41	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed