

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
 Data File : BM047779.D
 Acq On : 02 Oct 2024 16:38
 Operator : RC/JU
 Sample : P4018-07DL2 30X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCB3DL2

Quant Time: Oct 03 01:09:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 02:30:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	210856	20.000	ng/ul	0.00
20) Naphthalene-d8	10.598	136	852311	20.000	ng/ul	#-0.01
38) Acenaphthene-d10	14.439	164	563133	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.180	188	1223274	20.000	ng/ul	0.00
79) Chrysene-d12	21.403	240	1179309	20.000	ng/ul	0.00
88) Perylene-d12	24.409	264	1354211	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.263	96	894	0.137	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.975	99	9862	0.495	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.139	67	7747	0.548	ng/ul	0.00
11) 2-Chlorophenol-d4	7.339	132	8870	0.611	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113	6871	0.463	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	3688	0.543	ng/ul	0.00
24) 2-Nitrophenol-d4	9.686	143	2932	0.451	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	6692	0.515	ng/ul	0.00
31) 4-Chloroaniline-d4	10.739	131	8962	0.446	ng/ul	0.00
46) Dimethylphthalate-d6	13.851	166	30363	0.744	ng/ul	0.00
49) Acenaphthylene-d8	14.133	160	32287	0.667	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.433	176	27101	0.766	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.539	200	1372	0.192	ng/ul	-0.01
73) Anthracene-d10	17.274	188	41684	0.693	ng/ul	-0.01
81) Pyrene-d10	19.562	212	49979	0.747	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.197	264	48623	0.692	ng/ul	-0.01
Target Compounds						
58) 2,3,4,6-Tetrachlorophenol	15.062	232	54406	5.951	ng/ul#	98
71) Pentachlorophenol	16.833	266	634171	67.966	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
Data File : BM047779.D
Acq On : 02 Oct 2024 16:38
Operator : RC/JU
Sample : P4018-07DL2 30X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCB3DL2

Quant Time: Oct 03 01:09:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration




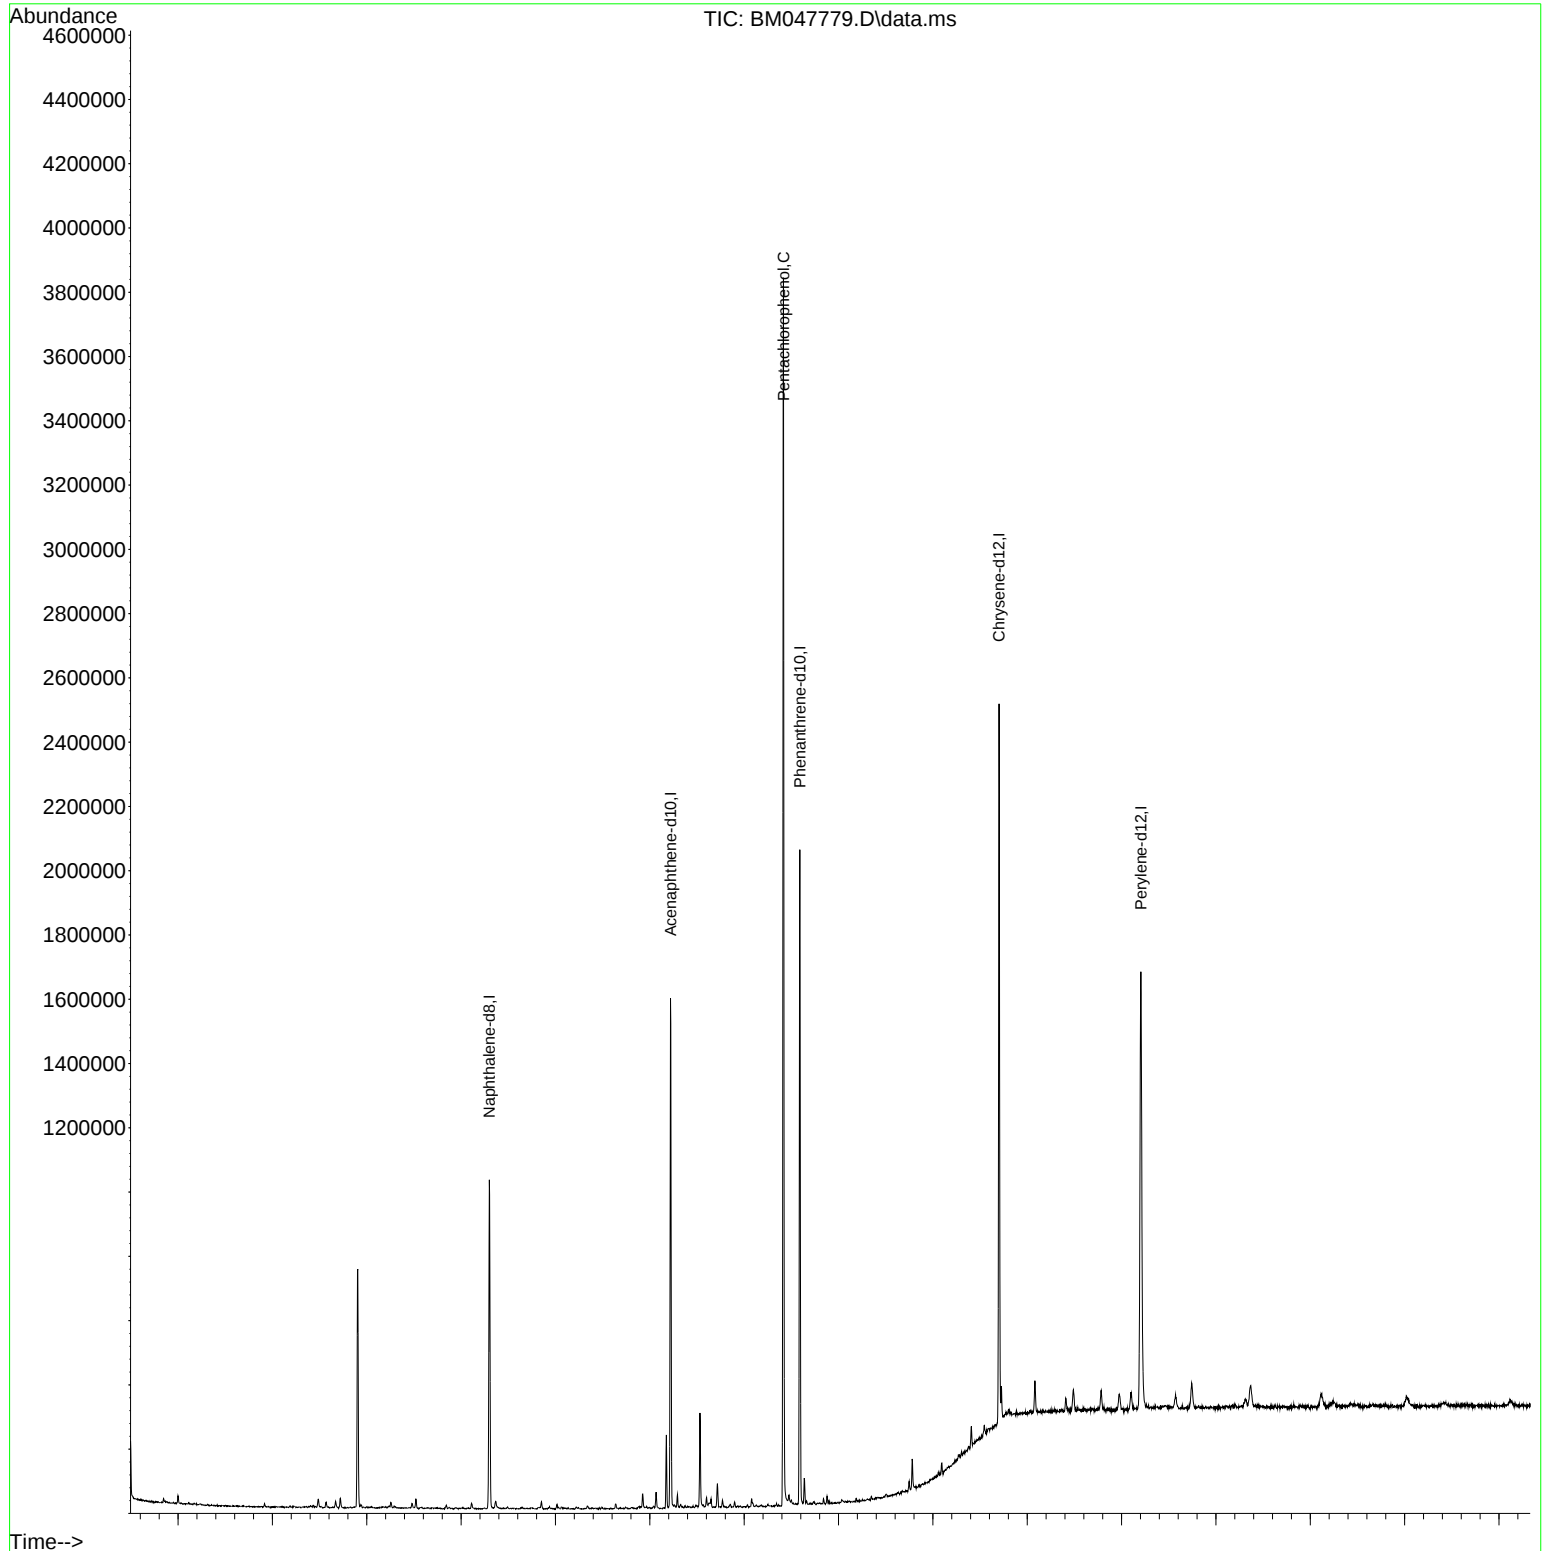


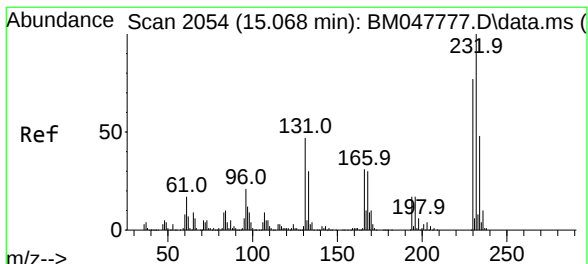

#58
 2,3,4,6-Tetrachlorophenol
 Concen: 5.951 ng/ul
 RT: 15.062 min Scan# 2053
 Delta R.T. -0.006 min
 Lab File: BM047779.D
 Acq: 02 Oct 2024 16:38

Instrument :
 BNA_M
 ClientSampleId :
 DDCB3DL2

Tgt Ion:	232	Resp:	54406
Ion Ratio	Lower	Upper	
232	100		
131	49.4	40.2	60.4
130	2.4	2.6	4.0
166	32.6	25.3	37.9

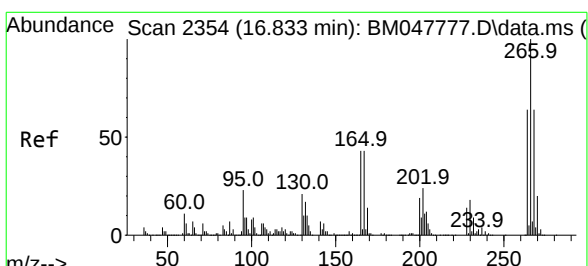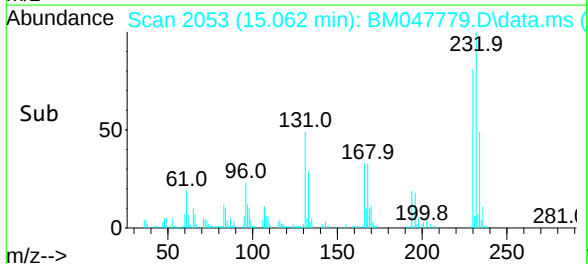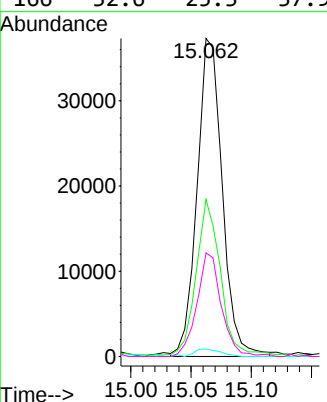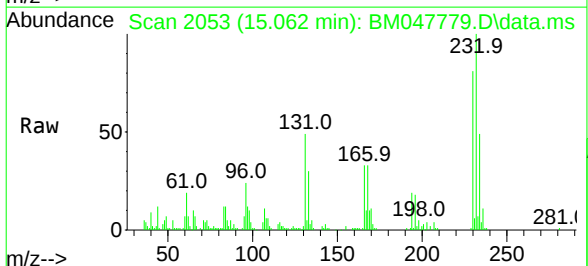

#71
 Pentachlorophenol
 Concen: 67.966 ng/ul
 RT: 16.833 min Scan# 2354
 Delta R.T. -0.006 min
 Lab File: BM047779.D
 Acq: 02 Oct 2024 16:38

Tgt Ion:	266	Resp:	634171
Ion Ratio	Lower	Upper	
266	100		
264	62.7	50.2	75.2
268	65.3	50.9	76.3

