

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
 Data File : BM047781.D
 Acq On : 02 Oct 2024 17:57
 Operator : RC/JU
 Sample : P4018-06DL 20X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCB2DL

Quant Time: Oct 03 01:12:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 02:30:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	187368	20.000	ng/ul	0.00
20) Naphthalene-d8	10.598	136	735827	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.439	164	462658	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.180	188	982113	20.000	ng/ul	0.00
79) Chrysene-d12	21.403	240	933825	20.000	ng/ul	0.00
88) Perylene-d12	24.409	264	1080974	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.975	99	9926	0.560	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	7615	0.606	ng/ul	0.00
11) 2-Chlorophenol-d4	7.345	132	8631	0.670	ng/ul	0.00
15) 4-Methylphenol-d8	8.510	113	6774	0.514	ng/ul	0.00
21) Nitrobenzene-d5	8.957	128	3666	0.626	ng/ul	-0.01
24) 2-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	10.228	165	6673	0.595	ng/ul	0.00
31) 4-Chloroaniline-d4	10.739	131	7826	0.451	ng/ul	0.00
46) Dimethylphthalate-d6	13.851	166	29725	0.886	ng/ul	0.00
49) Acenaphthylene-d8	14.133	160	31946	0.803	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.433	176	25007	0.861	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.274	188	38489	0.797	ng/ul	-0.01
81) Pyrene-d10	19.562	212	45201	0.853	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.197	264	44054	0.785	ng/ul	-0.01
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.833	266	415778	55.502	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
Data File : BM047781.D
Acq On : 02 Oct 2024 17:57
Operator : RC/JU
Sample : P4018-06DL 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCB2DL


Quant Time: Oct 03 01:12:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

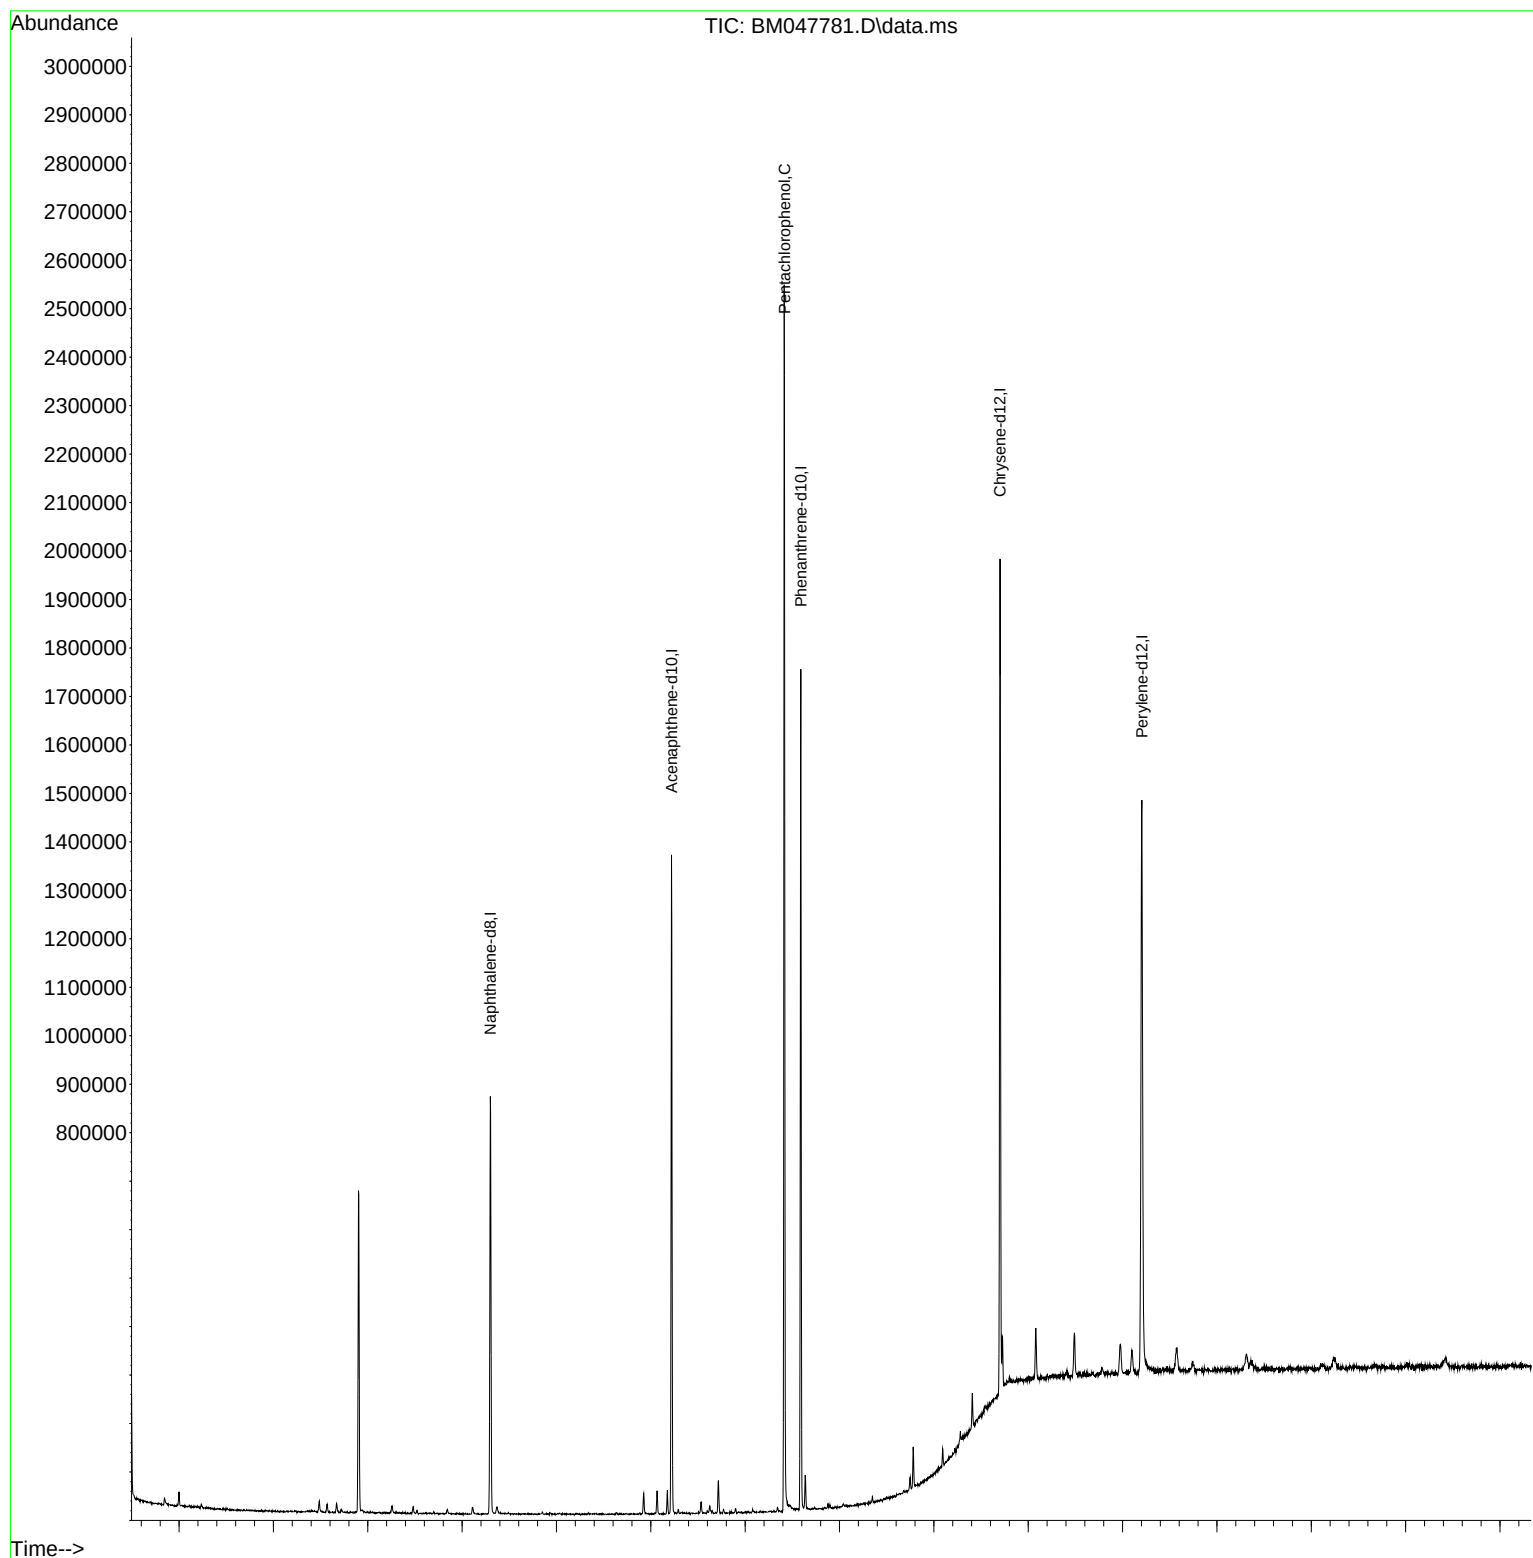

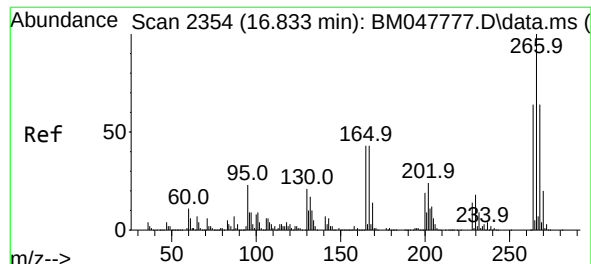

#71
 Pentachlorophenol
 Concen: 55.502 ng/ul
 RT: 16.833 min Scan# 2354
 Delta R.T. -0.006 min
 Lab File: BM047781.D
 Acq: 02 Oct 2024 17:57

Instrument :
 BNA_M
 ClientSampleId :
 DDCB2DL

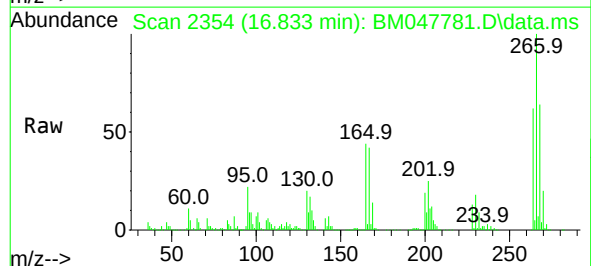

Tgt Ion:	266	Resp:	415778
Ion	Ratio	Lower	Upper
266	100		
264	62.0	50.2	75.2
268	64.2	50.9	76.3

