

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
 Data File : BM047788.D
 Acq On : 02 Oct 2024 22:32
 Operator : RC/JU
 Sample : P4020-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCJ9

Quant Time: Oct 02 23:25:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 02:30:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	244039	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.598	136	996836	20.000	ng/ul	#-0.01
38) Acenaphthene-d10	14.439	164	616290	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.180	188	1259462	20.000	ng/ul	0.00
79) Chrysene-d12	21.403	240	1240995	20.000	ng/ul	0.00
88) Perylene-d12	24.403	264	1443053	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.251	96	14760	1.955	ng/uL	0.00
4) Pyridine-d5	3.669	84	158423	7.165	ng/ul	0.00
7) Phenol-d5	6.969	99	286165	12.401	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	179719	10.975	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.339	132	225327	13.421	ng/ul	0.00
15) 4-Methylphenol-d8	8.510	113	231117	13.471	ng/ul	0.00
21) Nitrobenzene-d5	8.957	128	109216	13.761	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.680	143	110532	14.532	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.216	165	218616	14.388	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.727	131	309524	13.177	ng/ul	-0.01
46) Dimethylphthalate-d6	13.845	166	750585	16.799	ng/ul	-0.01
49) Acenaphthylene-d8	14.133	160	842690	15.907	ng/ul	0.00
54) 4-Nitrophenol-d4	14.627	143	102090	11.476	ng/ul	0.00
60) Fluorene-d10	15.427	176	653258	16.879	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.539	200	66887	9.075	ng/ul	-0.01
73) Anthracene-d10	17.274	188	1042078	16.827	ng/ul	-0.01
81) Pyrene-d10	19.562	212	1259723	17.886	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.197	264	1317793	17.601	ng/ul	-0.01
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.827	266	21188	2.206	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
Data File : BM047788.D
Acq On : 02 Oct 2024 22:32
Operator : RC/JU
Sample : P4020-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCJ9


Quant Time: Oct 02 23:25:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

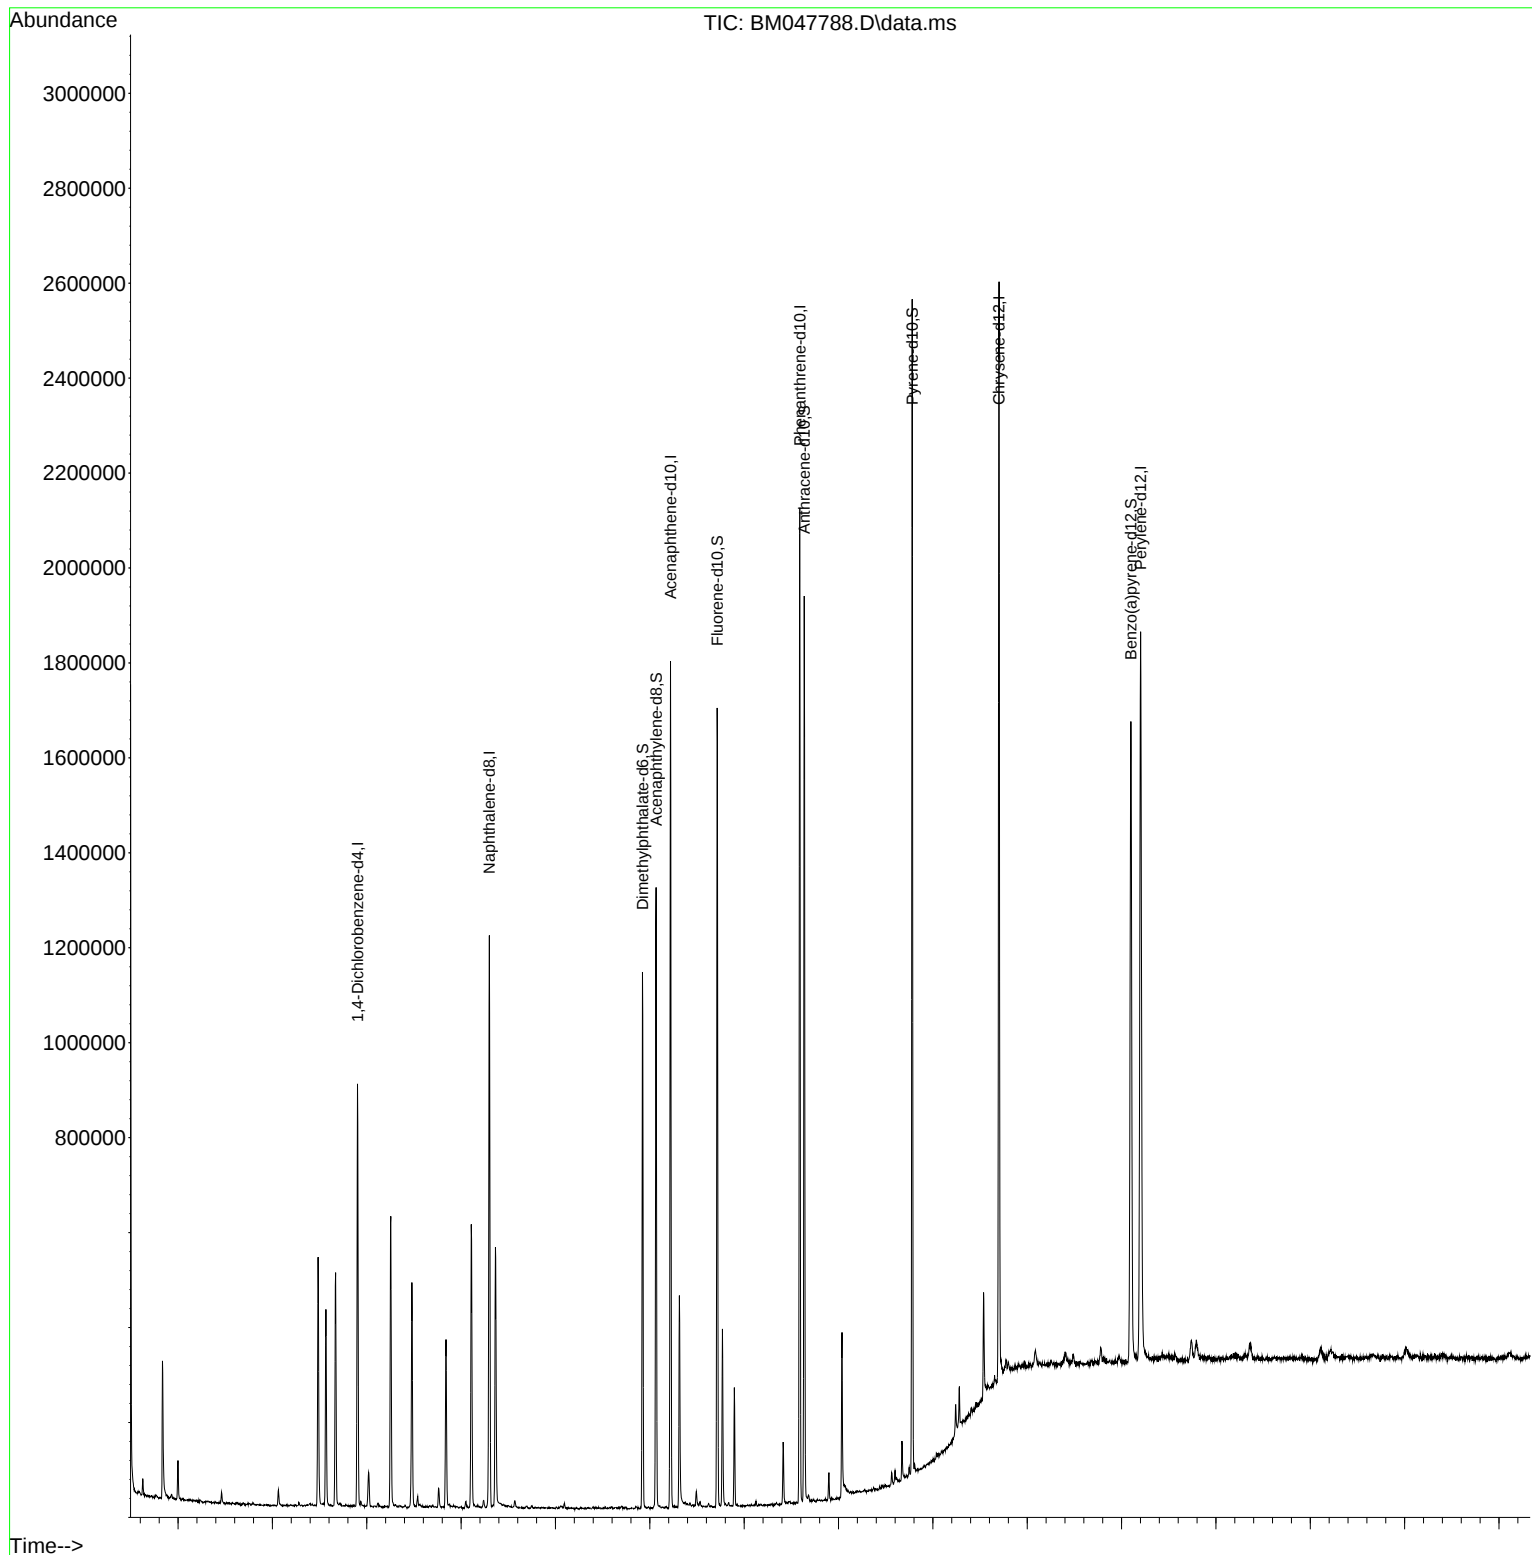

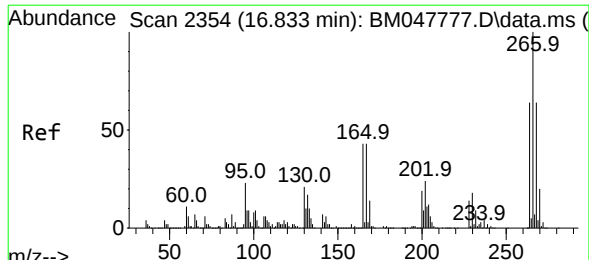

#71
Pentachlorophenol
Concen: 2.206 ng/ul
RT: 16.827 min Scan# 2353
Delta R.T. -0.012 min
Lab File: BM047788.D
Acq: 02 Oct 2024 22:32

Instrument :
BNA_M
ClientSampleId :
DDCJ9

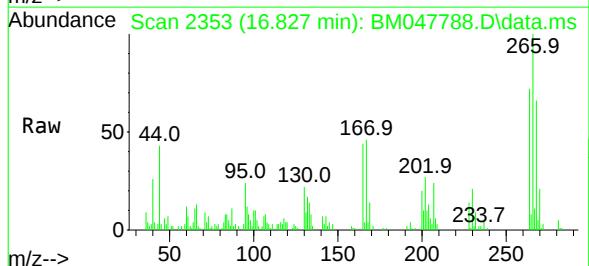

Tgt Ion:	266	Resp:	21188
Ion	Ratio	Lower	Upper
266	100		
264	72.4	50.2	75.2
268	65.5	50.9	76.3

