

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
 Data File : BM047778.D
 Acq On : 02 Oct 2024 15:59
 Operator : RC/JU
 Sample : PB163608BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK608

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047778.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	42	45	53	rVB	77143	104129	1.57%	0.141%
2	3.669	112	116	134	rBV	1036174	1552071	23.33%	2.097%
3	3.999	169	172	180	rVB	27767	36191	0.54%	0.049%
4	6.975	669	678	686	rBV	1087268	1740723	26.17%	2.352%
5	7.134	698	705	718	rBV	912360	1457877	21.92%	1.970%
6	7.340	733	740	756	rBV	1124084	1793238	26.96%	2.423%
7	7.810	812	820	829	rBV	1054306	1717962	25.83%	2.321%
8	8.510	930	939	952	rBV	1365752	2165423	32.56%	2.926%
9	8.963	1008	1016	1025	rBV	1046343	1753633	26.36%	2.369%
10	9.681	1131	1138	1150	rBV	845835	1400587	21.06%	1.892%
11	10.222	1223	1230	1240	rBV	1304828	2192433	32.96%	2.962%
12	10.604	1284	1295	1304	rBV	1493709	2559429	38.48%	3.458%
13	10.733	1309	1317	1330	rBV	1349277	2322830	34.92%	3.139%
14	11.392	1424	1429	1434	rBV7	4060	8373	0.13%	0.011%
15	12.192	1559	1565	1571	rBV3	20129	35810	0.54%	0.048%
16	13.851	1840	1847	1854	rBV	2625512	3562203	53.55%	4.813%
17	14.133	1888	1895	1906	rBV	2836599	4154005	62.45%	5.613%
18	14.439	1940	1947	1958	rBV	2445020	3603016	54.17%	4.868%
19	14.633	1973	1980	1989	rBV	1129156	1721364	25.88%	2.326%
20	14.798	2007	2008	2014	rVB6	5313	6857	0.10%	0.009%
21	14.851	2014	2017	2023	rVB8	5630	9869	0.15%	0.013%
22	15.433	2109	2116	2123	rBV	3587540	5170484	77.73%	6.986%
23	15.545	2128	2135	2143	rBV	1144216	1525260	22.93%	2.061%
24	15.674	2152	2157	2162	rVB3	16570	27509	0.41%	0.037%
25	16.215	2244	2249	2252	rVB6	9735	12104	0.18%	0.016%
26	16.827	2350	2353	2356	rBV5	6720	9288	0.14%	0.013%
27	16.857	2356	2358	2364	rVB7	7254	12839	0.19%	0.017%
28	16.962	2372	2376	2381	rBV	7286	10531	0.16%	0.014%
29	17.180	2406	2413	2421	rBV	3117897	4297995	64.62%	5.807%
30	17.280	2423	2430	2443	rVV	3894060	5729159	86.13%	7.741%
31	17.845	2525	2526	2532	rVB6	7790	8193	0.12%	0.011%
32	18.074	2562	2565	2567	rBV4	6794	8107	0.12%	0.011%
33	19.133	2740	2745	2749	rBV3	50153	73157	1.10%	0.099%
34	19.203	2753	2757	2762	rVB	42868	57266	0.86%	0.077%
35	19.503	2805	2808	2811	rBV3	18037	21069	0.32%	0.028%
36	19.568	2812	2819	2825	rBV	4912891	6651576	100.00%	8.987%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
Data File : BM047778.D
Acq On : 02 Oct 2024 15:59
Operator : RC/JU
Sample : PB163608BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK608

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	21.403	3125	3131	3140	rBV	3104312	4639380	69.75%	6.269%
38	24.209	3599	3608	3620	rVB2	2624468	6617127	99.48%	8.941%
39	24.415	3634	3643	3660	rVB	1943729	5241130	78.80%	7.082%




Sum of corrected areas: 74010197

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
Data File : BM047778.D
Acq On : 02 Oct 2024 15:59
Operator : RC/JU
Sample : PB163608BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK608

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

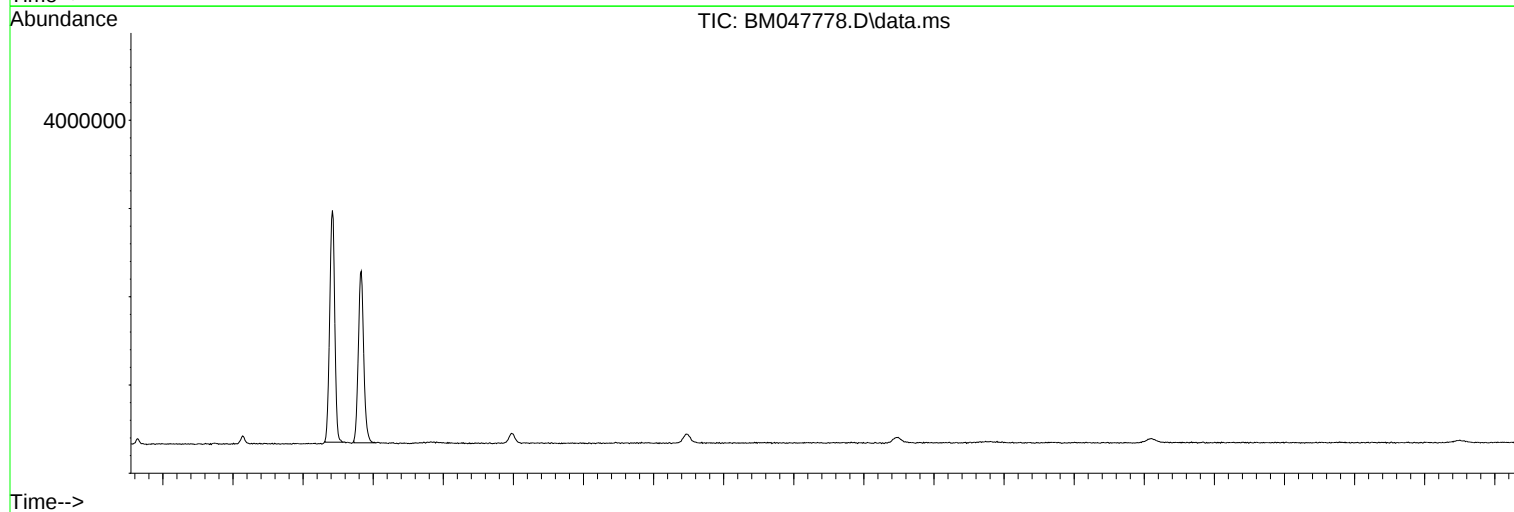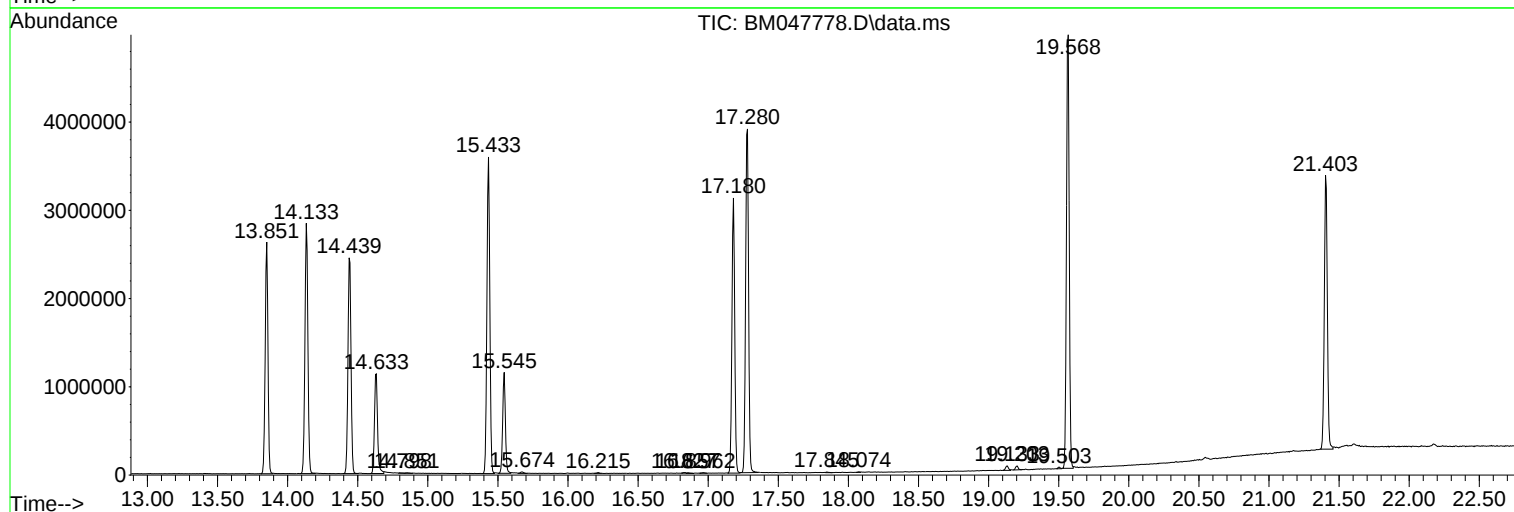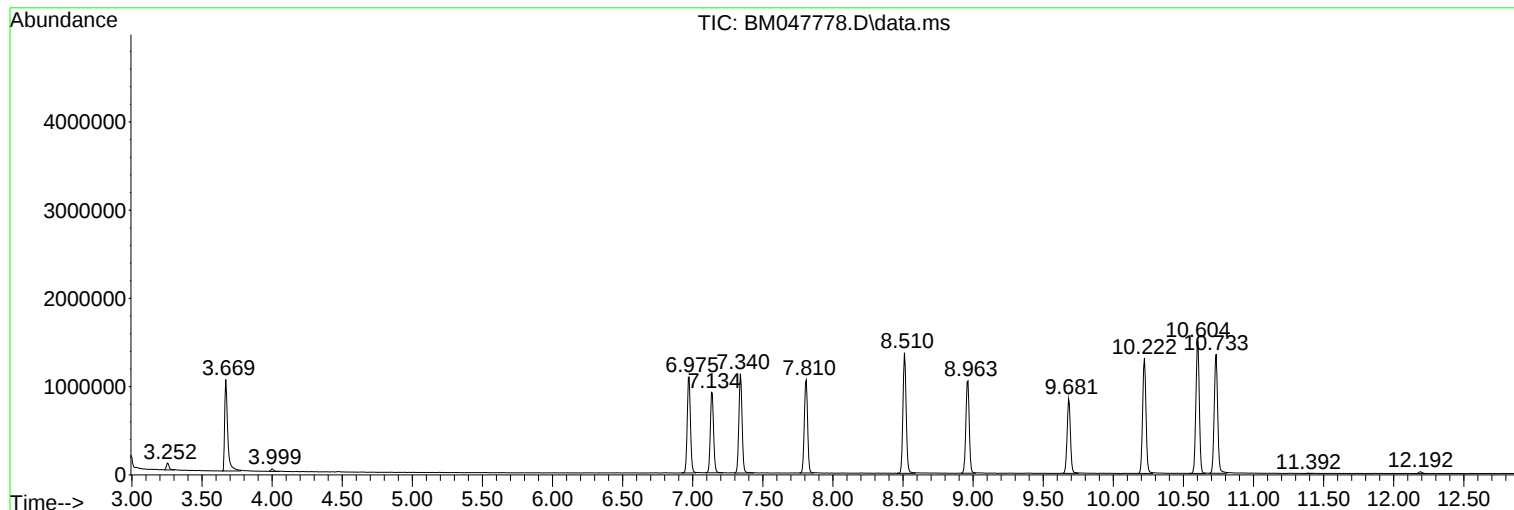

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
Data File : BM047778.D
Acq On : 02 Oct 2024 15:59
Operator : RC/JU
Sample : PB163608BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK608

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
Data File : BM047778.D
Acq On : 02 Oct 2024 15:59
Operator : RC/JU
Sample : PB163608BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK608

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc