

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
 Data File : BM047779.D
 Acq On : 02 Oct 2024 16:38
 Operator : RC/JU
 Sample : P4018-07DL2 30X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCB3DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047779.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.693	117	120	125	rBV3	13426	20181	0.37%	0.086%
2	3.998	169	172	179	rVB	24335	31219	0.58%	0.133%
3	5.834	480	484	490	rVB2	11371	16977	0.32%	0.073%
4	6.375	571	576	579	rBV5	5971	9863	0.18%	0.042%
5	6.451	586	589	597	rBV8	4635	10290	0.19%	0.044%
6	6.769	640	643	647	rBV6	3630	5660	0.11%	0.024%
7	6.804	647	649	656	rVV8	6070	11938	0.22%	0.051%
8	6.863	656	659	663	rVV6	7380	11352	0.21%	0.049%
9	6.916	665	668	671	rVV5	4109	5809	0.11%	0.025%
10	6.975	671	678	683	rVV3	26652	52377	0.97%	0.224%
11	7.034	685	688	693	rVB6	4784	8298	0.15%	0.035%
12	7.139	701	706	712	rBV2	16763	26208	0.49%	0.112%
13	7.339	735	740	748	rVB3	19779	32777	0.61%	0.140%
14	7.439	751	757	764	rBV4	31784	58546	1.09%	0.250%
15	7.810	813	820	827	rBV	739473	1206344	22.40%	5.158%
16	7.875	827	831	832	rBV4	6162	5827	0.11%	0.025%
17	8.004	848	853	856	rVB7	4160	6121	0.11%	0.026%
18	8.404	916	921	925	rVB5	5206	7778	0.14%	0.033%
19	8.475	929	933	936	rVV5	5886	11067	0.21%	0.047%
20	8.510	936	939	945	rVB5	17204	28037	0.52%	0.120%
21	8.580	947	951	954	rBV5	5724	8098	0.15%	0.035%
22	8.957	1011	1015	1023	rBV3	14238	24911	0.46%	0.107%
23	9.039	1023	1029	1035	rVB	28868	45573	0.85%	0.195%
24	9.169	1049	1051	1056	rVB5	4823	5679	0.11%	0.024%
25	9.686	1133	1139	1144	rBV5	12112	22393	0.42%	0.096%
26	9.745	1144	1149	1152	rVV5	4221	6923	0.13%	0.030%
27	9.892	1166	1174	1177	rBV7	5253	13729	0.25%	0.059%
28	9.957	1182	1185	1188	rBV3	3524	5389	0.10%	0.023%
29	10.222	1226	1230	1237	rBV4	16438	27375	0.51%	0.117%
30	10.598	1285	1294	1304	rBV	1023516	1769195	32.86%	7.564%
31	10.733	1309	1317	1323	rBV4	21053	46071	0.86%	0.197%
32	10.986	1352	1360	1365	rBV10	6199	11598	0.22%	0.050%
33	11.116	1380	1382	1389	rVB4	3753	7567	0.14%	0.032%
34	11.292	1407	1412	1414	rBV6	5029	6686	0.12%	0.029%
35	11.480	1441	1444	1449	rBV6	3554	6822	0.13%	0.029%
36	11.627	1466	1469	1474	rBV6	5324	11620	0.22%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
 Data File : BM047779.D
 Acq On : 02 Oct 2024 16:38
 Operator : RC/JU
 Sample : P4018-07DL2 30X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCB3DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

37	11.704	1477	1482	1489	rVB4	23047	39357	0.73%	0.168%
38	11.874	1503	1511	1517	rBV9	7973	15559	0.29%	0.067%
39	12.033	1532	1538	1541	rBV3	14984	24340	0.45%	0.104%
40	12.063	1541	1543	1549	rVB5	5597	8220	0.15%	0.035%
41	12.127	1549	1554	1557	rBV7	6246	9820	0.18%	0.042%
42	12.268	1574	1578	1582	rVB6	4335	6007	0.11%	0.026%
43	12.439	1602	1607	1611	rBV8	6917	12540	0.23%	0.054%
44	12.674	1642	1647	1652	rBV7	8753	16063	0.30%	0.069%
45	12.986	1697	1700	1705	rVB7	5667	7288	0.14%	0.031%
46	13.274	1743	1749	1757	rBV3	15345	26256	0.49%	0.112%
47	13.627	1801	1809	1810	rBV7	4682	9839	0.18%	0.042%
48	13.768	1827	1833	1835	rBV6	6301	12263	0.23%	0.052%
49	13.851	1842	1847	1854	rVV	42694	62907	1.17%	0.269%
50	13.933	1858	1861	1865	rVB5	7024	8459	0.16%	0.036%
51	14.080	1883	1886	1889	rVB4	6442	8423	0.16%	0.036%
52	14.133	1889	1895	1900	rBV2	49596	71804	1.33%	0.307%
53	14.351	1927	1932	1938	rBV	228641	292092	5.42%	1.249%
54	14.439	1940	1947	1954	rBV	1585229	2367771	43.97%	10.124%
55	14.521	1959	1961	1966	rVV5	10113	16792	0.31%	0.072%
56	14.586	1966	1972	1977	rVV	42085	60692	1.13%	0.259%
57	14.657	1979	1984	1988	rVV8	10205	18718	0.35%	0.080%
58	14.692	1988	1990	1995	rVB4	5105	6252	0.12%	0.027%
59	14.980	2034	2039	2040	rBV4	7338	10895	0.20%	0.047%
60	15.004	2040	2043	2046	rVV5	6928	11036	0.20%	0.047%
61	15.062	2046	2053	2062	rVV	294788	433969	8.06%	1.855%
62	15.133	2062	2065	2070	rVV6	9049	15851	0.29%	0.068%
63	15.204	2071	2077	2082	rVV2	31248	53877	1.00%	0.230%
64	15.251	2082	2085	2087	rVV3	13196	20816	0.39%	0.089%
65	15.298	2090	2093	2098	rVB2	27188	34806	0.65%	0.149%
66	15.433	2110	2116	2121	rVB2	73080	112991	2.10%	0.483%
67	15.539	2129	2134	2139	rBV3	22833	35041	0.65%	0.150%
68	15.704	2155	2162	2168	rBV8	9766	20339	0.38%	0.087%
69	15.798	2174	2178	2184	rVB4	17087	25752	0.48%	0.110%
70	15.915	2194	2198	2202	rVB6	5285	9487	0.18%	0.041%
71	16.074	2219	2225	2228	rBV9	7598	12496	0.23%	0.053%
72	16.156	2235	2239	2242	rBV2	24728	34776	0.65%	0.149%
73	16.256	2251	2256	2262	rVB8	5189	8920	0.17%	0.038%
74	16.356	2269	2273	2274	rBV4	4046	5667	0.11%	0.024%
75	16.504	2292	2298	2299	rBV6	7751	9430	0.18%	0.040%
76	16.686	2327	2329	2332	rVB3	9217	8655	0.16%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
 Data File : BM047779.D
 Acq On : 02 Oct 2024 16:38
 Operator : RC/JU
 Sample : P4018-07DL2 30X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCB3DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

77	16.833	2347	2354	2369	rBV	3822386	5384429	100.00%	23.022%
78	16.951	2370	2374	2380	rVV6	30038	61707	1.15%	0.264%
79	17.003	2380	2383	2388	rVB6	12344	18714	0.35%	0.080%
80	17.180	2407	2413	2423	rBV	2035535	2922008	54.27%	12.493%
81	17.274	2425	2429	2434	rVV2	80733	116687	2.17%	0.499%
82	17.321	2435	2437	2441	rVB5	11047	12341	0.23%	0.053%
83	17.468	2458	2462	2464	rBV4	7675	10847	0.20%	0.046%
84	17.680	2496	2498	2505	rVB4	17531	24515	0.46%	0.105%
85	17.756	2507	2511	2515	rVV4	23290	29886	0.56%	0.128%
86	17.798	2515	2518	2520	rVV4	9050	7582	0.14%	0.032%
87	18.068	2561	2564	2569	rBV7	7442	11978	0.22%	0.051%
88	18.374	2613	2616	2619	rBV4	11547	16158	0.30%	0.069%
89	18.697	2667	2671	2673	rBV4	13036	18165	0.34%	0.078%
90	19.497	2804	2807	2812	rVB3	26788	31962	0.59%	0.137%
91	19.562	2814	2818	2825	rVV	91591	134076	2.49%	0.573%
92	20.191	2921	2925	2929	rVB5	35670	51426	0.96%	0.220%
93	21.403	3125	3131	3137	rBV	2237798	3256252	60.48%	13.922%
94	24.409	3634	3642	3659	rVB	1354809	3727347	69.22%	15.937%

Sum of corrected areas: 23388644


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
Data File : BM047779.D
Acq On : 02 Oct 2024 16:38
Operator : RC/JU
Sample : P4018-07DL2 30X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCB3DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

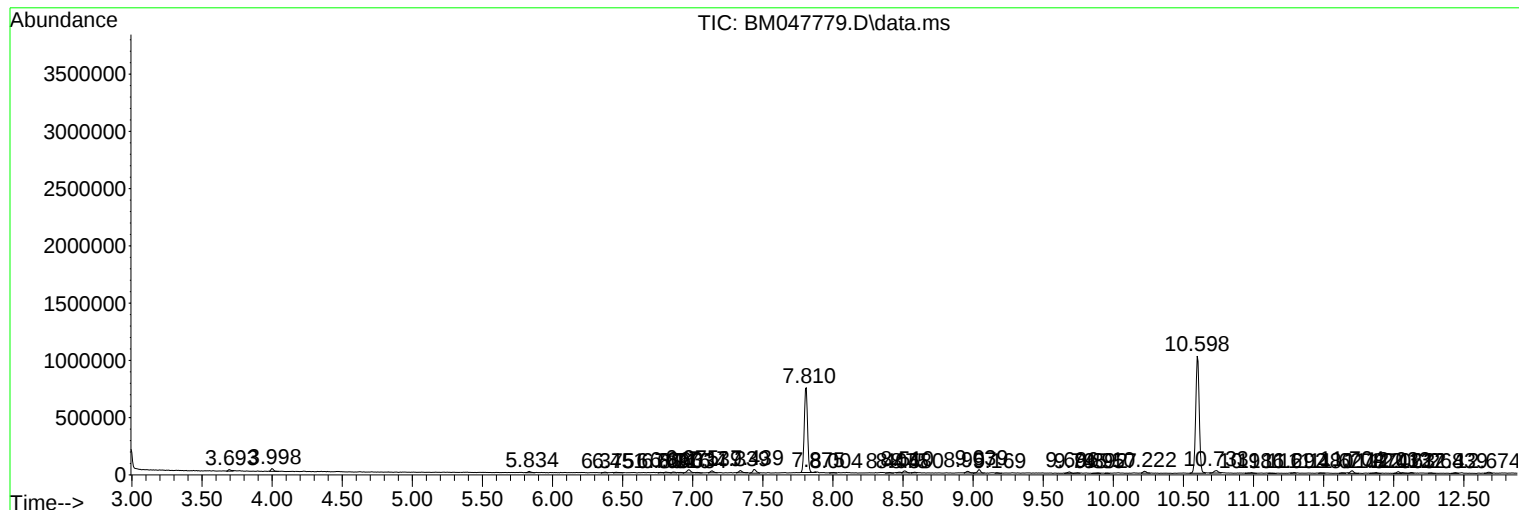

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
Data File : BM047779.D
Acq On : 02 Oct 2024 16:38
Operator : RC/JU
Sample : P4018-07DL2 30X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCB3DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION










TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

Peak Number 1 Oxalic acid, 2-ethylhexyl o... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.351	2.47 ng/ul	292092	Acenaphthene-d10	14.439

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Oxalic acid, 2-ethylhexyl octyl ...	314	C18H34O4	1000309-39-1	72
2	Octane, 2,3,6-trimethyl-	156	C11H24	062016-33-5	64
3	Sulfurous acid, 2-ethylhexyl oct...	446	C26H54O3S	1000309-20-1	64
4	Octane, 3,6-dimethyl-	142	C10H22	015869-94-0	64
5	Oxalic acid, decyl 2-ethylhexyl ...	342	C20H38O4	1000309-39-3	64

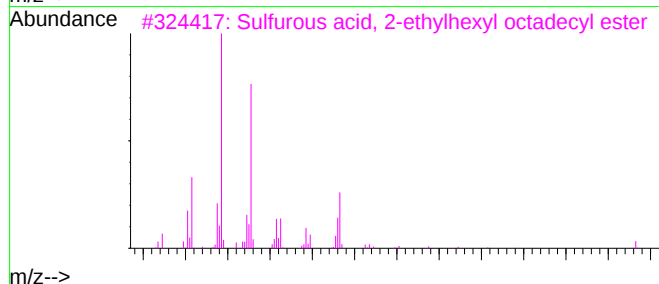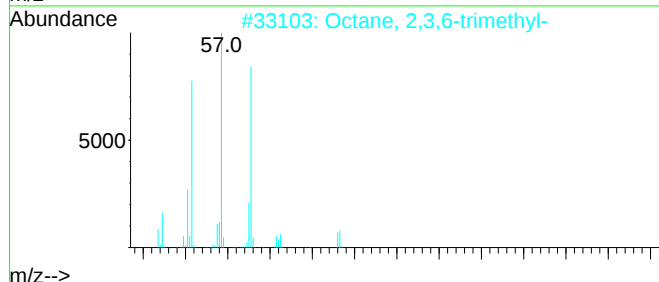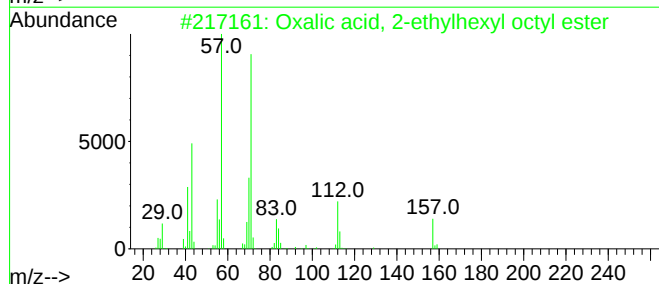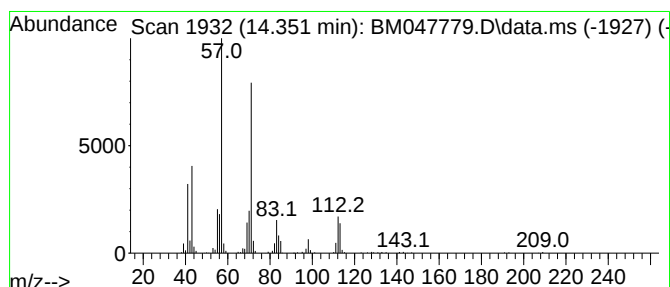

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
Data File : BM047779.D
Acq On : 02 Oct 2024 16:38
Operator : RC/JU
Sample : P4018-07DL2 30X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCB3DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Oxalic acid, 2-...	14.351	2.5	ng/u1	292092	3	14.439	2367770	20.0