

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
 Data File : BM047781.D
 Acq On : 02 Oct 2024 17:57
 Operator : RC/JU
 Sample : P4018-06DL 20X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCB2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047781.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.693	117	120	127	rBV2	13233	24725	0.70%	0.144%
2	3.999	167	172	177	rVV	29328	39451	1.12%	0.230%
3	4.469	248	252	257	rBV4	8038	15049	0.43%	0.088%
4	5.310	394	395	400	rVB3	2746	3604	0.10%	0.021%
5	5.922	496	499	505	rVB5	3272	4631	0.13%	0.027%
6	6.093	524	528	532	rVB6	3291	4681	0.13%	0.027%
7	6.975	672	678	683	rBV3	23099	38271	1.08%	0.223%
8	7.140	699	706	712	rVB	17915	30339	0.86%	0.177%
9	7.340	735	740	745	rBV3	19232	32758	0.93%	0.191%
10	7.440	753	757	765	rBV6	7585	15293	0.43%	0.089%
11	7.804	811	819	827	rBV	663695	1087780	30.82%	6.343%
12	8.398	918	920	925	rBV6	3114	4409	0.12%	0.026%
13	8.481	931	934	936	rBV4	4026	4329	0.12%	0.025%
14	8.516	936	940	947	rVB3	15119	27514	0.78%	0.160%
15	8.963	1010	1016	1020	rBV2	15046	25536	0.72%	0.149%
16	9.045	1025	1030	1035	rVB6	7907	12273	0.35%	0.072%
17	9.398	1086	1090	1091	rBV3	4213	4044	0.11%	0.024%
18	9.686	1135	1139	1147	rVB9	9073	16040	0.45%	0.094%
19	10.222	1224	1230	1237	rBV4	14359	30116	0.85%	0.176%
20	10.598	1285	1294	1306	rBV	861625	1494538	42.35%	8.715%
21	10.739	1312	1318	1325	rBV4	13417	30067	0.85%	0.175%
22	10.981	1354	1359	1361	rBV5	2978	3817	0.11%	0.022%
23	11.698	1475	1481	1486	rVB7	5381	9101	0.26%	0.053%
24	11.863	1506	1509	1516	rBV7	4665	11747	0.33%	0.069%
25	12.669	1642	1646	1648	rBV4	2991	4120	0.12%	0.024%
26	13.275	1746	1749	1753	rBV5	4164	7104	0.20%	0.041%
27	13.763	1827	1832	1834	rBV3	3330	4363	0.12%	0.025%
28	13.851	1841	1847	1852	rBV	42232	63008	1.79%	0.367%
29	13.892	1852	1854	1859	rVB4	2736	3929	0.11%	0.023%
30	14.086	1884	1887	1890	rBV4	3061	4717	0.13%	0.028%
31	14.133	1890	1895	1905	rVB	48736	75426	2.14%	0.440%
32	14.351	1926	1932	1936	rBV2	49190	63776	1.81%	0.372%
33	14.439	1939	1947	1958	rVV	1359299	1964998	55.68%	11.459%
34	14.580	1966	1971	1976	rBV2	8902	13309	0.38%	0.078%
35	14.857	2015	2018	2021	rBV4	2954	4579	0.13%	0.027%
36	15.069	2048	2054	2062	rVB5	23541	37672	1.07%	0.220%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
 Data File : BM047781.D
 Acq On : 02 Oct 2024 17:57
 Operator : RC/JU
 Sample : P4018-06DL 20X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCB2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

37	15.198	2072	2076	2079	rBV4	6477	9338	0.26%	0.054%
38	15.251	2079	2085	2091	rVV2	16015	31824	0.90%	0.186%
39	15.298	2091	2093	2097	rVB3	6401	7962	0.23%	0.046%
40	15.433	2109	2116	2122	rVB2	67944	107320	3.04%	0.626%
41	15.539	2131	2134	2139	rBV5	8536	12398	0.35%	0.072%
42	15.798	2172	2178	2182	rVB3	9831	16443	0.47%	0.096%
43	16.157	2234	2239	2241	rBV6	7633	9069	0.26%	0.053%
44	16.686	2324	2329	2333	rBV6	9135	14732	0.42%	0.086%
45	16.727	2333	2336	2341	rVB7	3359	5297	0.15%	0.031%
46	16.827	2347	2353	2366	rBV	2531727	3529292	100.00%	20.581%
47	17.180	2406	2413	2423	rBV	1734989	2362516	66.94%	13.777%
48	17.274	2424	2429	2435	rVB	69634	104115	2.95%	0.607%
49	17.757	2508	2511	2514	rVB4	8905	10254	0.29%	0.060%
50	17.798	2514	2518	2521	rVB6	6931	6985	0.20%	0.041%
51	18.145	2574	2577	2579	rVB4	3950	4060	0.12%	0.024%
52	18.698	2669	2671	2674	rVB3	13953	11746	0.33%	0.068%
53	19.498	2803	2807	2812	rVB3	24229	30025	0.85%	0.175%
54	19.562	2814	2818	2824	rBV	84212	120792	3.42%	0.704%
55	20.186	2921	2924	2929	rBV3	37520	51170	1.45%	0.298%
56	20.815	3028	3031	3035	rVB	64664	75514	2.14%	0.440%
57	21.403	3125	3131	3137	rBV	1721835	2601378	73.71%	15.170%
58	24.409	3634	3642	3655	rVB	1159836	2809100	79.59%	16.381%




Sum of corrected areas: 17148444

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
Data File : BM047781.D
Acq On : 02 Oct 2024 17:57
Operator : RC/JU
Sample : P4018-06DL 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCB2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

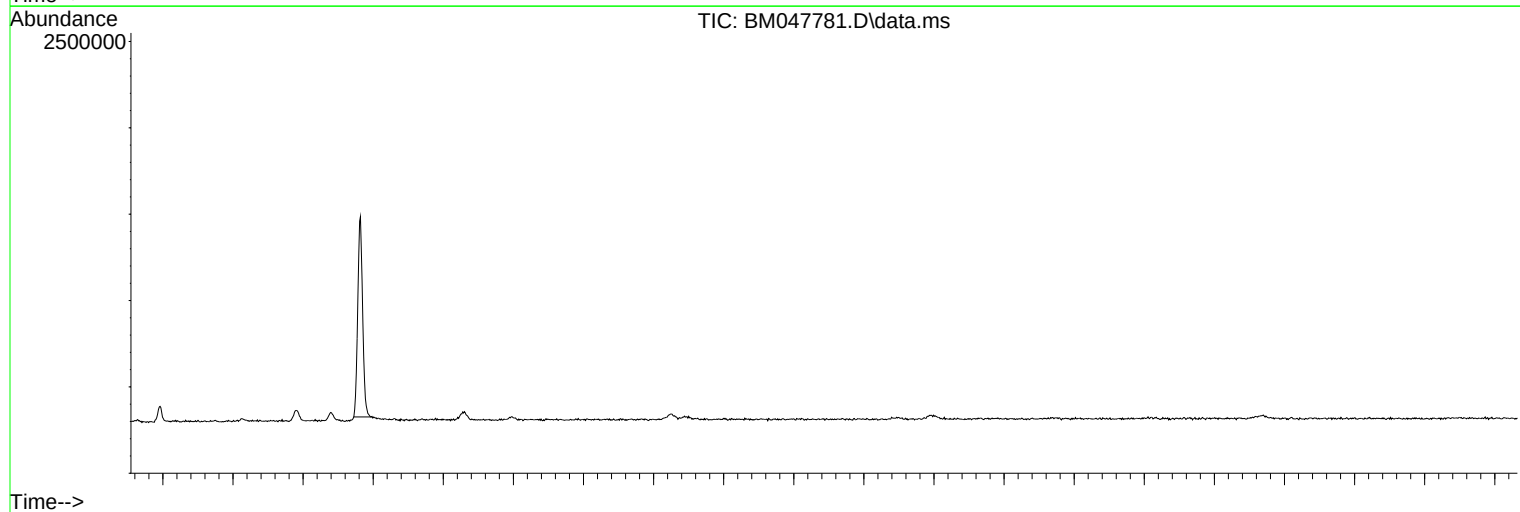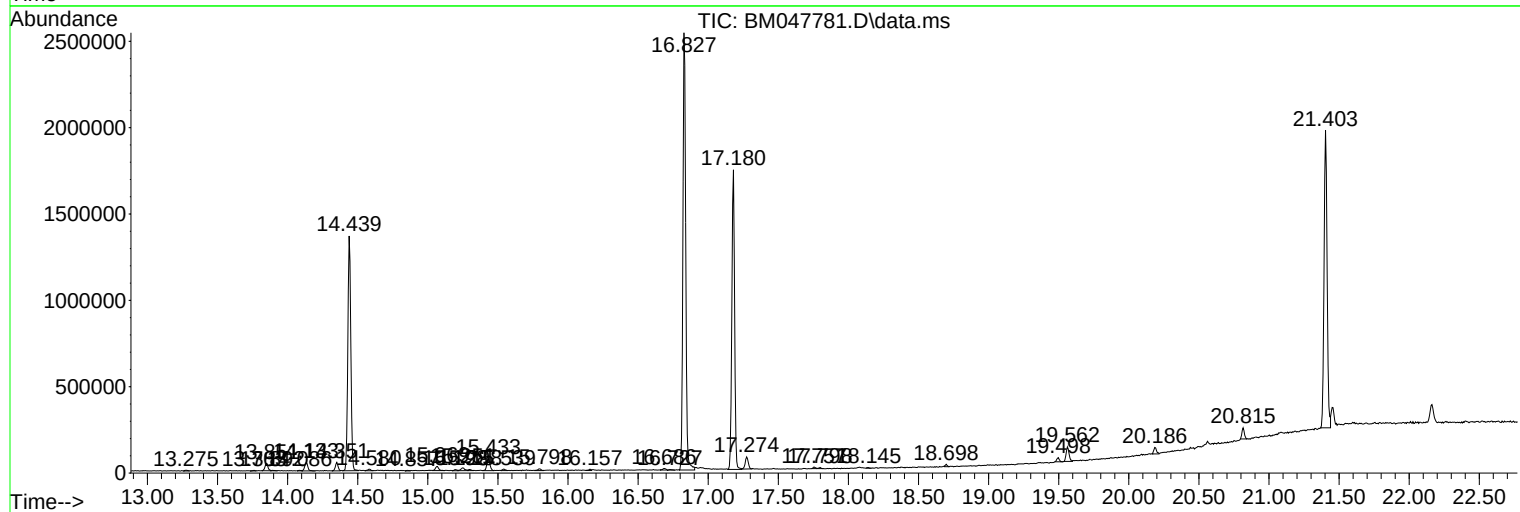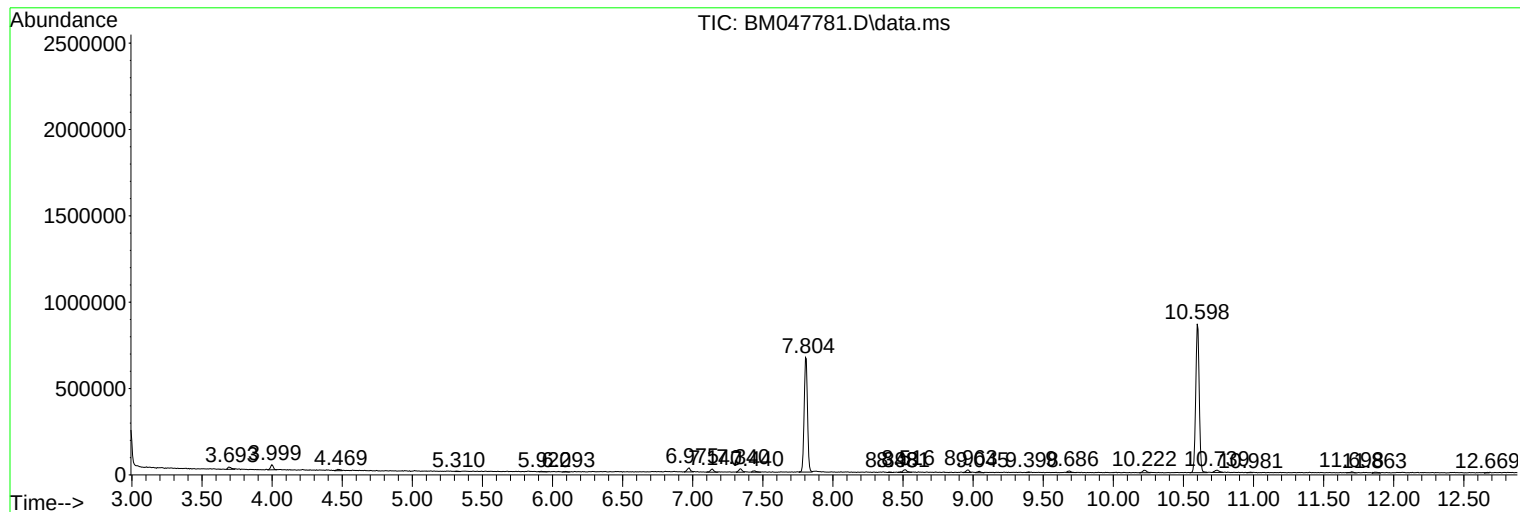

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
Data File : BM047781.D
Acq On : 02 Oct 2024 17:57
Operator : RC/JU
Sample : P4018-06DL 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCB2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100224\
Data File : BM047781.D
Acq On : 02 Oct 2024 17:57
Operator : RC/JU
Sample : P4018-06DL 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCB2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
