

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100317\
 Data File : BM011863.D
 Acq On : 03 Oct 2017 22:32
 Operator : SJ/JU
 Sample : I5525-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 04 03:52:49 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 03 15:47:54 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	189472	20.00	ng/ul	0.00
18) Naphthalene-d8	10.68	136	868601	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.52	164	579271	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.26	188	1439580	20.00	ng/ul	0.00
75) Chrysene-d12	21.43	240	1742517	20.00	ng/ul	0.00
83) Perylene-d12	23.76	264	1928933	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	24617	6.14	ng/uL	0.00
5) Phenol-d5	7.03	99	105563	6.48	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.20	67	275068	28.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.40	132	324537	24.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.57	113	208340	14.78	ng/ul	0.00
19) Nitrobenzene-d5	9.04	128	189341	30.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.76	143	213657	30.67	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.30	165	388648	27.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.85	131	5052	0.33	ng/ul	0.03
43) Dimethylphthalate-d6	13.92	166	1628692	32.44	ng/ul	0.00
46) Acenaphthylene-d8	14.21	160	1777885	30.14	ng/ul	0.00
51) 4-Nitrophenol-d4	14.72	143	26226	2.99	ng/ul	0.00
57) Fluorene-d10	15.51	176	1374689	31.02	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.63	200	250697	25.88	ng/ul	0.00
70) Anthracene-d10	17.36	188	2337497	32.95	ng/ul	0.00
76) Pyrene-d10	19.64	212	2916782	37.11	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.60	264	3018206	32.53	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) 2,6-Dinitrotoluene	13.93	165	11489	1.262	ng/ul#	31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100317\
Data File : BM011863.D
Acq On : 03 Oct 2017 22:32
Operator : SJ/JU
Sample : I5525-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 04 03:52:49 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 03 15:47:54 2017
Response via : Initial Calibration

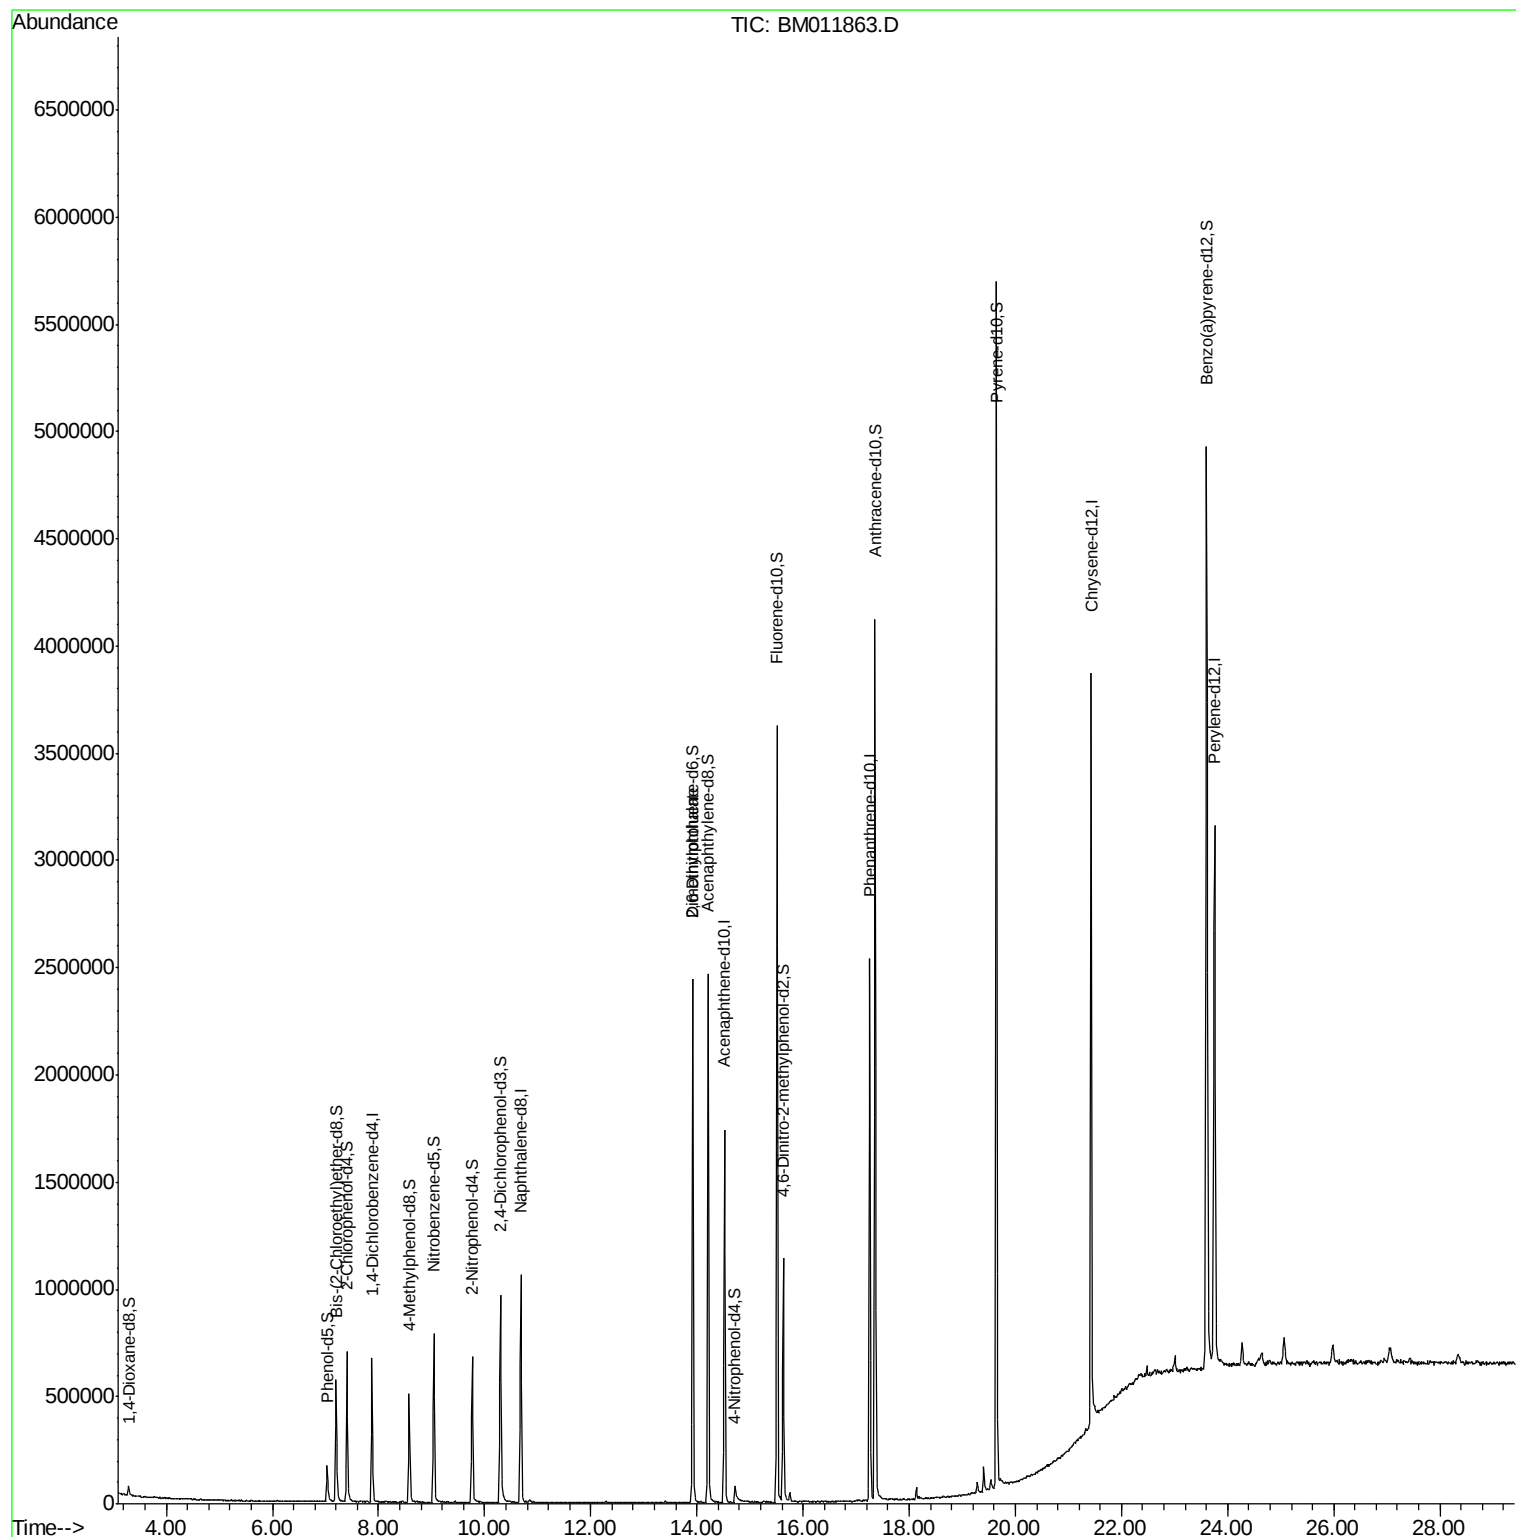

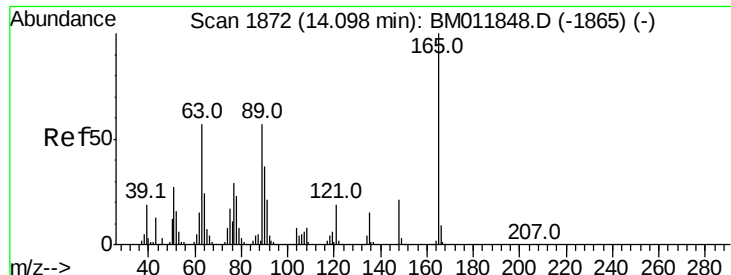

#45

2,6-Dinitrotoluene

Concen: 1.262 ng/ul

RT: 13.93 min Scan# 1843

Delta R.T. -0.17 min

Lab File: BM011863.D

Acq: 03 Oct 2017 22:32

Instrument :

BNA_M

ClientSampleId :


Tot Ion:165 Resp: 11489

Ion Ratio Lower Upper

165 100

89 0.0 52.6 79.0#

121 27.3 14.6 22.0#

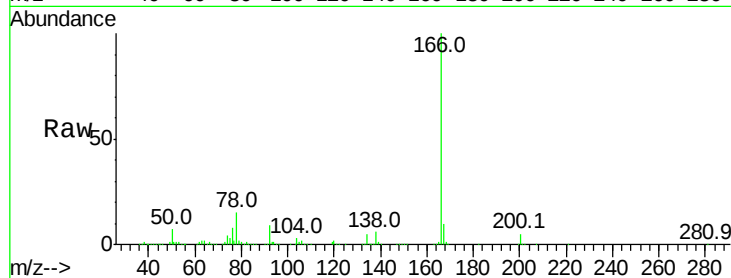

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

