

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100317\
 Data File : BM011872.D
 Acq On : 04 Oct 2017 03:56
 Operator : SJ/JU
 Sample : I5525-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 04 05:50:50 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 04 05:30:09 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	268564	20.00	ng/ul	0.00
18) Naphthalene-d8	10.68	136	1194180	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.52	164	753851	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.26	188	1781458	20.00	ng/ul	0.00
75) Chrysene-d12	21.43	240	1832587	20.00	ng/ul	0.00
83) Perylene-d12	23.75	264	1580124	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	33885	5.97	ng/uL	0.00
5) Phenol-d5	7.03	99	195609	8.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.20	67	479479	35.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.40	132	571393	30.83	ng/ul	0.00
13) 4-Methylphenol-d8	8.57	113	387972	19.42	ng/ul	0.00
19) Nitrobenzene-d5	9.04	128	336639	39.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.76	143	388446	40.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.30	165	699265	36.12	ng/ul	0.00
29) 4-Chloroaniline-d4	10.84	131	10448	0.49	ng/ul	0.02
43) Dimethylphthalate-d6	13.92	166	2700005	41.33	ng/ul	0.00
46) Acenaphthylene-d8	14.21	160	3029812	39.46	ng/ul	0.00
51) 4-Nitrophenol-d4	14.72	143	51021	4.47	ng/ul	0.00
57) Fluorene-d10	15.51	176	2262396	39.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.63	200	420643	35.09	ng/ul	0.00
70) Anthracene-d10	17.36	188	3683153	41.96	ng/ul	0.00
76) Pyrene-d10	19.64	212	4290587	51.91	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.60	264	3167816	41.67	ng/ul	0.00


Target Compounds				Ovalue	
45) 2,6-Dinitrotoluene	13.92	165	17364	1.465 ng/ul#	31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM100317\
Data File : BM011872.D
Acq On : 04 Oct 2017 03:56
Operator : SJ/JU
Sample : I5525-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 04 05:50:50 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM100317.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 04 05:30:09 2017
Response via : Initial Calibration

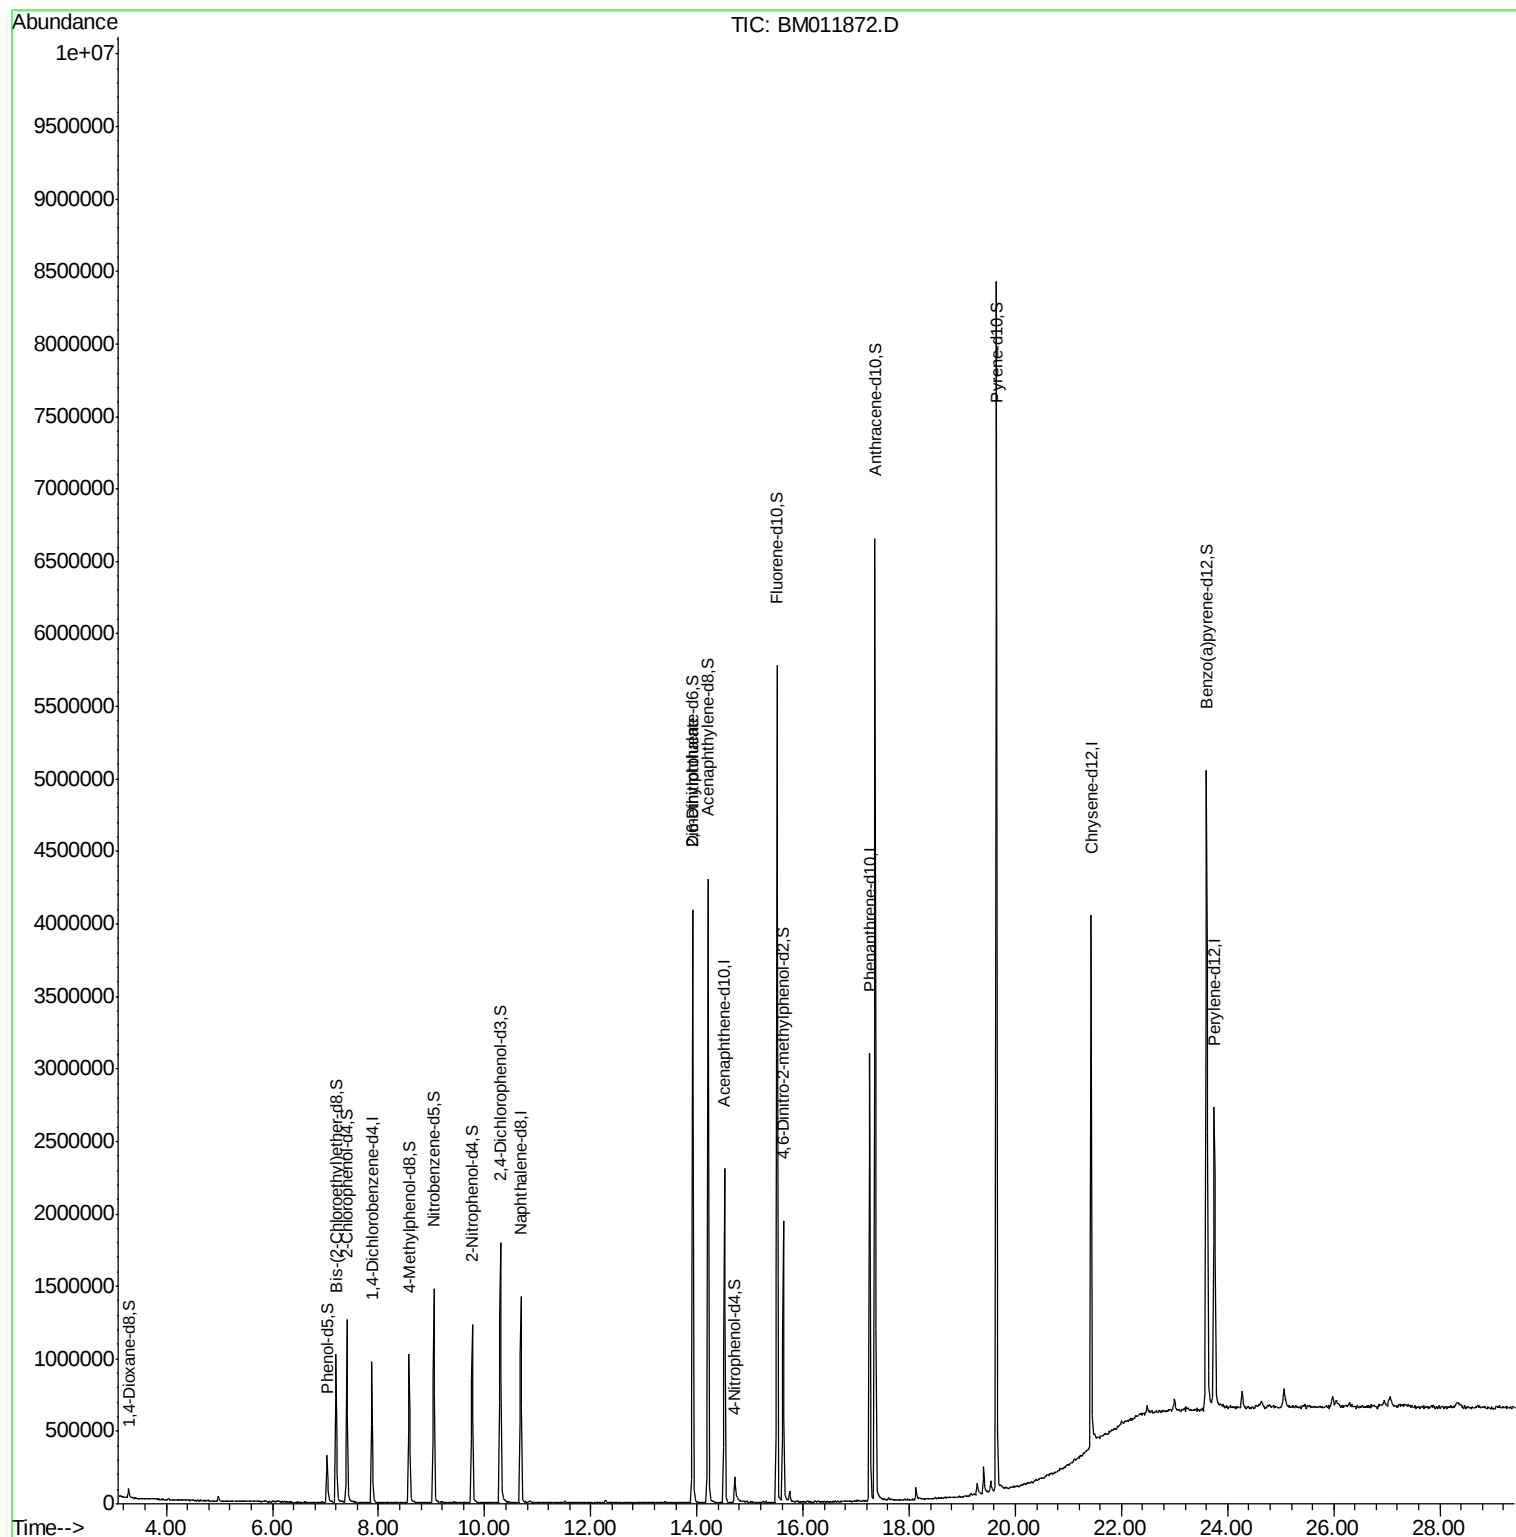

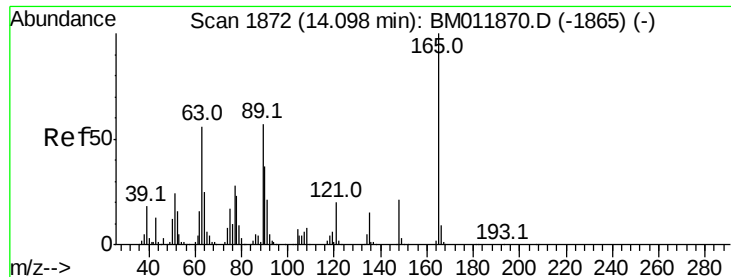

#45

2,6-Dinitrotoluene

Concen: 1.465 ng/ul

RT: 13.92 min Scan# 1842

Delta R.T. -0.18 min

Lab File: BM011872.D

Acq: 04 Oct 2017 03:56

Instrument :

BNA_M

ClientSampleId :


Tot Ion:165 Resp: 17364

Ion Ratio Lower Upper

165 100

89 3.1 52.6 79.0#

121 33.6 14.6 22.0#

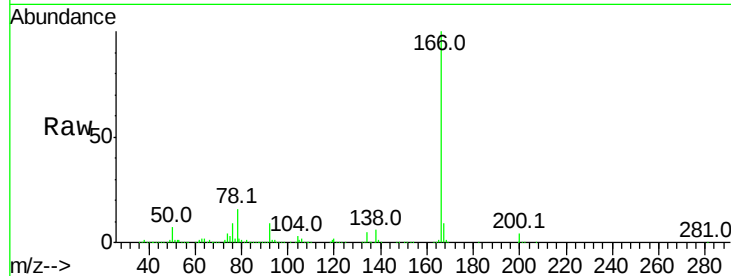

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

